

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101019\
 Data File : P0061856.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2019 14:06
 Operator : HP/AJ
 Sample : K5292-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20190853-COMPOSITE-E

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:10:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 14:20:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 10 11:46:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.513	786997	584440	19.188	18.072
2) SA Decachlor...	10.010	8.372	574030	414042	12.326	12.789m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101019\
Data File : PO061856.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2019 14:06
Operator : HP/AJ
Sample : K5292-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20190853-COMPOSITE-E


Manual Integrations
APPROVED

Ankita
10/11/2019 2:10:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 14:20:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 11:46:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

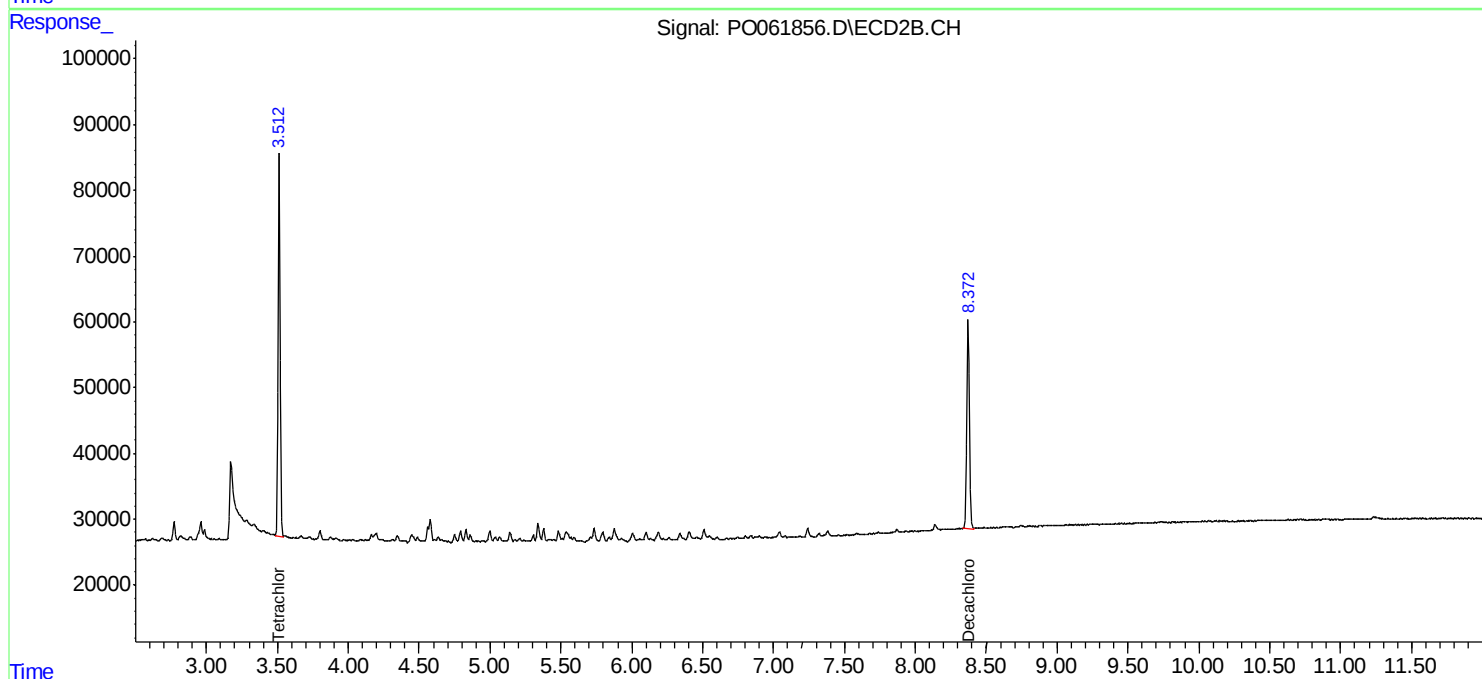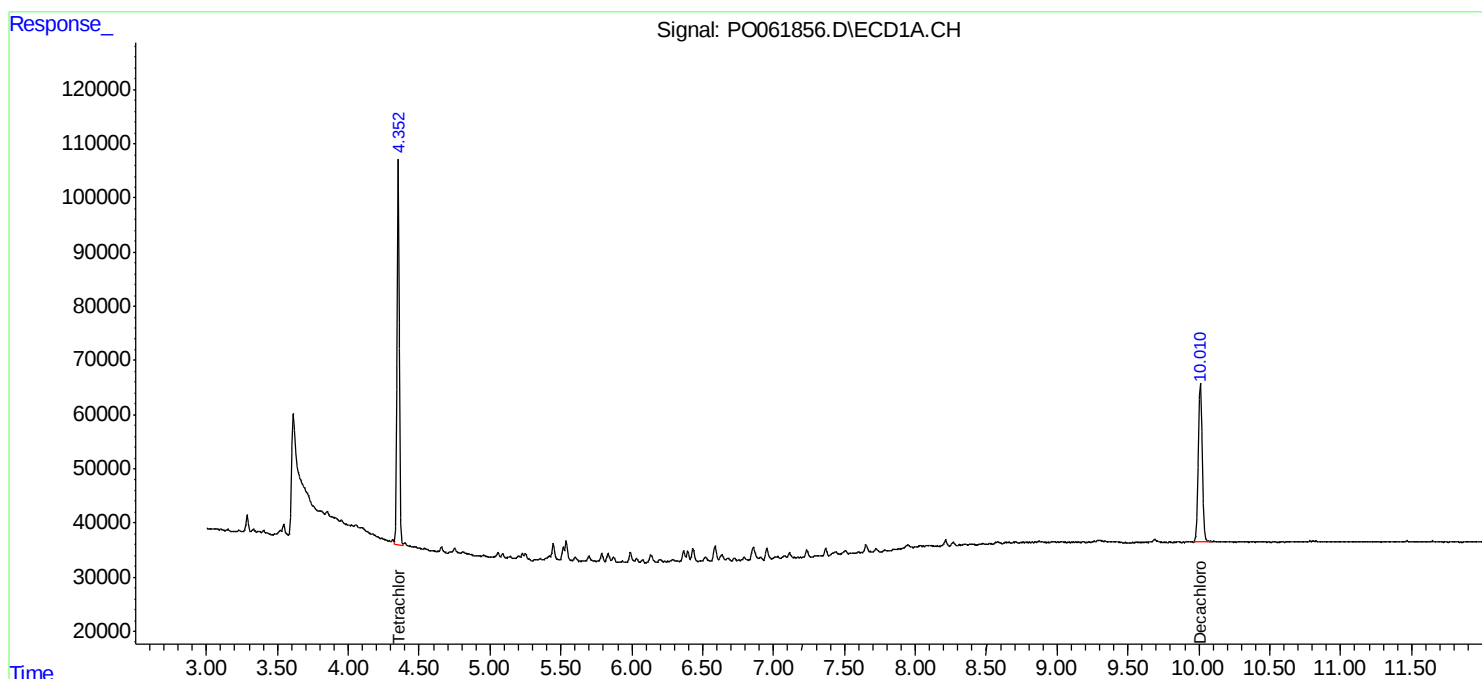

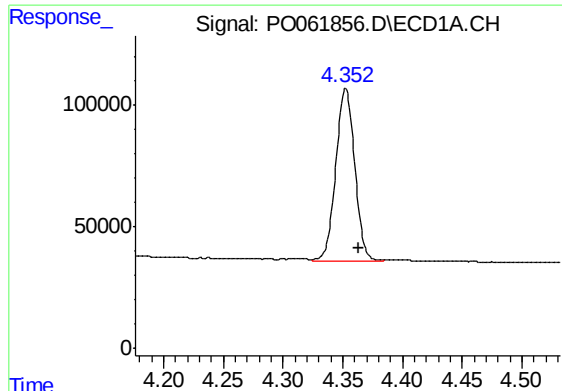


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.011 min
Response: 786997
Conc: 19.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190853-COMPOSITE-E


Manual Integrations
APPROVED

Ankita
10/11/2019 2:10:25 PM

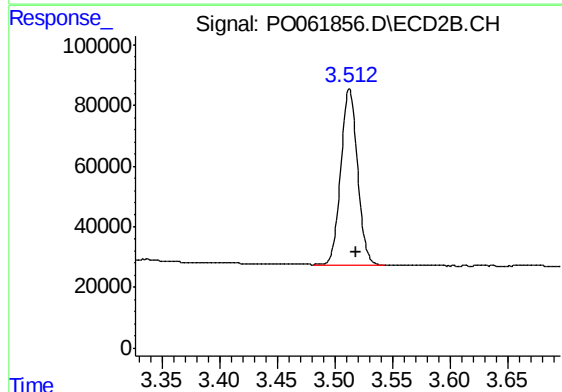


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.006 min
Response: 584440
Conc: 18.07 ng/ml

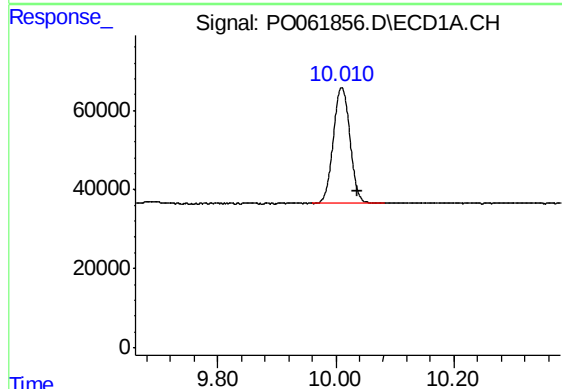

#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.026 min
Response: 574030
Conc: 12.33 ng/ml

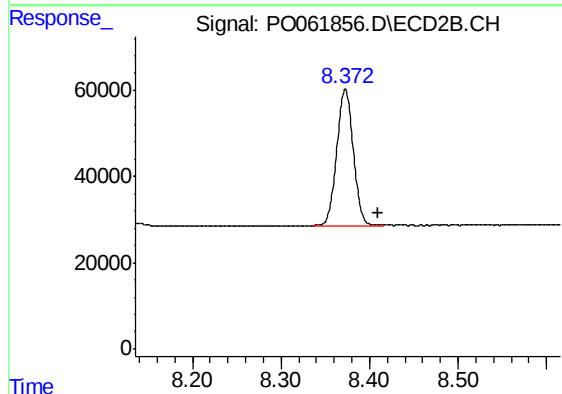

#2 Decachlorobiphenyl

R.T.: 8.372 min
Delta R.T.: -0.037 min
Response: 414042
Conc: 12.79 ng/ml m