

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101019\
 Data File : P0061865.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2019 16:57
 Operator : HP/AJ
 Sample : K5297-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HH-CONCRETE

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:10:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 10 11:46:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.353	3.513	926186	642417	22.582	19.865
2)	SA Decachlor...	10.010	8.372	915320	633013	19.654	19.552m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101019\
Data File : PO061865.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2019 16:57
Operator : HP/AJ
Sample : K5297-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HH-CONCRETE


Manual Integrations
APPROVED

Ankita
10/11/2019 2:10:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 11:46:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

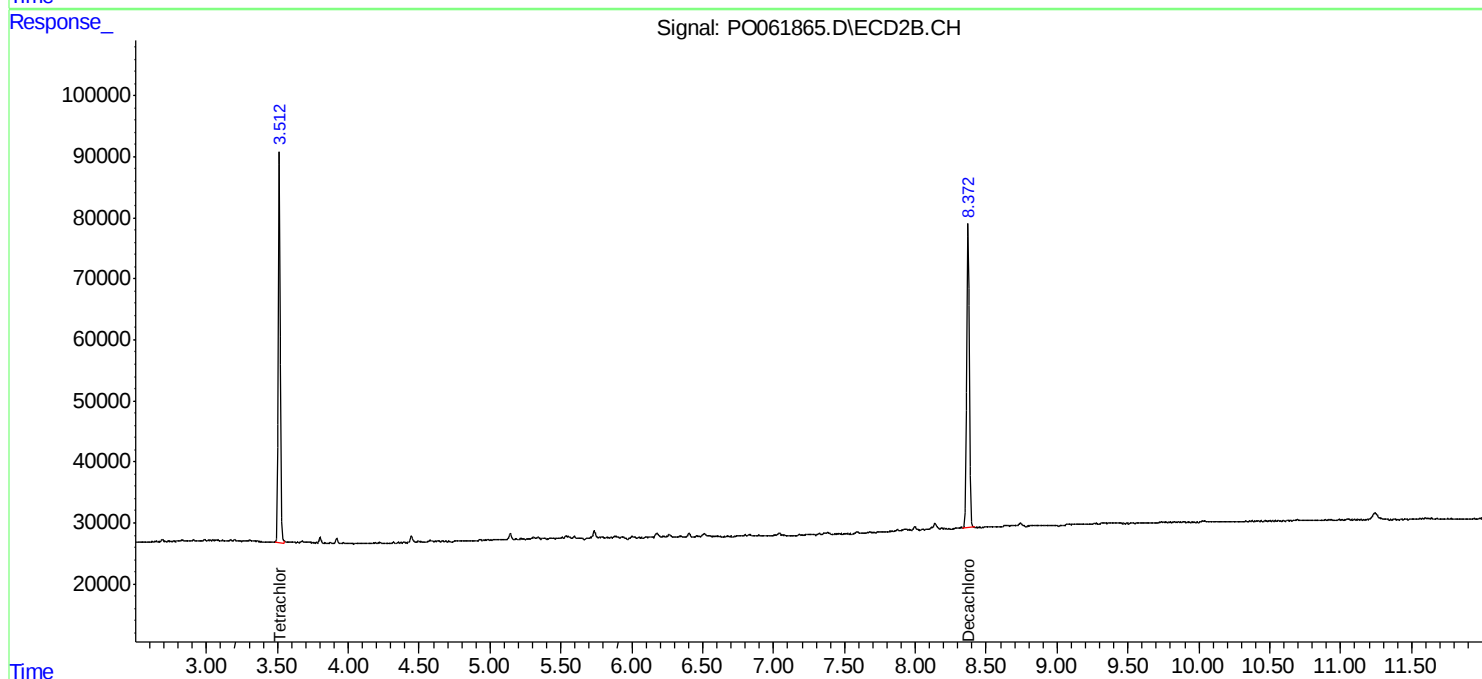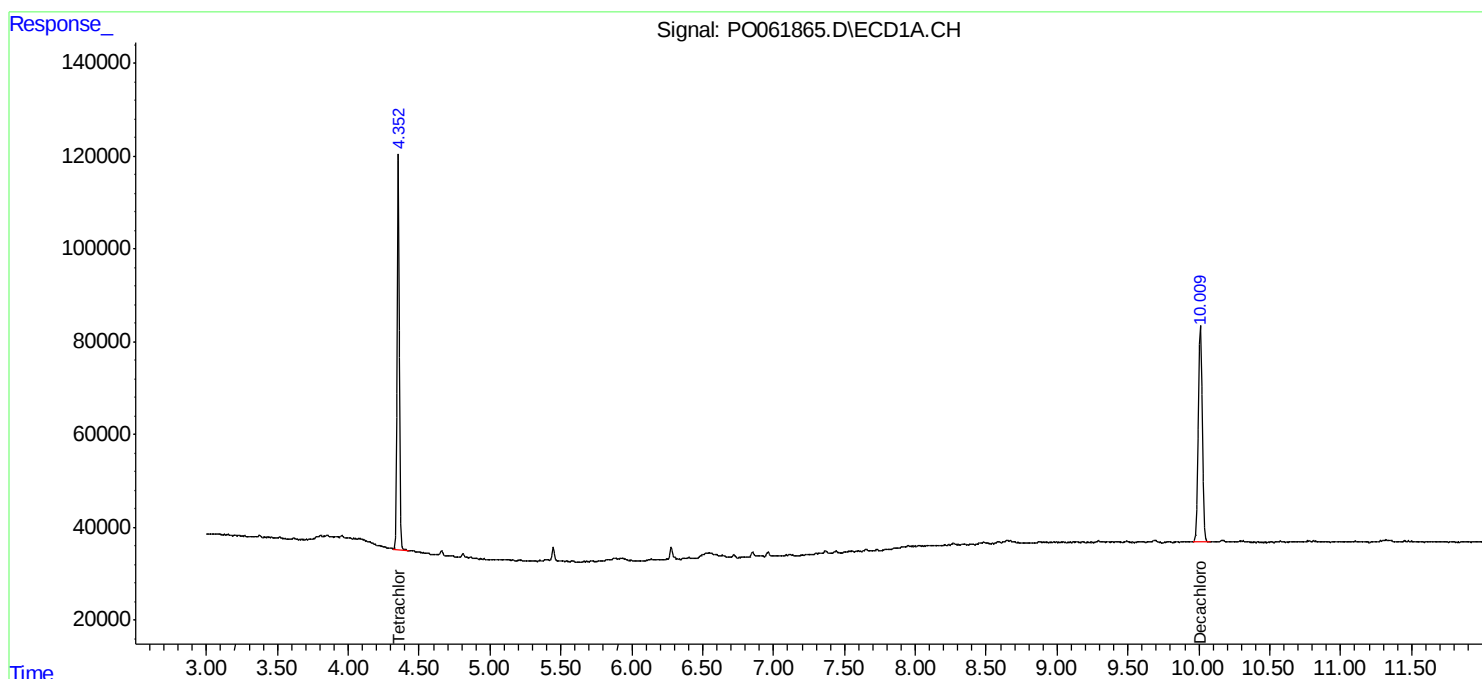

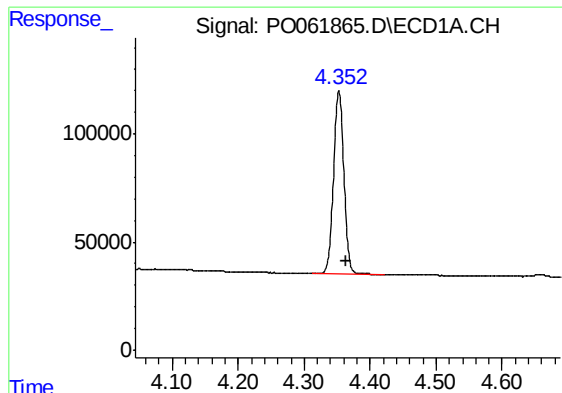


#1 Tetrachloro-m-xylene

R.T.: 4.353 min
Delta R.T.: -0.010 min
Response: 926186
Conc: 22.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
HH-CONCRETE


Manual Integrations
APPROVED

Ankita
10/11/2019 2:10:58 PM

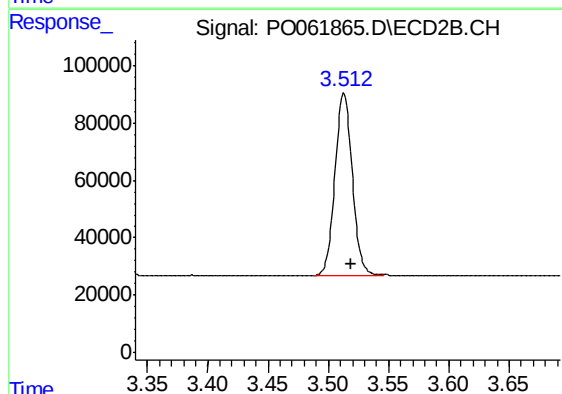


#1 Tetrachloro-m-xylene

R.T.: 3.513 min
Delta R.T.: -0.006 min
Response: 642417
Conc: 19.86 ng/ml

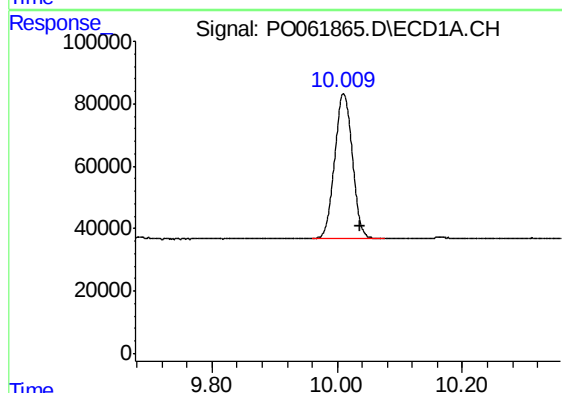

#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.026 min
Response: 915320
Conc: 19.65 ng/ml

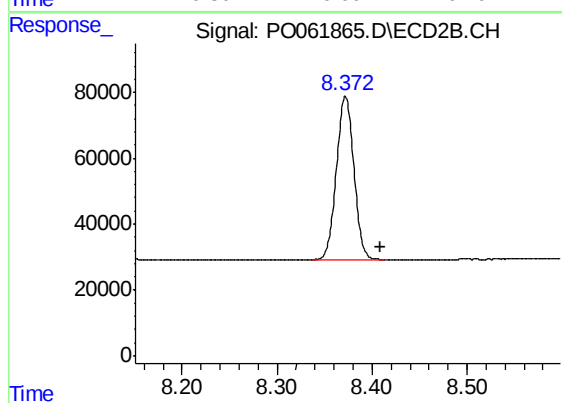

#2 Decachlorobiphenyl

R.T.: 8.372 min
Delta R.T.: -0.037 min
Response: 633013
Conc: 19.55 ng/ml m