

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101019\
 Data File : P0061868.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2019 17:45
 Operator : HP/AJ
 Sample : K5297-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 10/11/2019 2:11:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 03:15:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 10 11:46:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.352	3.512	900240	614016	21.949	18.987m
2)	SA Decachlor...	10.008	8.371	579691	401530	12.447	12.402m
Target Compounds							
26)	L6 AR-1254-1	6.366	5.339	34904	40620	15.300m	18.520m
27)	L6 AR-1254-2	6.583	5.483	139308	30942	38.557m	15.783m#
28)	L6 AR-1254-3	6.957	5.876	115827	39755	29.643	12.487m#
29)	L6 AR-1254-4	7.235	6.100	24595	21036	8.121m	10.368m#
30)	L6 AR-1254-5	7.651	6.508	39324	44733	12.522m	15.815m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101019\
Data File : PO061868.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2019 17:45
Operator : HP/AJ
Sample : K5297-08
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-3


Manual Integrations
APPROVED

Ankita
10/11/2019 2:11:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 03:15:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100119.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 10 11:46:12 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

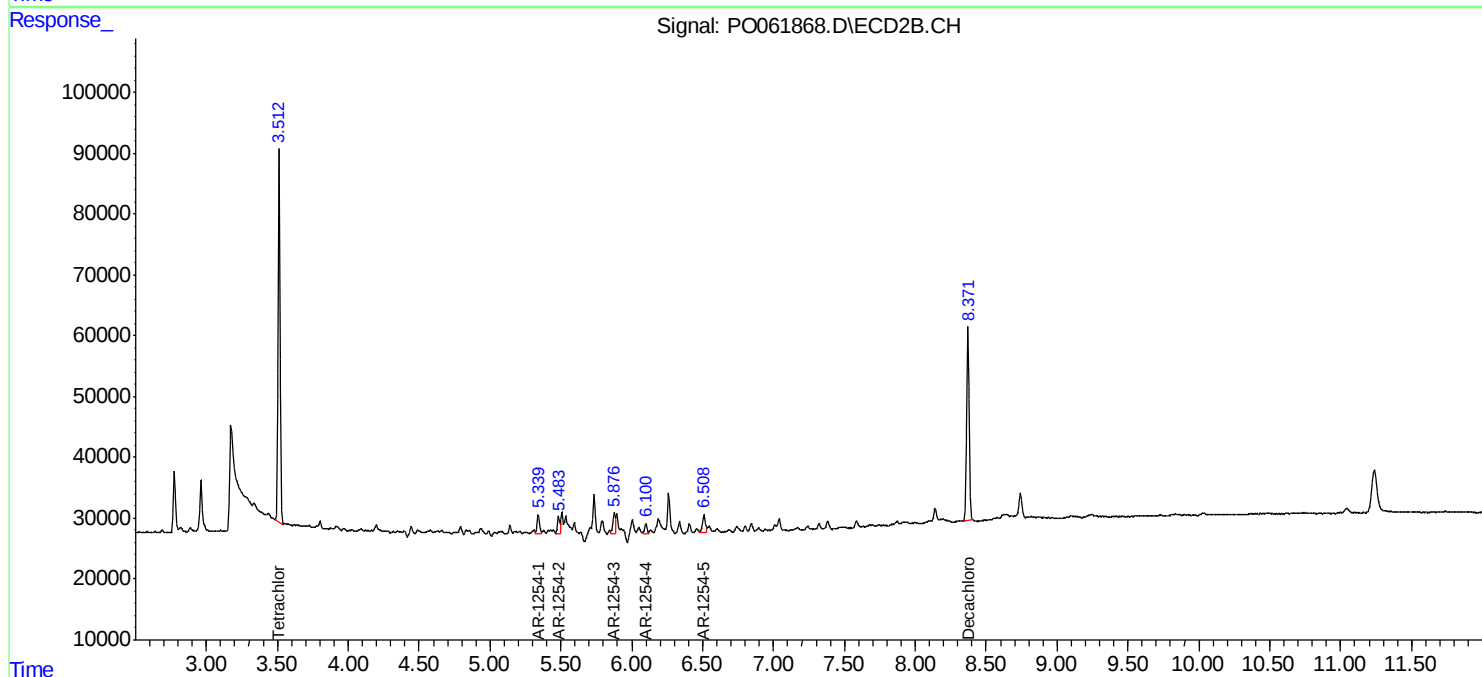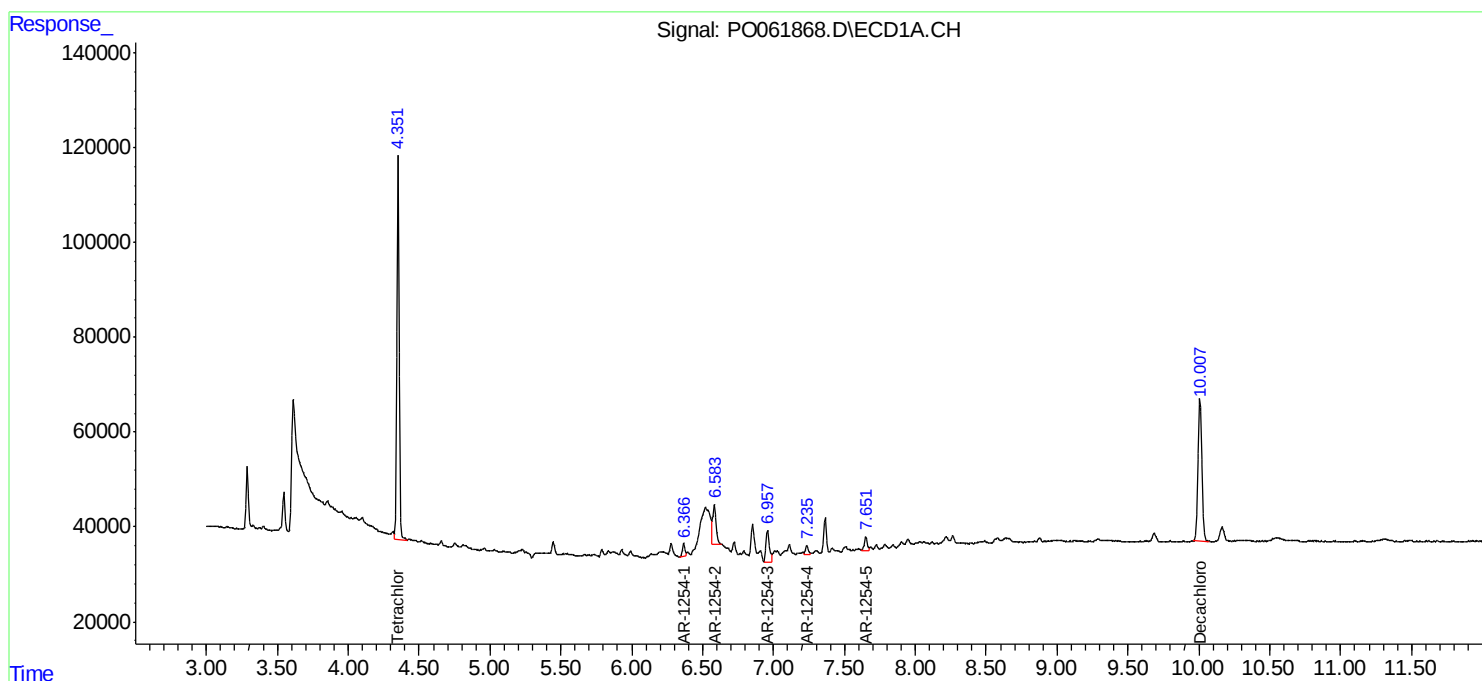

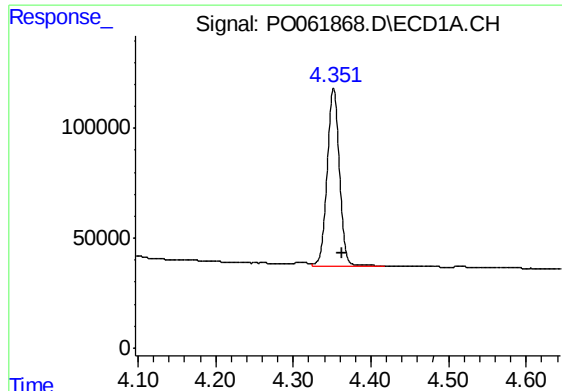


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.011 min
Response: 900240
Conc: 21.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
10/11/2019 2:11:04 PM

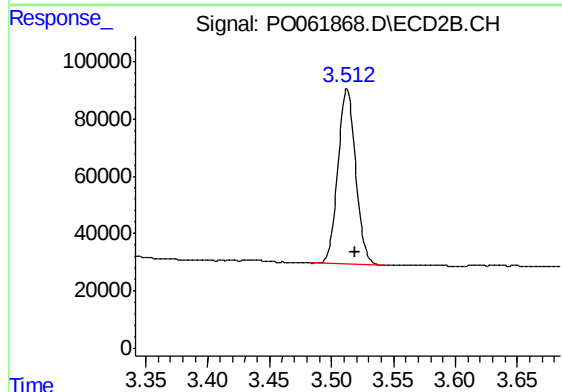


#1 Tetrachloro-m-xylene

R.T.: 3.512 min
Delta R.T.: -0.007 min
Response: 614016
Conc: 18.99 ng/ml m

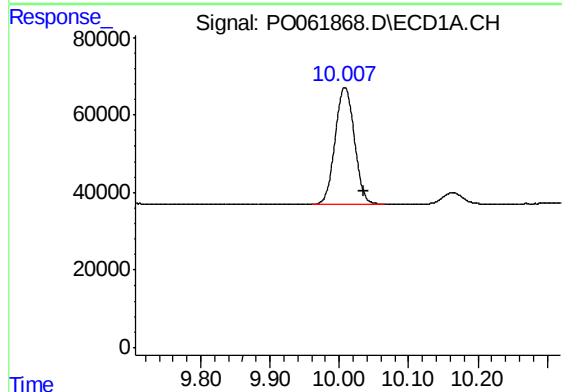


#2 Decachlorobiphenyl

R.T.: 10.008 min
Delta R.T.: -0.028 min
Response: 579691
Conc: 12.45 ng/ml

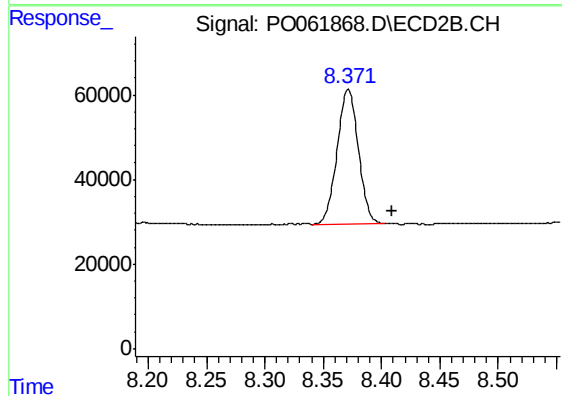

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.038 min
Response: 401530
Conc: 12.40 ng/ml m

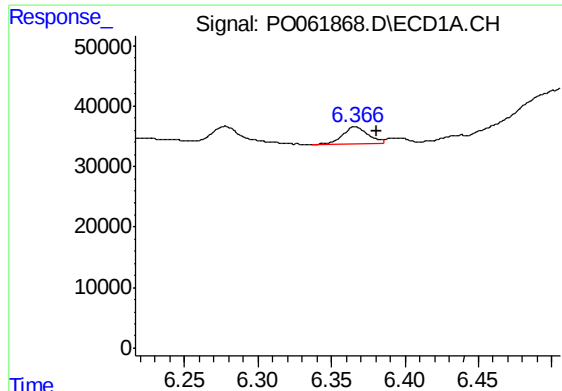


#26 AR-1254-1

R.T.: 6.366 min
Delta R.T.: -0.015 min
Response: 34904
Conc: 15.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
10/11/2019 2:11:04 PM

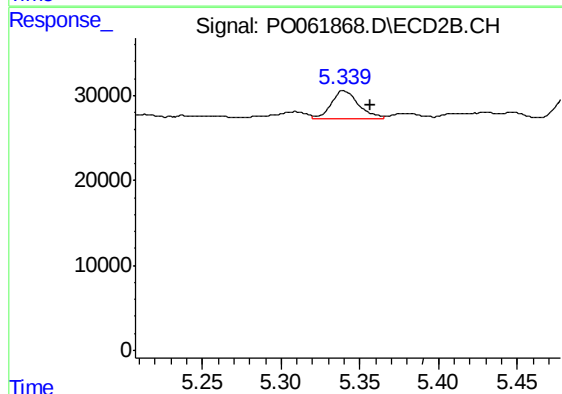


#26 AR-1254-1

R.T.: 5.339 min
Delta R.T.: -0.018 min
Response: 40620
Conc: 18.52 ng/ml m

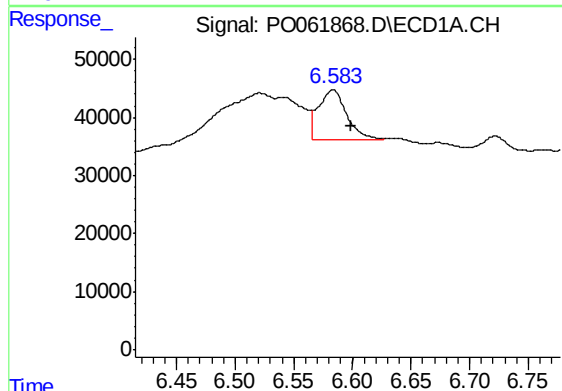


#27 AR-1254-2

R.T.: 6.583 min
Delta R.T.: -0.016 min
Response: 139308
Conc: 38.56 ng/ml m

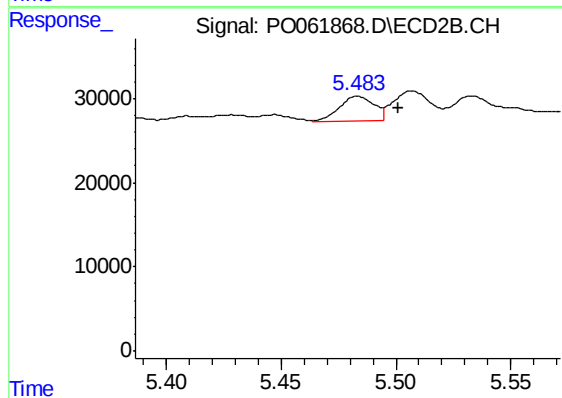

#27 AR-1254-2

R.T.: 5.483 min
Delta R.T.: -0.018 min
Response: 30942
Conc: 15.78 ng/ml m

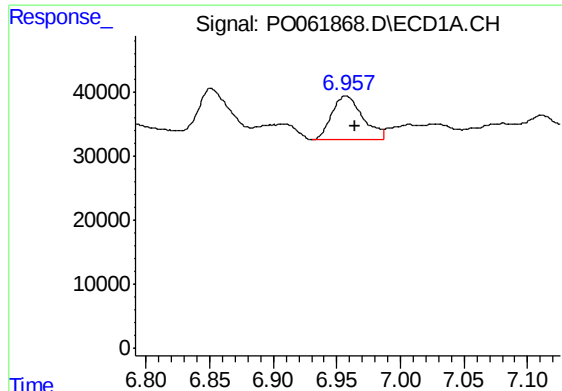


#28 AR-1254-3

R.T.: 6.957 min
Delta R.T.: -0.007 min
Response: 115827
Conc: 29.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
10/11/2019 2:11:04 PM

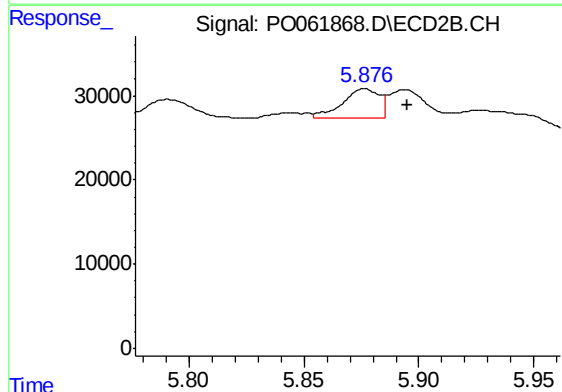


#28 AR-1254-3

R.T.: 5.876 min
Delta R.T.: -0.019 min
Response: 39755
Conc: 12.49 ng/ml m

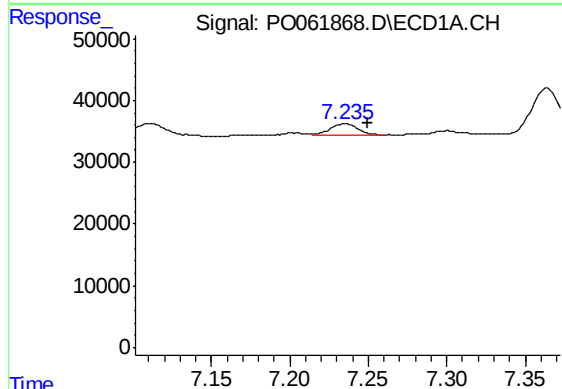


#29 AR-1254-4

R.T.: 7.235 min
Delta R.T.: -0.015 min
Response: 24595
Conc: 8.12 ng/ml m

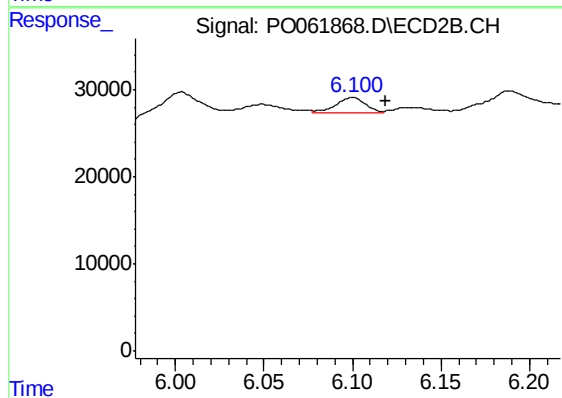

#29 AR-1254-4

R.T.: 6.100 min
Delta R.T.: -0.019 min
Response: 21036
Conc: 10.37 ng/ml m

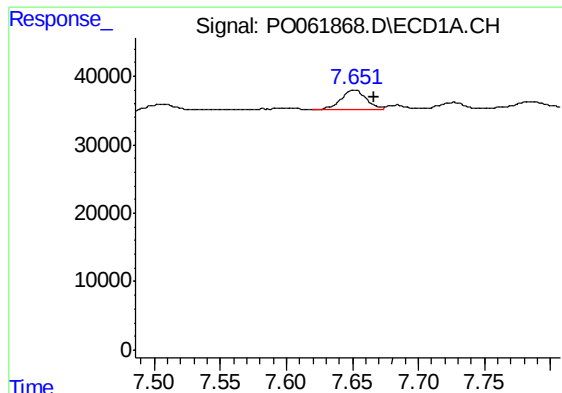


#30 AR-1254-5

R.T.: 7.651 min
Delta R.T.: -0.016 min
Response: 39324
Conc: 12.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Ankita
10/11/2019 2:11:04 PM

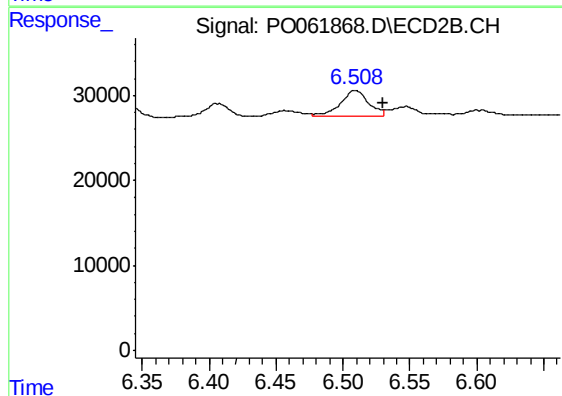

#30 AR-1254-5

R.T.: 6.508 min
Delta R.T.: -0.022 min
Response: 44733
Conc: 15.82 ng/ml m