

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101020\
 Data File : PO072235.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2020 8:56
 Operator : DD\AJ
 Sample : L4317-03DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 11935DL

Manual Integrations
 APPROVED

Ankita
 10/12/2020 2:07:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 04:17:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.323	3.507	295134	162013	4.109	4.325
2) SA Decachlor...	9.927	8.676	427451	224887	3.882	3.954
Target Compounds						
26) L6 AR-1254-1	6.517	5.580	1479641	1004231	423.511	420.209m
27) L6 AR-1254-2	6.743	5.741	2284535	815989	414.953	381.487
28) L6 AR-1254-3	7.120	6.149	2800816	1354281	484.975	398.886m
29) L6 AR-1254-4	7.415	6.389	2969729	1107501	509.741	456.105m
30) L6 AR-1254-5	7.835	6.810	2492199	1421223	463.074	434.345

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101020\
Data File : PO072235.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2020 8:56
Operator : DD\AJ
Sample : L4317-03DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
11935DL


Manual Integrations
APPROVED

Ankita
10/12/2020 2:07:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 04:17:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

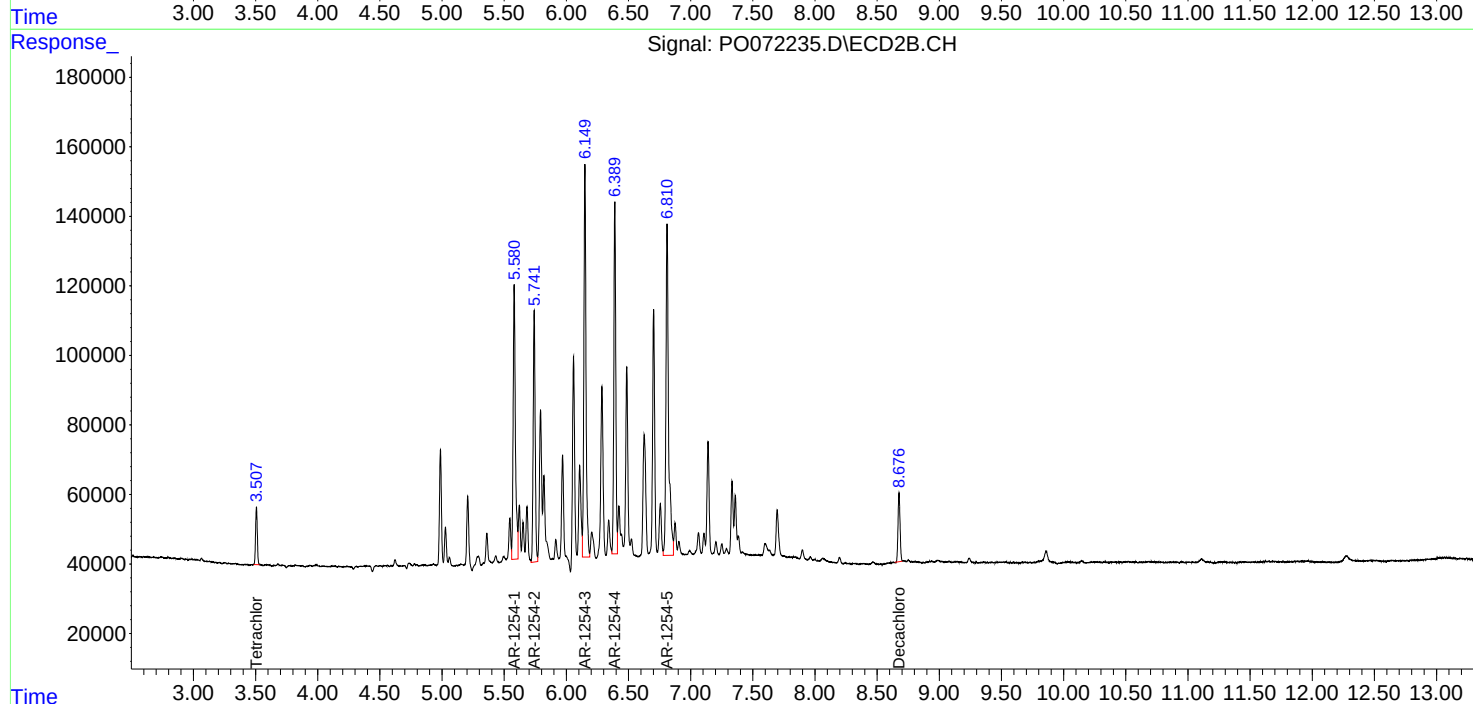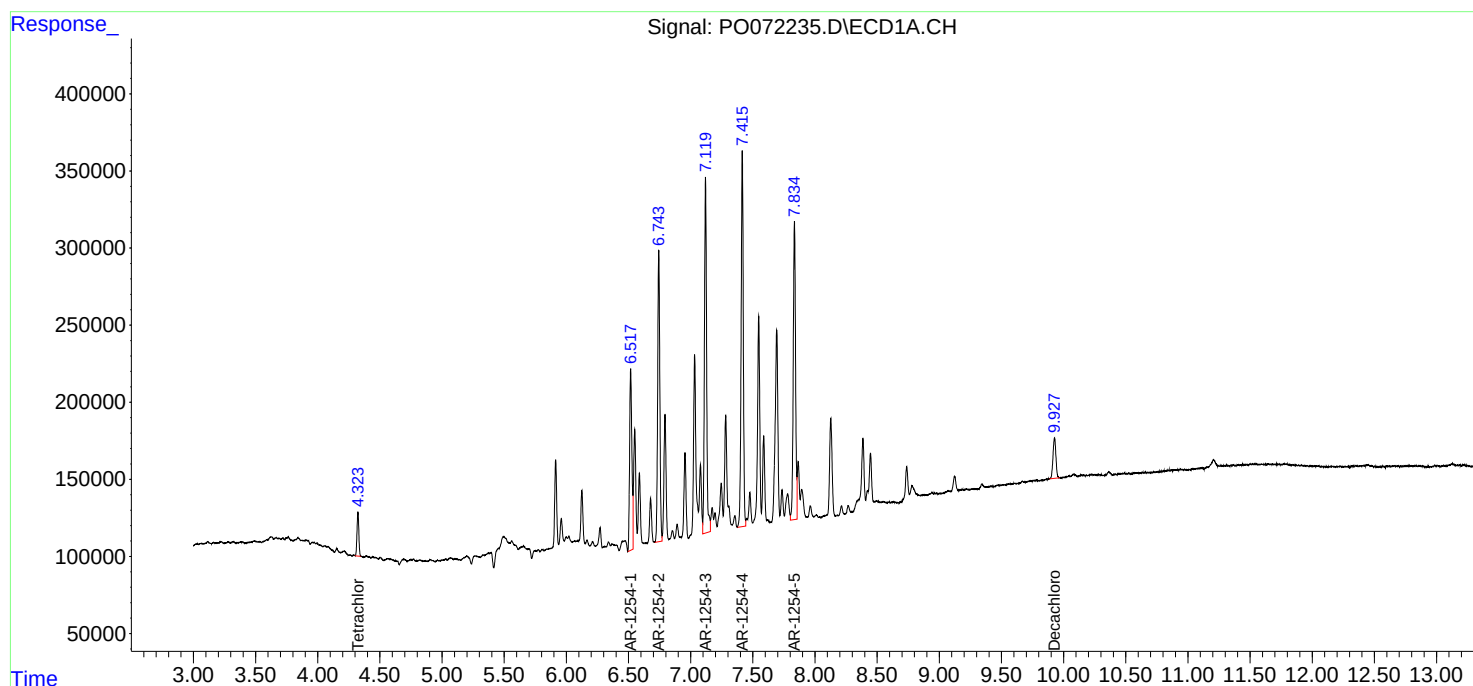

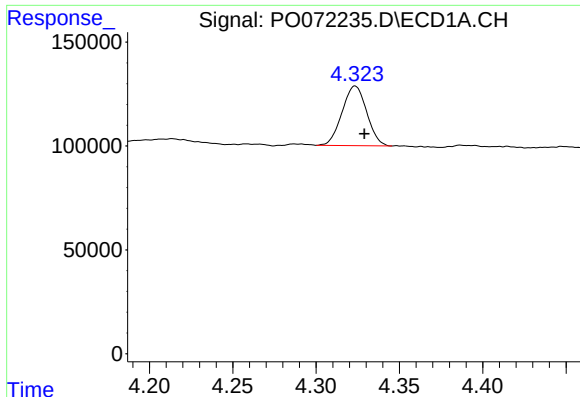


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.006 min
Response: 295134
Conc: 4.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
11935DL


Manual Integrations
APPROVED

Ankita
10/12/2020 2:07:33 PM

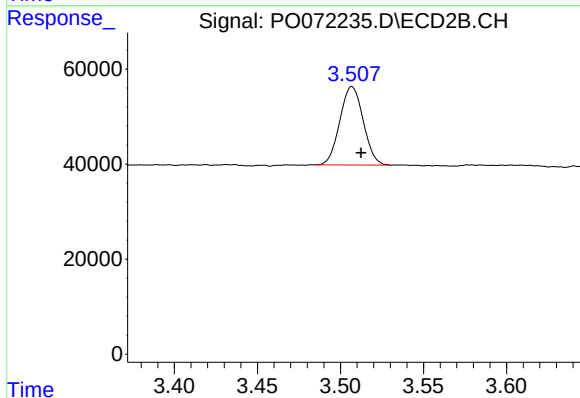


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: -0.005 min
Response: 162013
Conc: 4.33 ng/ml

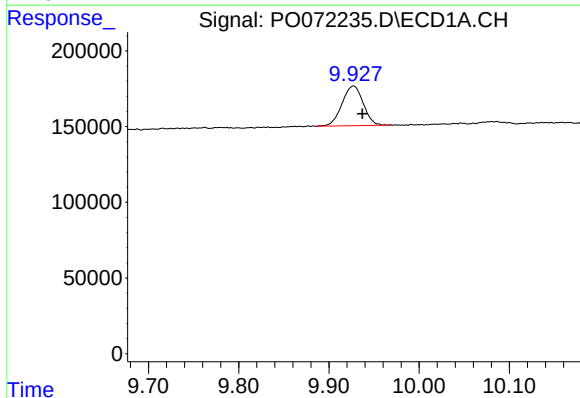


#2 Decachlorobiphenyl

R.T.: 9.927 min
Delta R.T.: -0.010 min
Response: 427451
Conc: 3.88 ng/ml

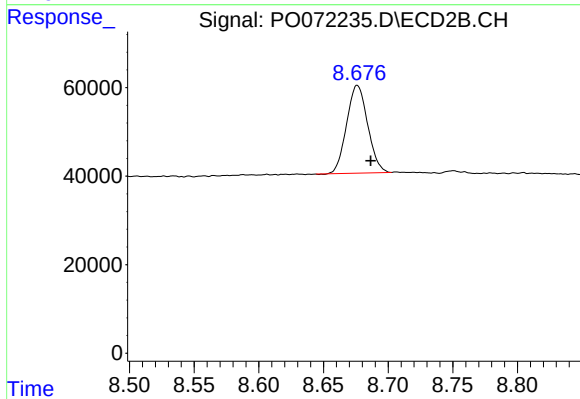

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.010 min
Response: 224887
Conc: 3.95 ng/ml

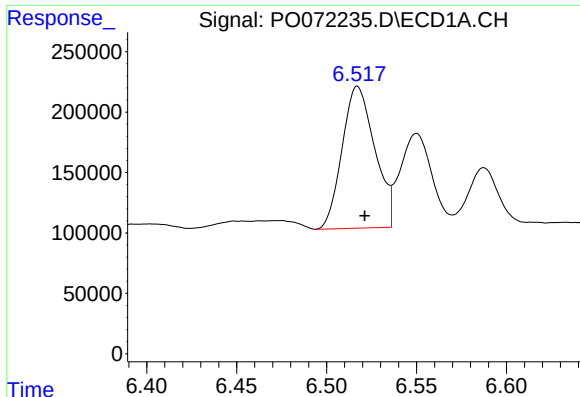


#26 AR-1254-1

R.T.: 6.517 min
Delta R.T.: -0.004 min
Response: 1479641
Conc: 423.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
11935DL


Manual Integrations
APPROVED

Ankita
10/12/2020 2:07:33 PM

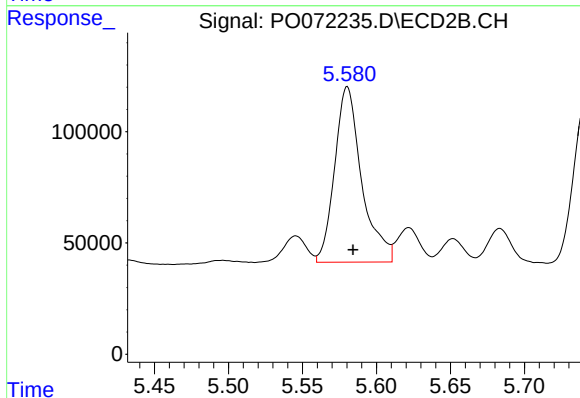


#26 AR-1254-1

R.T.: 5.580 min
Delta R.T.: -0.004 min
Response: 1004231
Conc: 420.21 ng/ml m

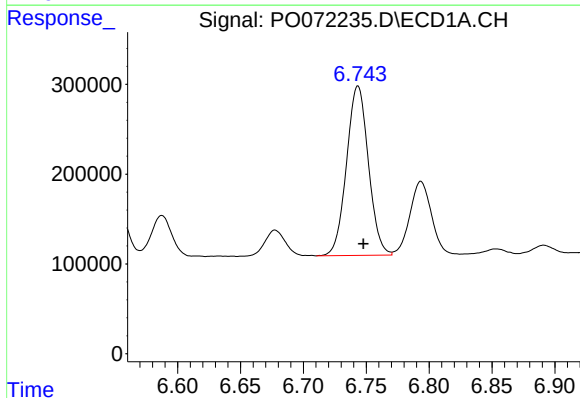


#27 AR-1254-2

R.T.: 6.743 min
Delta R.T.: -0.004 min
Response: 2284535
Conc: 414.95 ng/ml

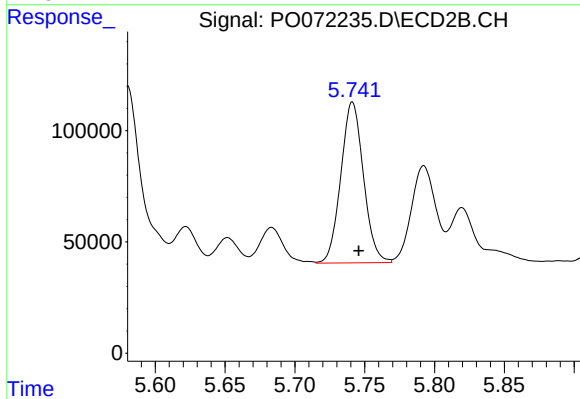

#27 AR-1254-2

R.T.: 5.741 min
Delta R.T.: -0.005 min
Response: 815989
Conc: 381.49 ng/ml

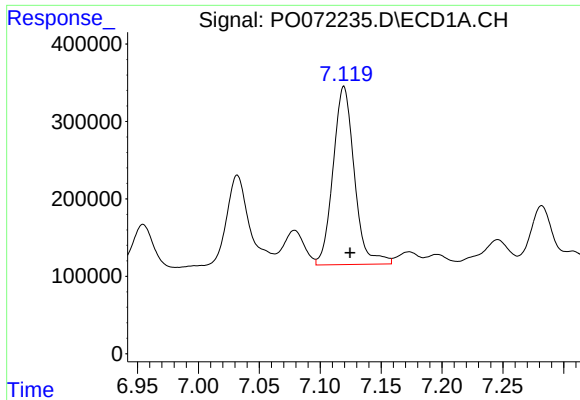


#28 AR-1254-3

R.T.: 7.120 min
Delta R.T.: -0.005 min
Response: 2800816
Conc: 484.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
11935DL


Manual Integrations
APPROVED

Ankita
10/12/2020 2:07:33 PM

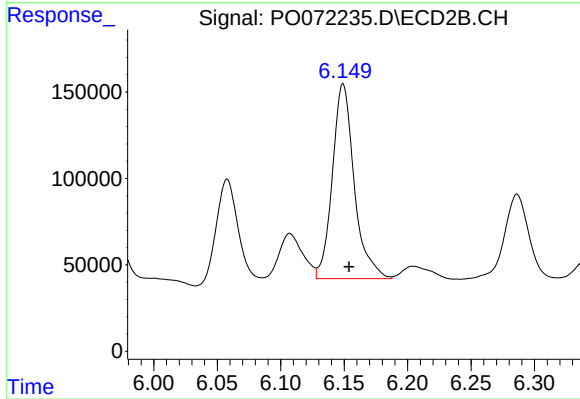


#28 AR-1254-3

R.T.: 6.149 min
Delta R.T.: -0.005 min
Response: 1354281
Conc: 398.89 ng/ml m

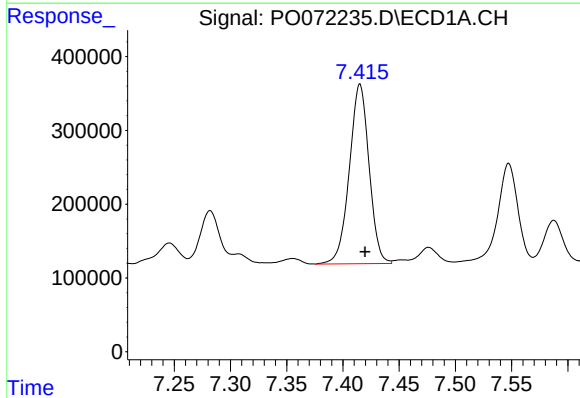


#29 AR-1254-4

R.T.: 7.415 min
Delta R.T.: -0.005 min
Response: 2969729
Conc: 509.74 ng/ml

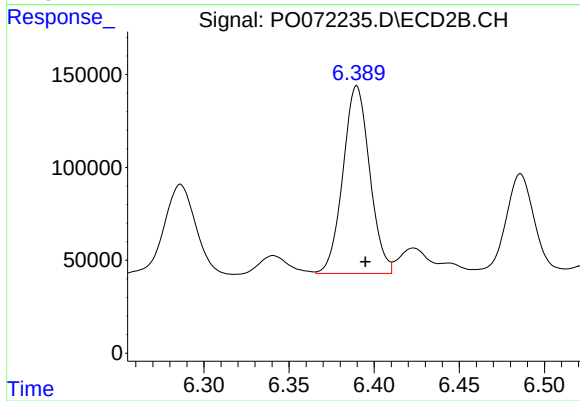

#29 AR-1254-4

R.T.: 6.389 min
Delta R.T.: -0.006 min
Response: 1107501
Conc: 456.10 ng/ml m

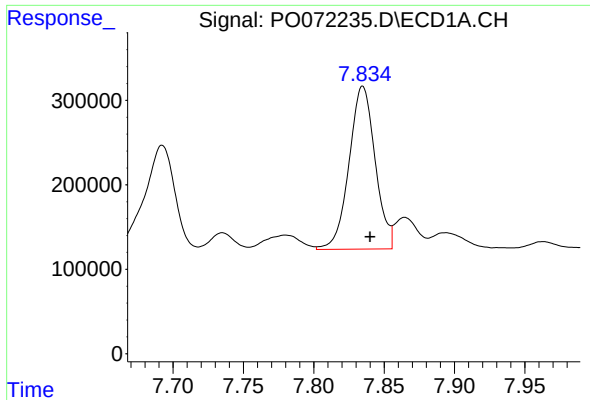


#30 AR-1254-5

R.T.: 7.835 min
Delta R.T.: -0.005 min
Response: 2492199
Conc: 463.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
11935DL

Manual Integrations
APPROVED

Ankita
10/12/2020 2:07:33 PM

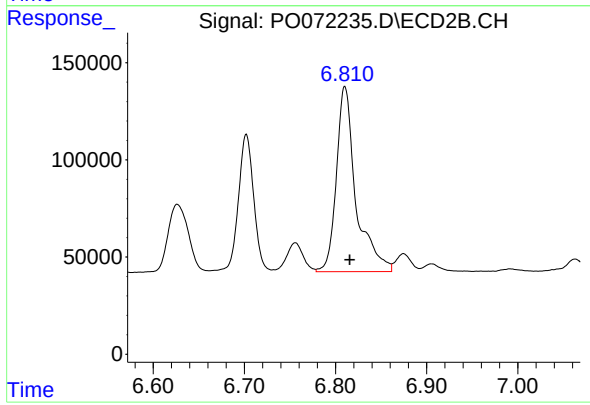

#30 AR-1254-5

R.T.: 6.810 min
Delta R.T.: -0.005 min
Response: 1421223
Conc: 434.34 ng/ml