

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101023\
 Data File : PO098642.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 14:15
 Operator : YP/AJ
 Sample : 04699-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 04:20:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	3.635	23225767	9348322	12.096	12.003
2)	SA Decachlor...	10.295	8.643	15041596	7287651	12.391	13.602
Target Compounds							
8)	L2 AR-1221-1	4.691	3.848	357501	191237	15.878	20.815 #
9)	L2 AR-1221-2	4.787	3.935	741760	232911	43.961	35.027
10)	L2 AR-1221-3	4.854	4.011	773335	294269	15.812	14.588



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101023\
Data File : PO098642.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 14:15
Operator : YP/AJ
Sample : 04699-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 04:20:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

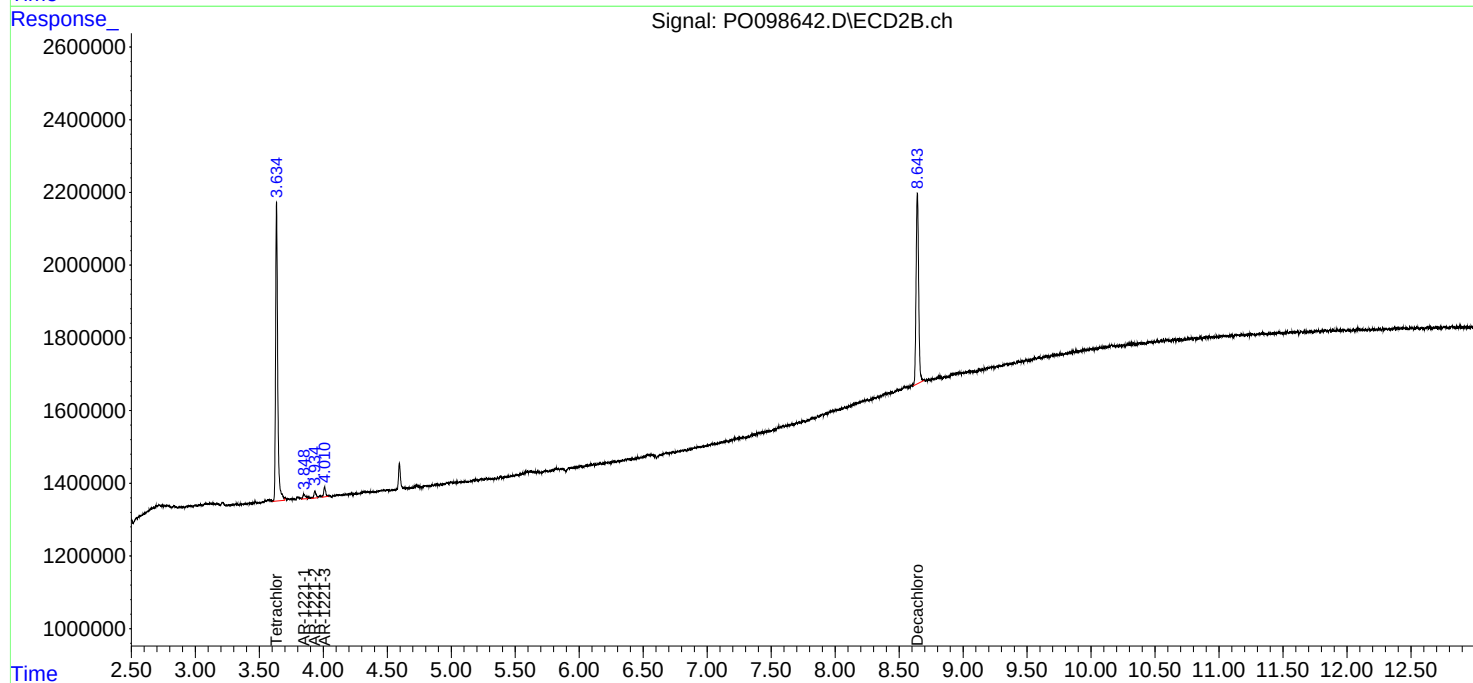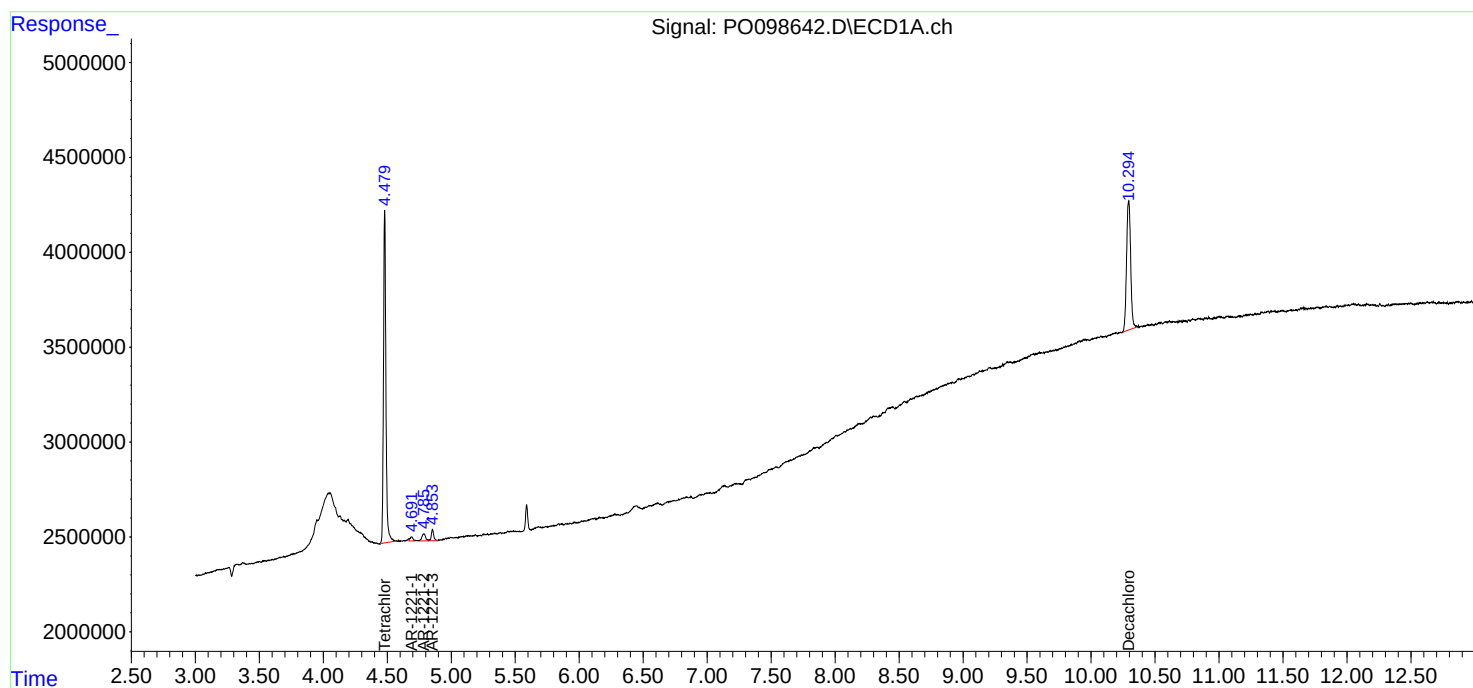


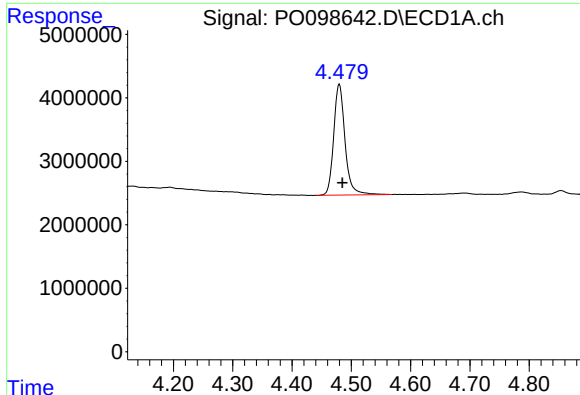

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.005 min
Response: 23225767
Conc: 12.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

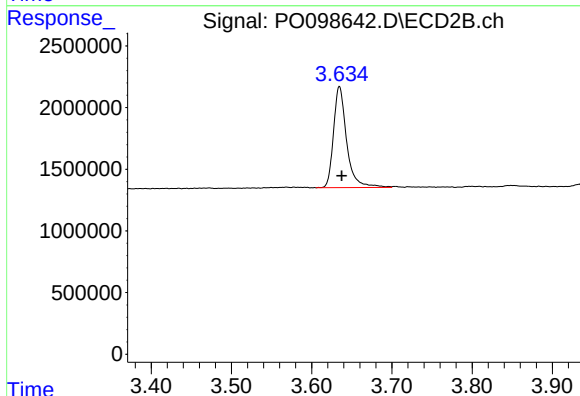


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.003 min
Response: 9348322
Conc: 12.00 ng/ml

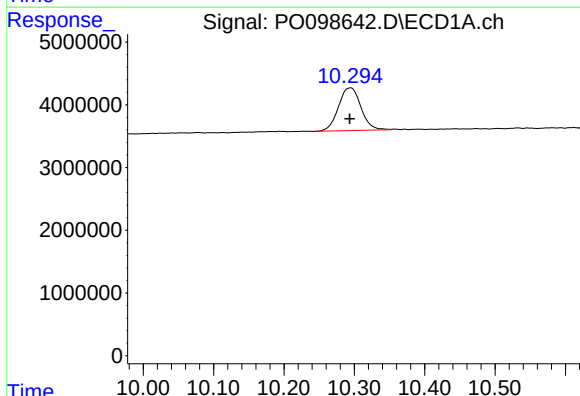


#2 Decachlorobiphenyl

R.T.: 10.295 min
Delta R.T.: 0.001 min
Response: 15041596
Conc: 12.39 ng/ml

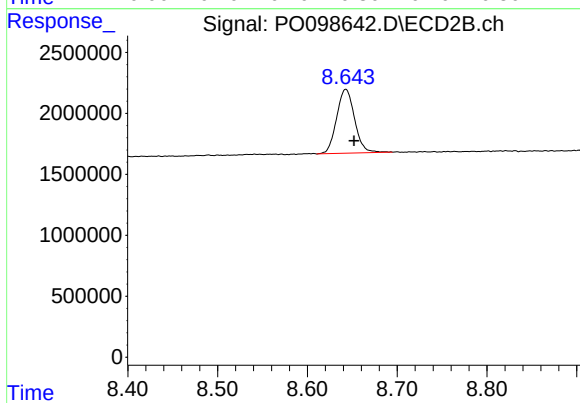

#2 Decachlorobiphenyl


R.T.: 8.643 min
Delta R.T.: -0.009 min
Response: 7287651
Conc: 13.60 ng/ml

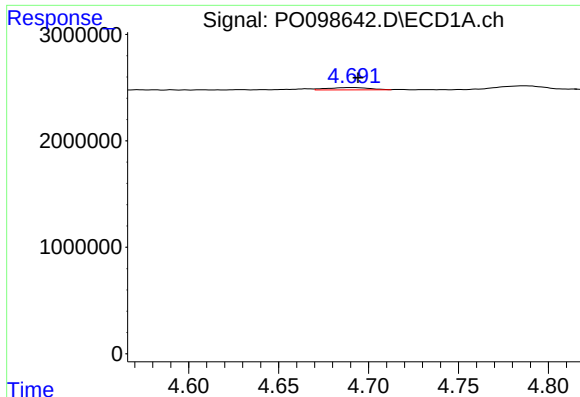

#8 AR-1221-1


R.T.: 4.691 min
Delta R.T.: -0.003 min
Response: 357501
Conc: 15.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

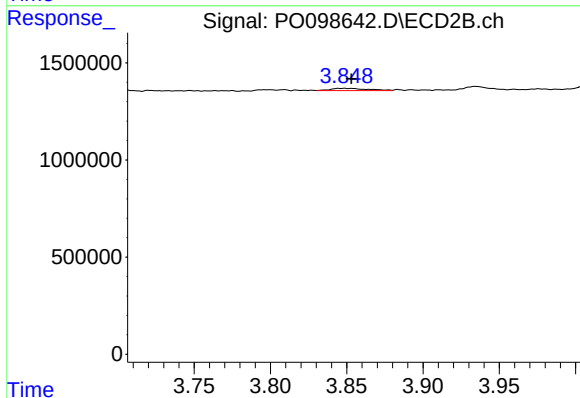


#8 AR-1221-1

R.T.: 3.848 min
Delta R.T.: -0.005 min
Response: 191237
Conc: 20.81 ng/ml

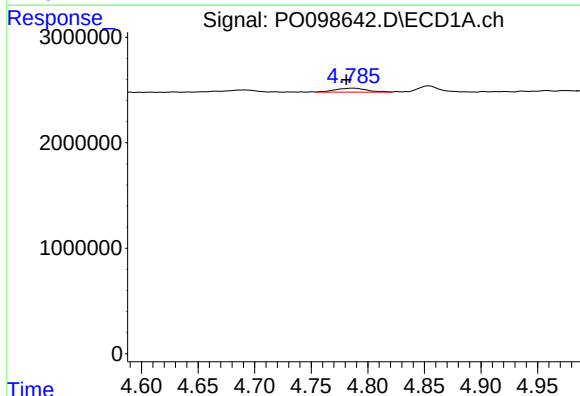


#9 AR-1221-2

R.T.: 4.787 min
Delta R.T.: 0.006 min
Response: 741760
Conc: 43.96 ng/ml

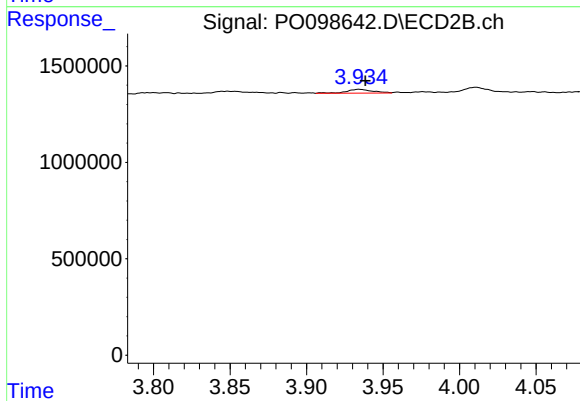

#9 AR-1221-2


R.T.: 3.935 min
Delta R.T.: -0.004 min
Response: 232911
Conc: 35.03 ng/ml

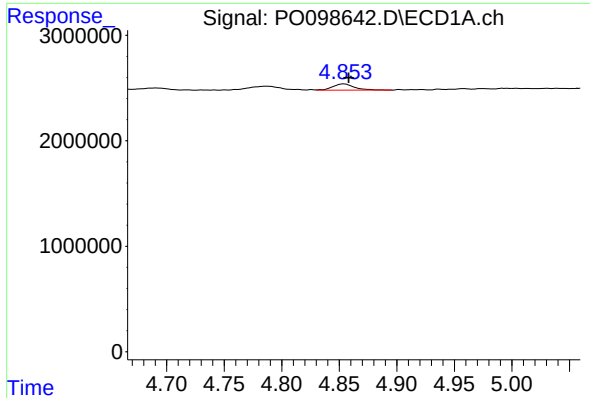

#10 AR-1221-3

R.T.: 4.854 min
Delta R.T.: -0.004 min
Response: 773335
Conc: 15.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

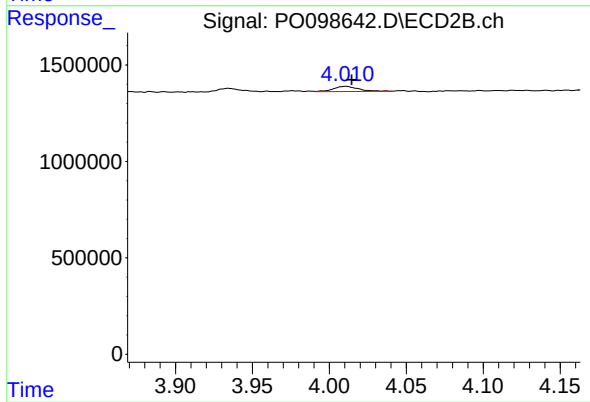

#10 AR-1221-3

R.T.: 4.011 min
Delta R.T.: -0.004 min
Response: 294269
Conc: 14.59 ng/ml