

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101023\
 Data File : PO098643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 14:32
 Operator : YP/AJ
 Sample : 04699-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 04:21:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	3.634	37245688	15027917	19.397	19.295
2)	SA Decachlor...	10.293	8.642	24804950	11689643	20.435	21.819
Target Compounds							
11)	L3 AR-1232-1	4.853	4.010	900823	375610	22.054	22.347
12)	L3 AR-1232-2	5.385	4.736	512925	394714	23.716	26.268
13)	L3 AR-1232-3	5.678	4.915	748207	142415	21.048	18.196
14)	L3 AR-1232-4	5.838	4.998	405024	201170	23.858	26.754
15)	L3 AR-1232-5	5.929	5.168	165048	218192	11.592	26.971 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101023\
Data File : PO098643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 14:32
Operator : YP/AJ
Sample : 04699-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 04:21:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

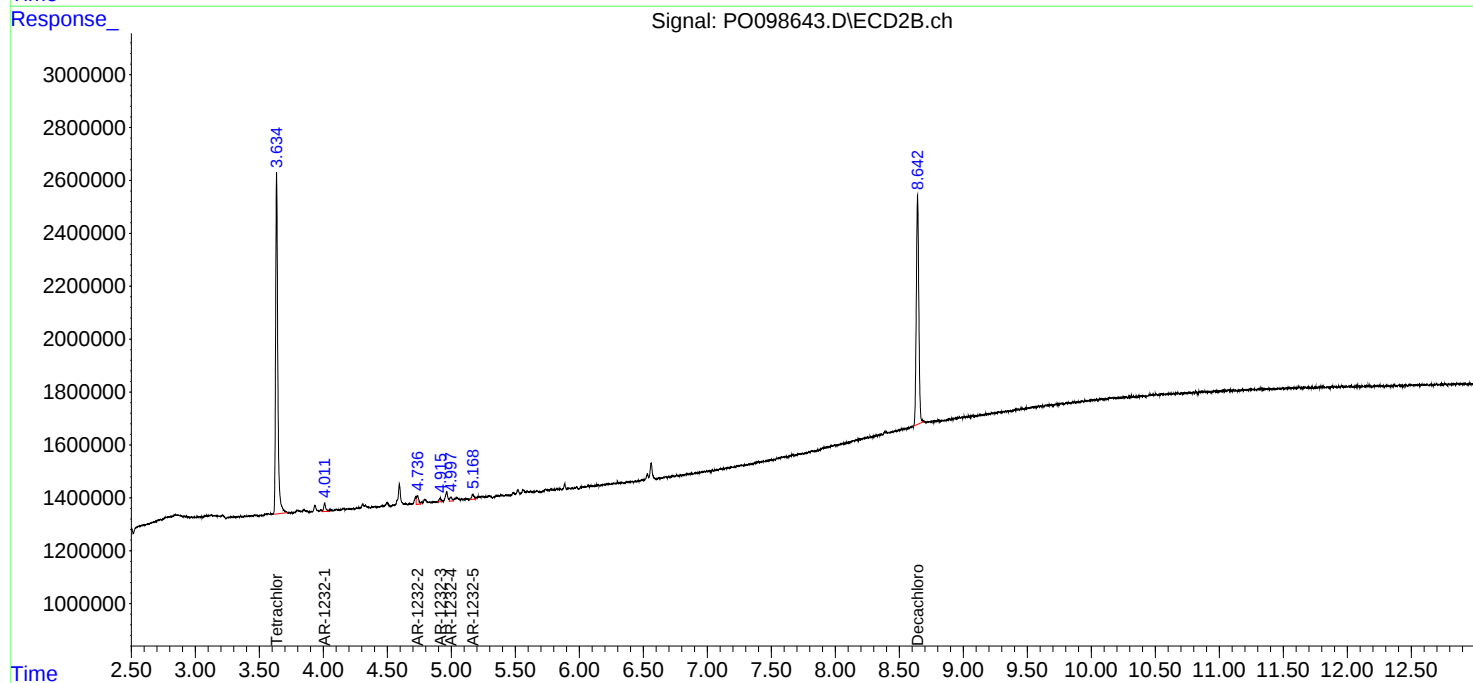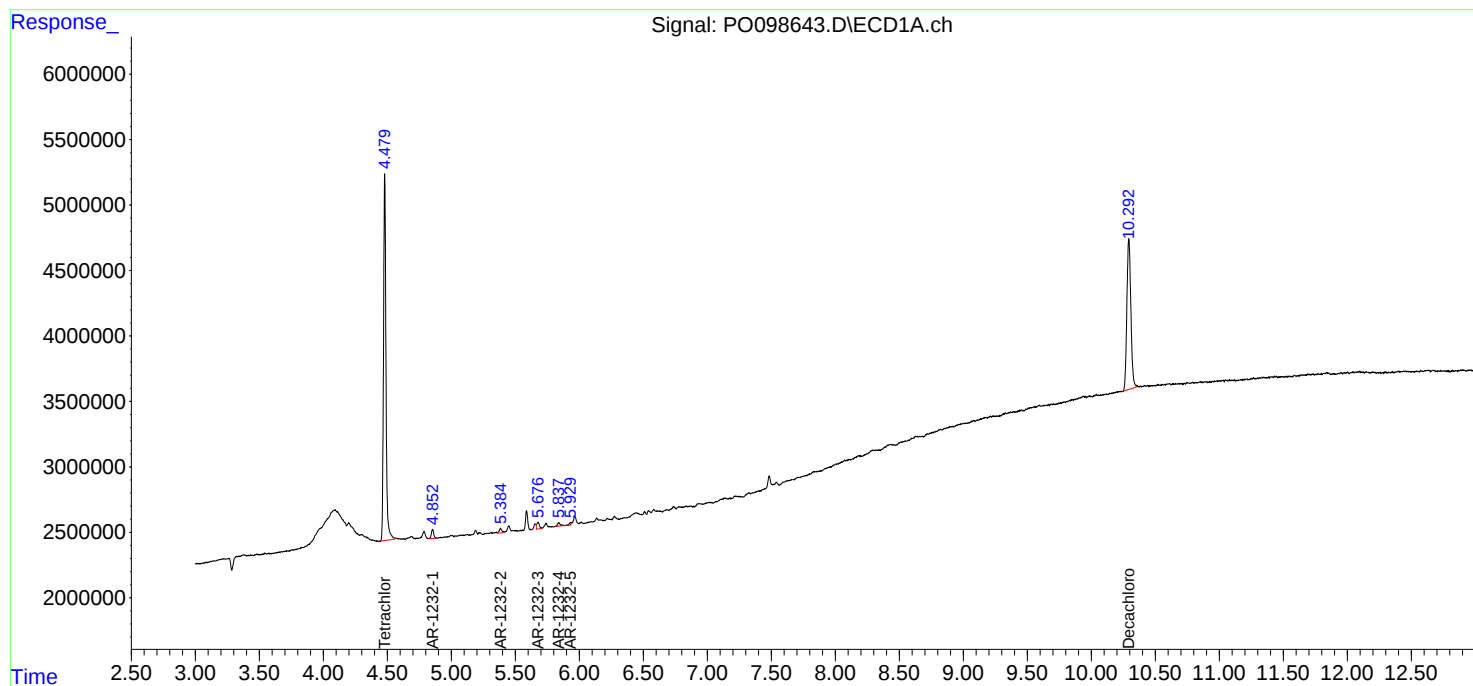


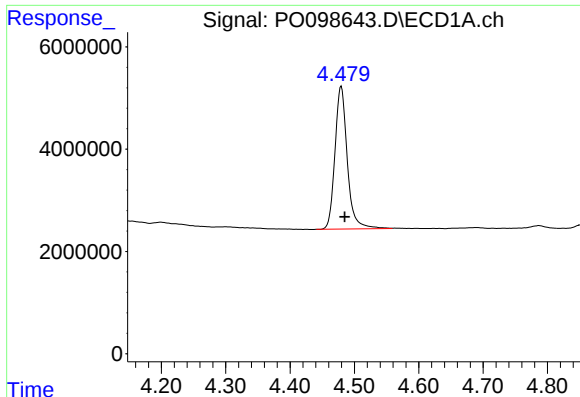

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.006 min
Response: 37245688
Conc: 19.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

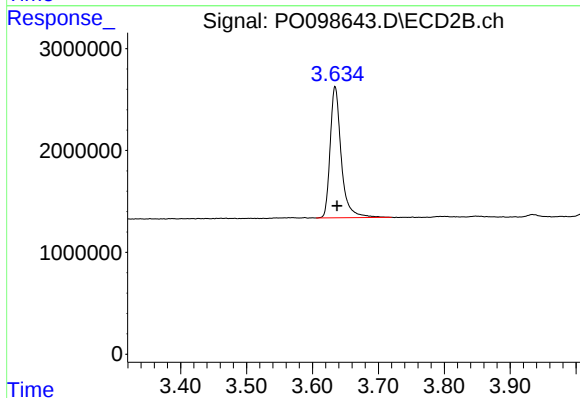


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.003 min
Response: 15027917
Conc: 19.29 ng/ml

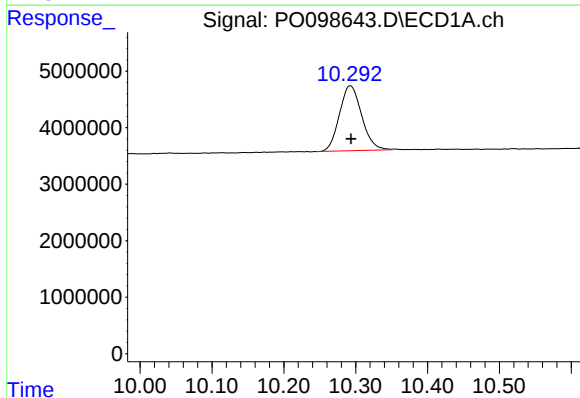


#2 Decachlorobiphenyl

R.T.: 10.293 min
Delta R.T.: 0.000 min
Response: 24804950
Conc: 20.43 ng/ml

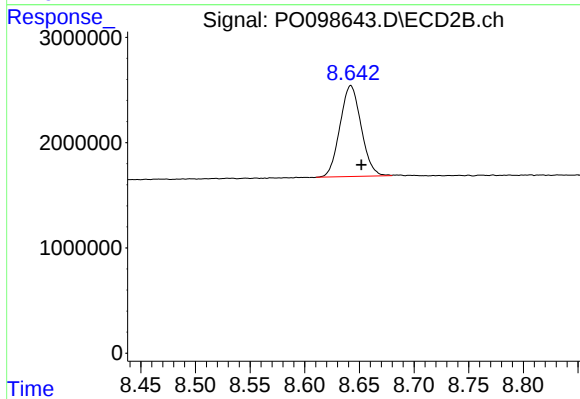

#2 Decachlorobiphenyl


R.T.: 8.642 min
Delta R.T.: -0.010 min
Response: 11689643
Conc: 21.82 ng/ml

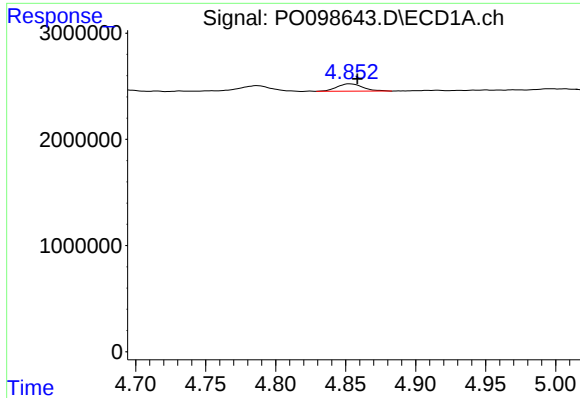

#11 AR-1232-1


R.T.: 4.853 min
Delta R.T.: -0.005 min
Response: 900823
Conc: 22.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

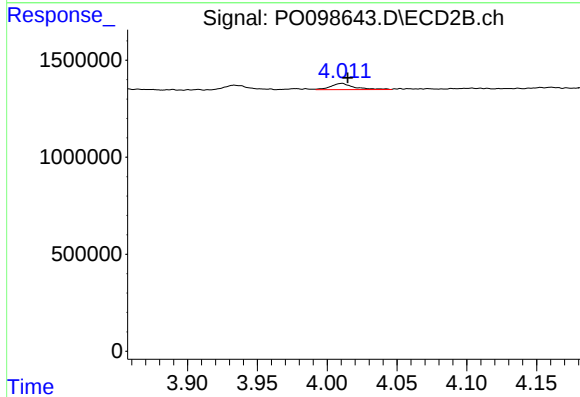


#11 AR-1232-1

R.T.: 4.010 min
Delta R.T.: -0.004 min
Response: 375610
Conc: 22.35 ng/ml

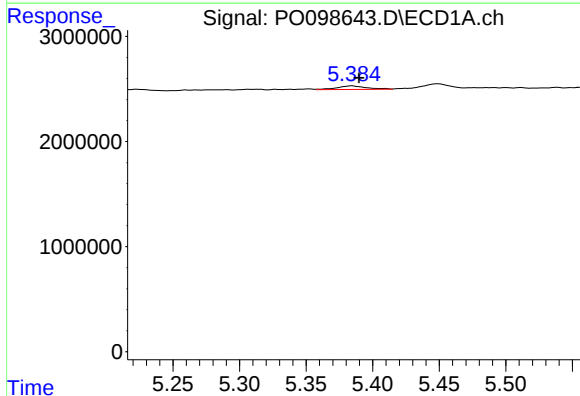


#12 AR-1232-2

R.T.: 5.385 min
Delta R.T.: -0.005 min
Response: 512925
Conc: 23.72 ng/ml

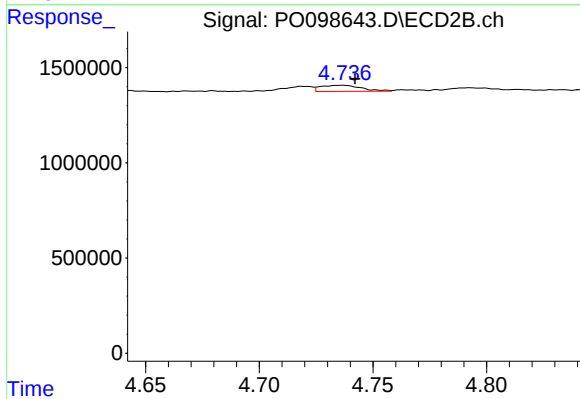

#12 AR-1232-2


R.T.: 4.736 min
Delta R.T.: -0.006 min
Response: 394714
Conc: 26.27 ng/ml

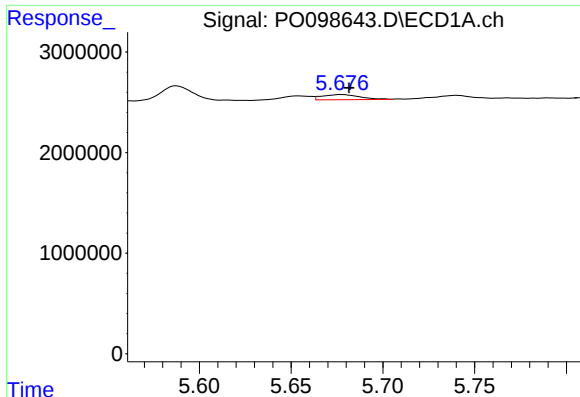

#13 AR-1232-3


R.T.: 5.678 min
Delta R.T.: -0.004 min
Response: 748207
Conc: 21.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

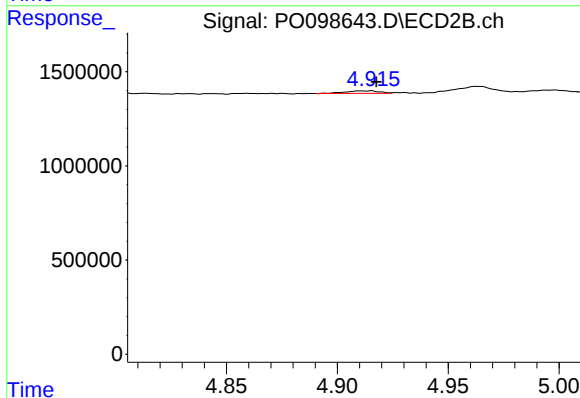


#13 AR-1232-3

R.T.: 4.915 min
Delta R.T.: -0.003 min
Response: 142415
Conc: 18.20 ng/ml

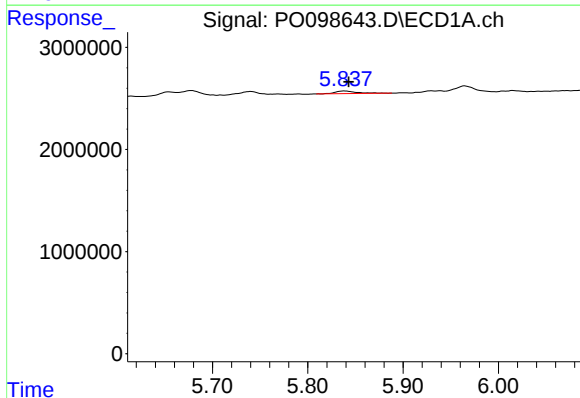


#14 AR-1232-4

R.T.: 5.838 min
Delta R.T.: -0.005 min
Response: 405024
Conc: 23.86 ng/ml

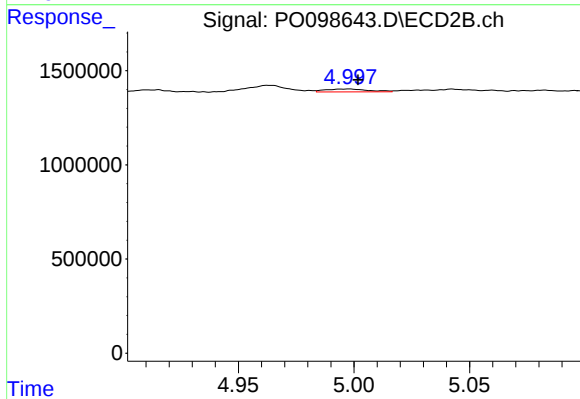

#14 AR-1232-4


R.T.: 4.998 min
Delta R.T.: -0.004 min
Response: 201170
Conc: 26.75 ng/ml

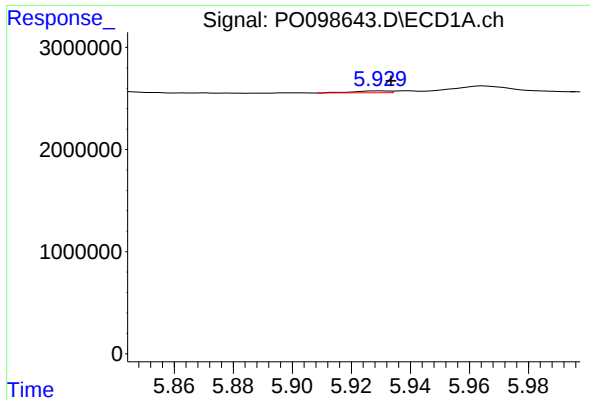

#15 AR-1232-5

R.T.: 5.929 min
Delta R.T.: -0.004 min
Response: 165048
Conc: 11.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

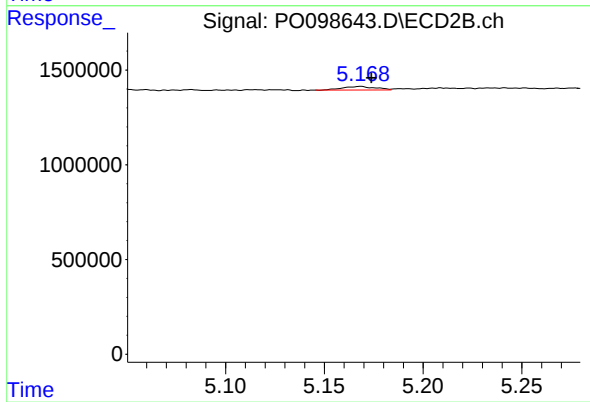

#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: -0.005 min
Response: 218192
Conc: 26.97 ng/ml