

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101023\
 Data File : PO098646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2023 15:23
 Operator : YP/AJ
 Sample : 04699-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 04:23:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	3.635	25303451	10219885	13.178	13.122
2) SA Decachlor...	10.294	8.643	16407042	7935832	13.516	14.812
Target Compounds						
26) L6 AR-1254-1	6.514	5.520	1126723	679788	17.838	17.729
27) L6 AR-1254-2	6.733	5.669	1745455	648890	18.188	18.848
28) L6 AR-1254-3	7.100	6.073	1558602	928374	16.565	17.866
29) L6 AR-1254-4	7.387	6.301	798366	484129	13.712	17.638 #
30) L6 AR-1254-5	7.806	6.720	1135124	762887	16.252	17.611



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101023\
Data File : PO098646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2023 15:23
Operator : YP/AJ
Sample : 04699-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 04:23:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

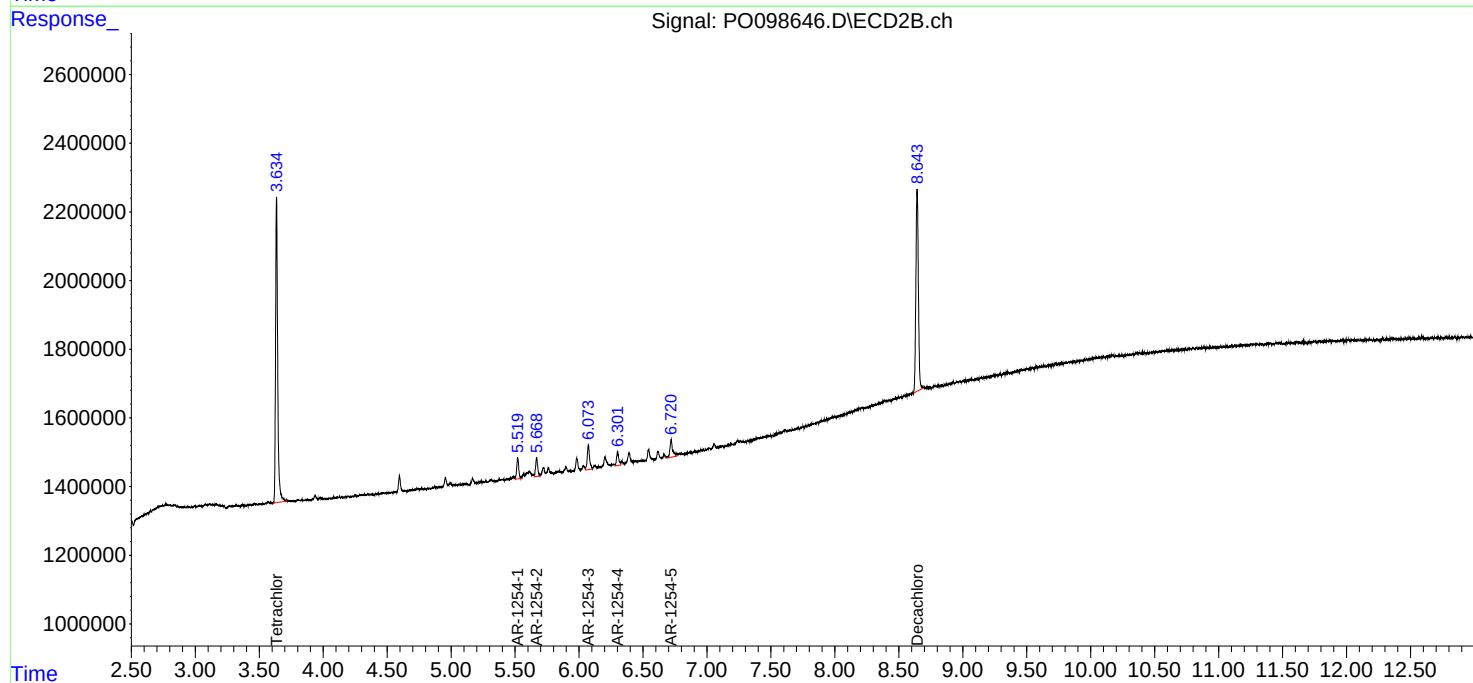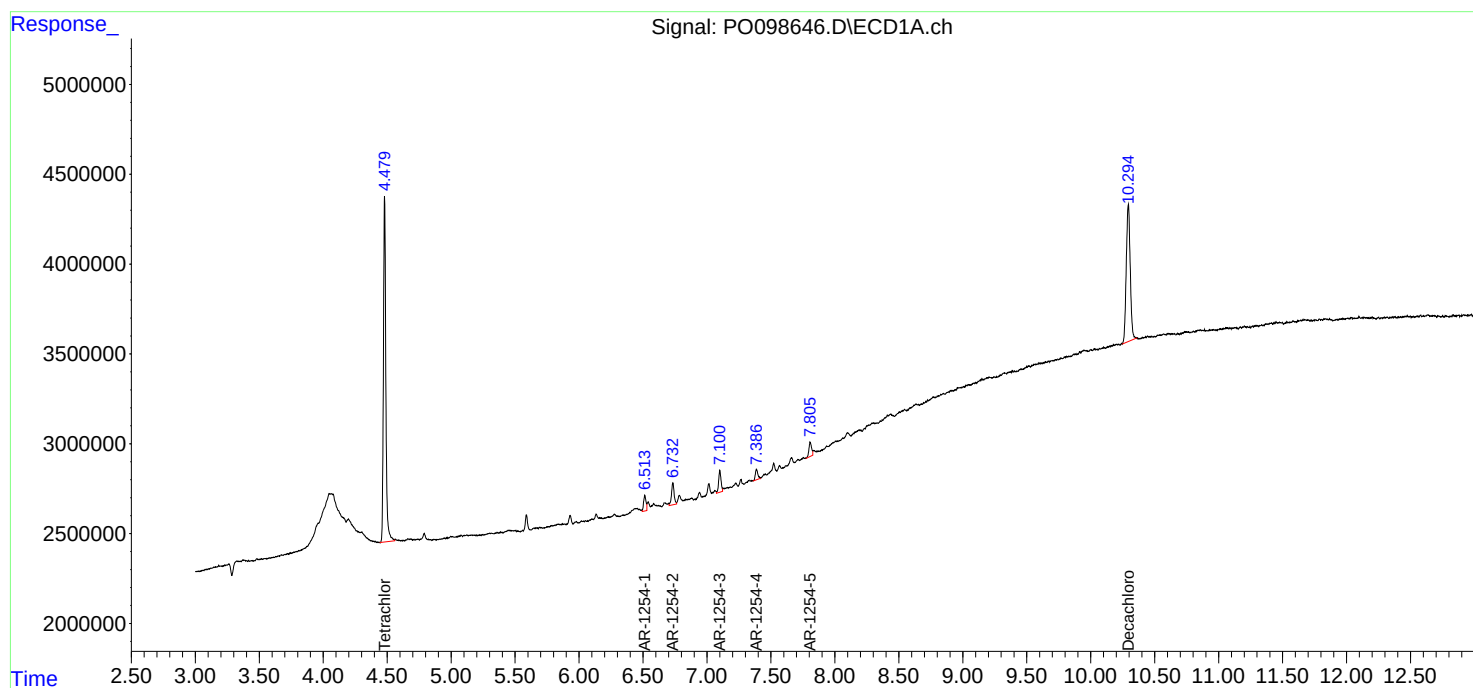


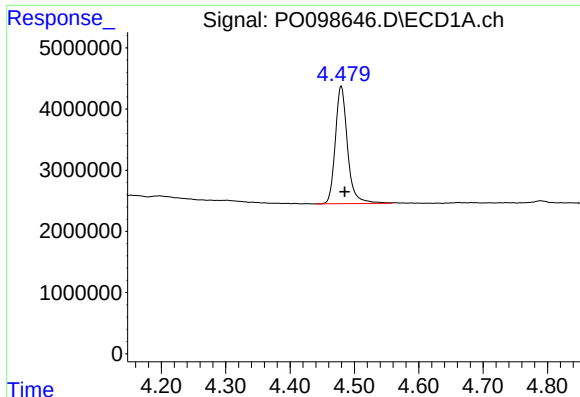

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: -0.005 min
Response: 25303451
Conc: 13.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

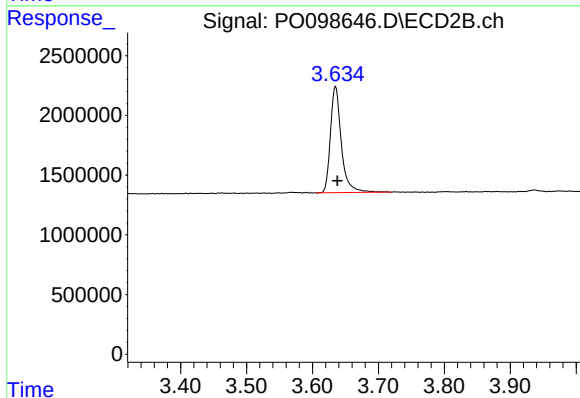


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: -0.003 min
Response: 10219885
Conc: 13.12 ng/ml

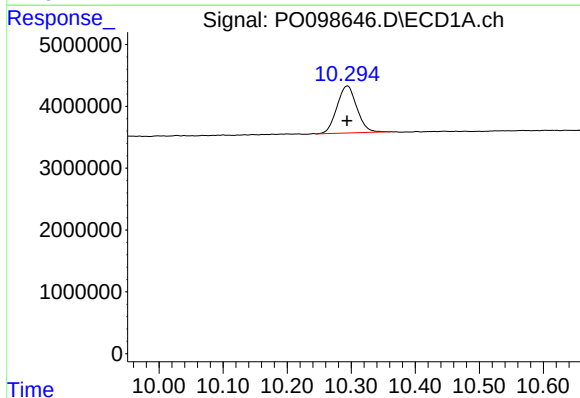


#2 Decachlorobiphenyl

R.T.: 10.294 min
Delta R.T.: 0.000 min
Response: 16407042
Conc: 13.52 ng/ml

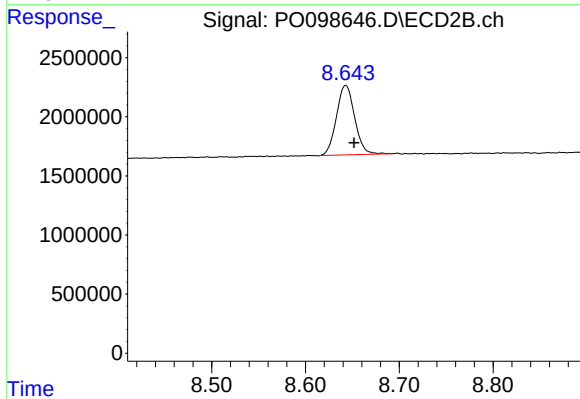

#2 Decachlorobiphenyl


R.T.: 8.643 min
Delta R.T.: -0.009 min
Response: 7935832
Conc: 14.81 ng/ml

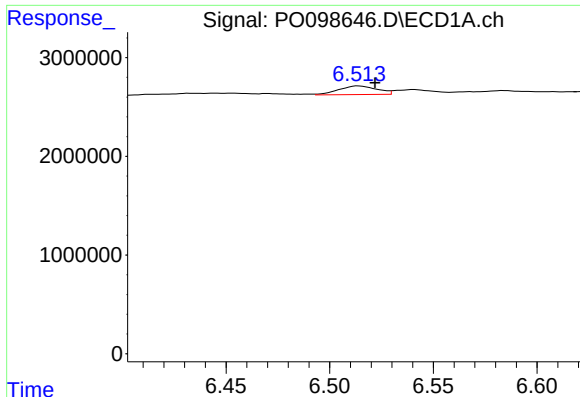

#26 AR-1254-1


R.T.: 6.514 min
Delta R.T.: -0.008 min
Response: 1126723
Conc: 17.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

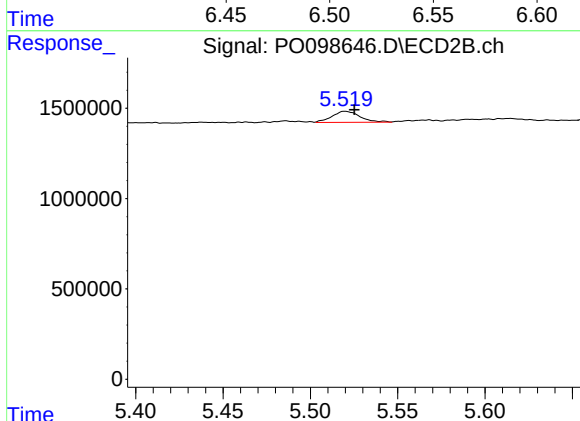


#26 AR-1254-1

R.T.: 5.520 min
Delta R.T.: -0.005 min
Response: 679788
Conc: 17.73 ng/ml

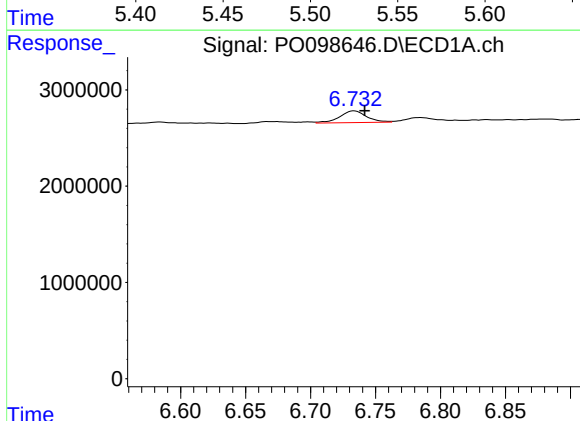


#27 AR-1254-2

R.T.: 6.733 min
Delta R.T.: -0.008 min
Response: 1745455
Conc: 18.19 ng/ml

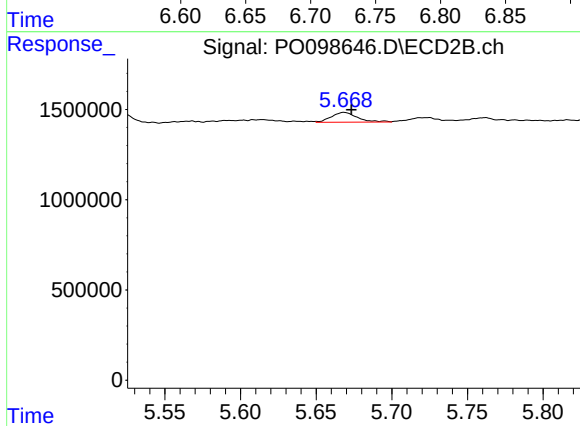

#27 AR-1254-2


R.T.: 5.669 min
Delta R.T.: -0.005 min
Response: 648890
Conc: 18.85 ng/ml

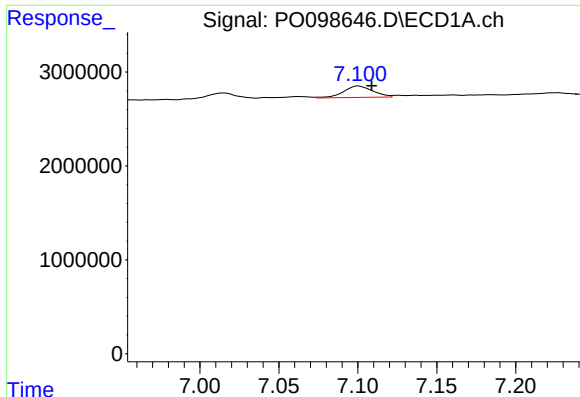

#28 AR-1254-3


R.T.: 7.100 min
Delta R.T.: -0.008 min
Response: 1558602
Conc: 16.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

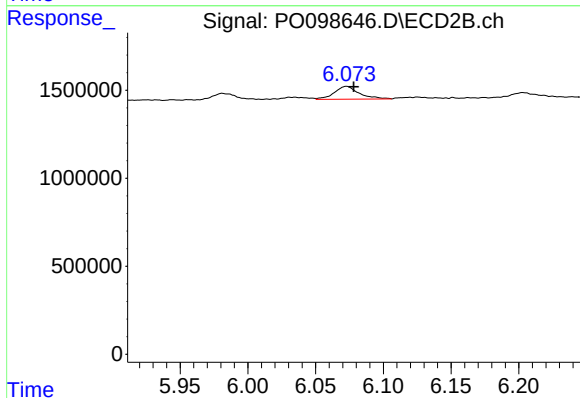


#28 AR-1254-3

R.T.: 6.073 min
Delta R.T.: -0.005 min
Response: 928374
Conc: 17.87 ng/ml

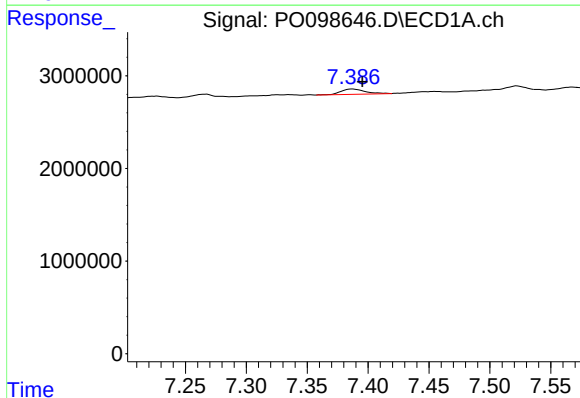


#29 AR-1254-4

R.T.: 7.387 min
Delta R.T.: -0.008 min
Response: 798366
Conc: 13.71 ng/ml

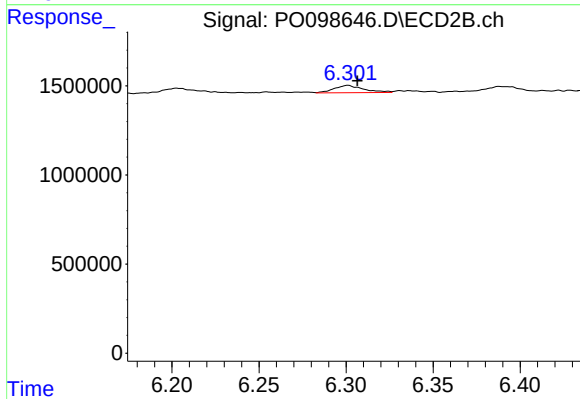

#29 AR-1254-4


R.T.: 6.301 min
Delta R.T.: -0.006 min
Response: 484129
Conc: 17.64 ng/ml

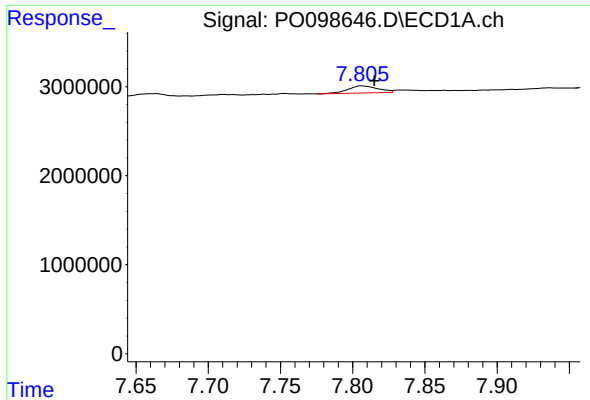

#30 AR-1254-5

R.T.: 7.806 min
Delta R.T.: -0.009 min
Response: 1135124
Conc: 16.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2023

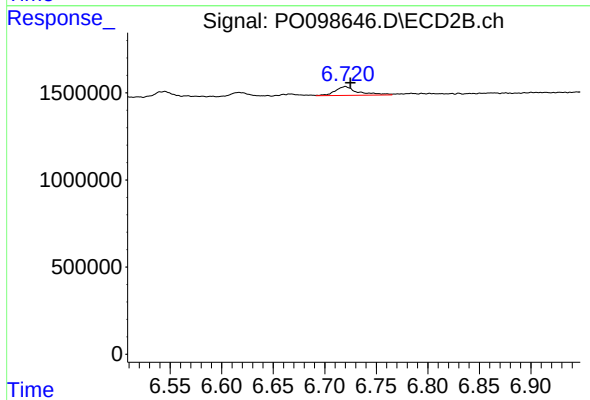

#30 AR-1254-5

R.T.: 6.720 min
Delta R.T.: -0.005 min
Response: 762887
Conc: 17.61 ng/ml