

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101024\
 Data File : P0107073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Oct 2024 18:28
 Operator : YP/AJ
 Sample : P4373-06 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2306-0016-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/11/2024
 Supervised By :Ankita Jodhani 10/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 01:56:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 04:48:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.373	3.646	9266615	4437445	0.772	1.113 #
2) SA Decachlor...	10.049	8.641	3174572	3358561	1.269	1.196m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101024\
Data File : PO107073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Oct 2024 18:28
Operator : YP/AJ
Sample : P4373-06 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2306-0016-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :Ankita Jodhani 10/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 01:56:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 04:48:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

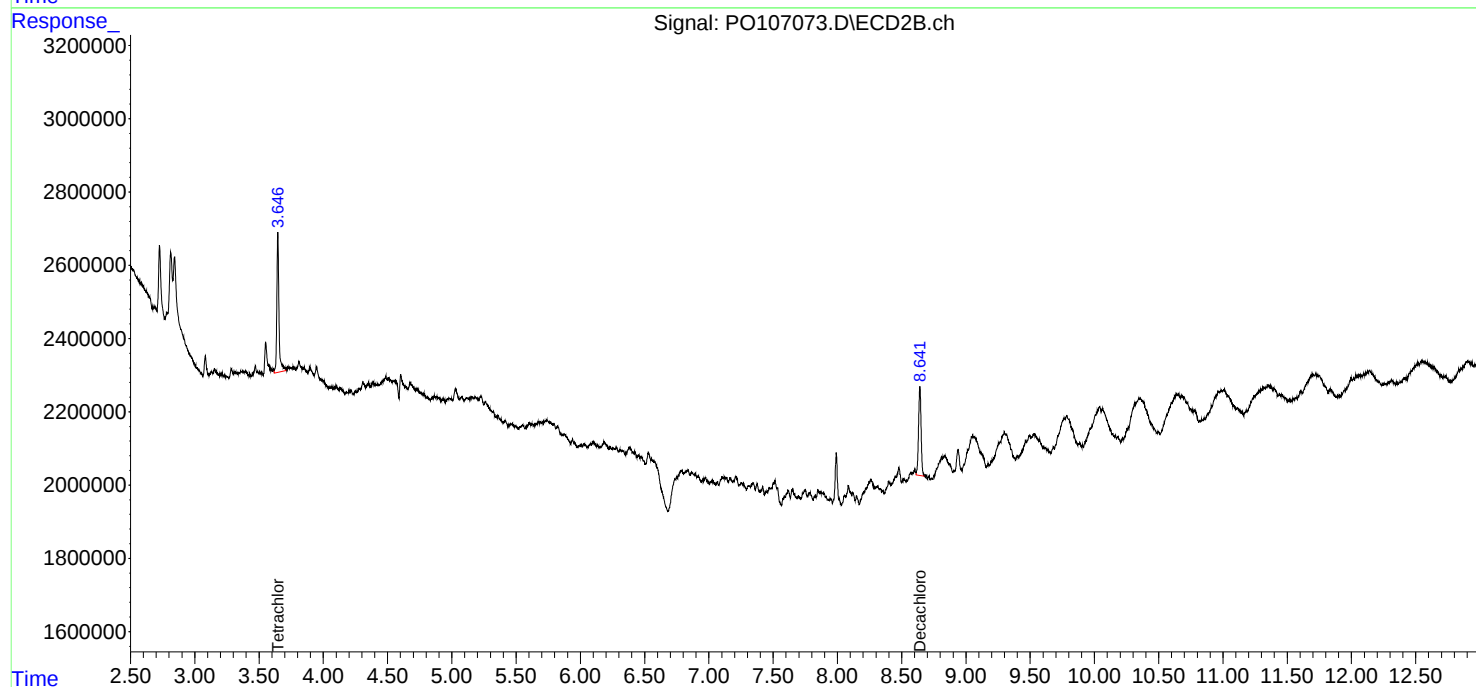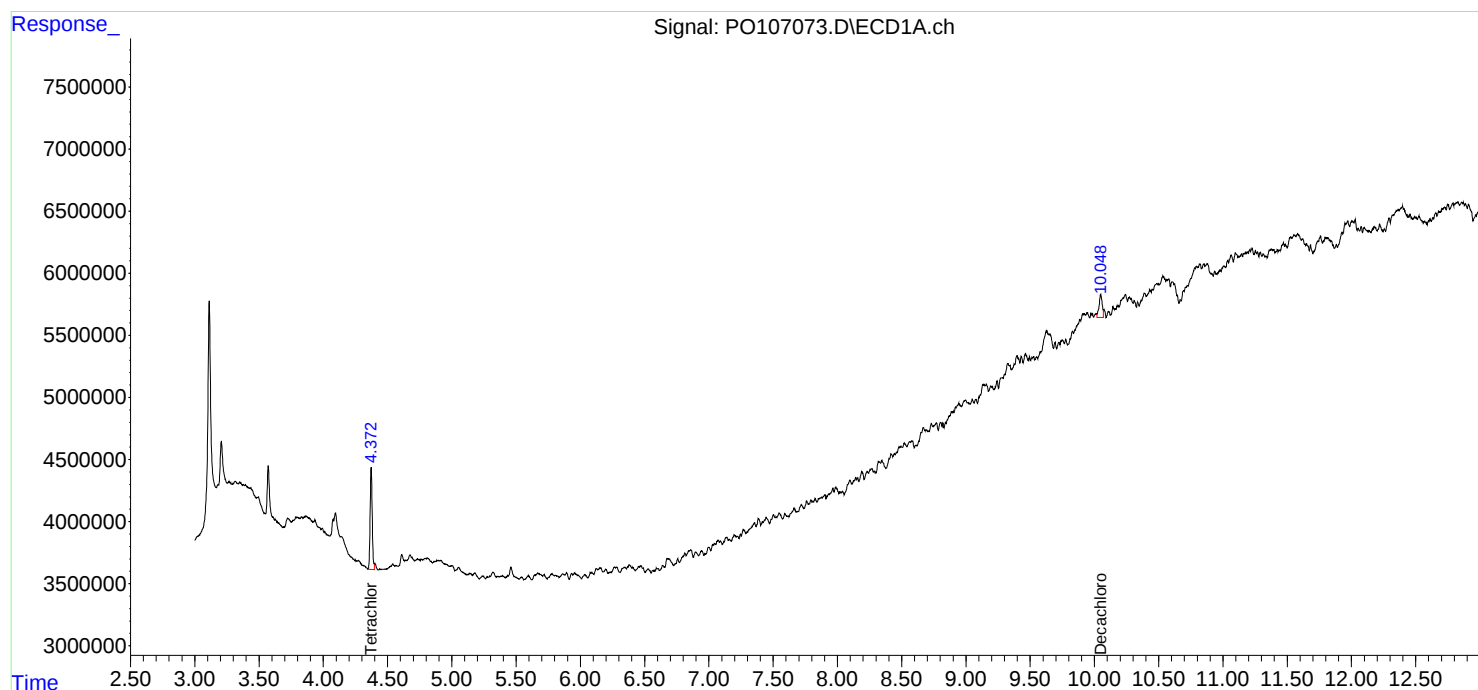

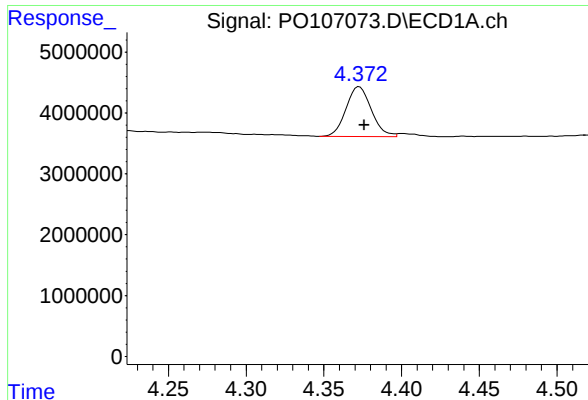


#1 Tetrachloro-m-xylene

R.T.: 4.373 min
Delta R.T.: -0.003 min
Response: 9266615
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2306-0016-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/11/2024
Supervised By :Ankita Jodhani 10/11/2024

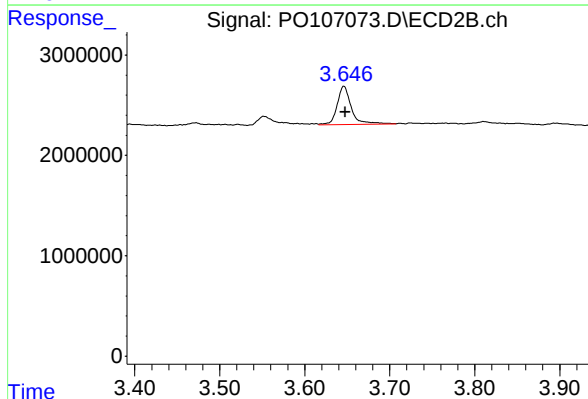


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.002 min
Response: 4437445
Conc: 1.11 ng/ml

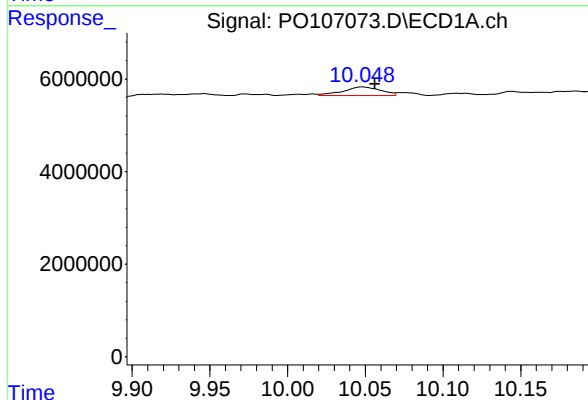

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: -0.008 min
Response: 3174572
Conc: 1.27 ng/ml

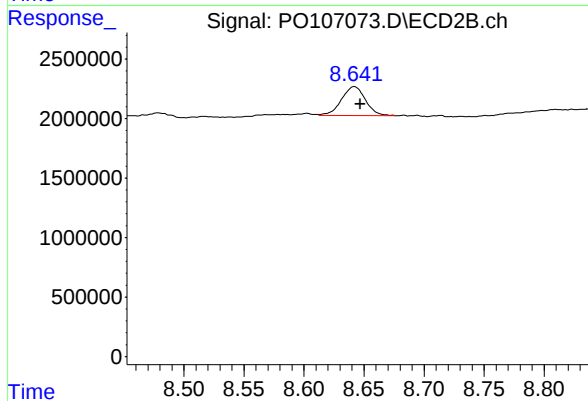

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: -0.006 min
Response: 3358561
Conc: 1.20 ng/ml m