

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101118\
 Data File : PO049911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2018 14:15
 Operator : SM/SJ
 Sample : J5326-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FL-PIT-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 14:43:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.368	3.546	6269921	6013793	27.736	24.934
2) SA Decachlor...	10.054	8.423	5655297	3779332	16.973	14.449

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101118\
Data File : PO049911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2018 14:15
Operator : SM/SJ
Sample : J5326-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FL-PIT-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 14:43:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

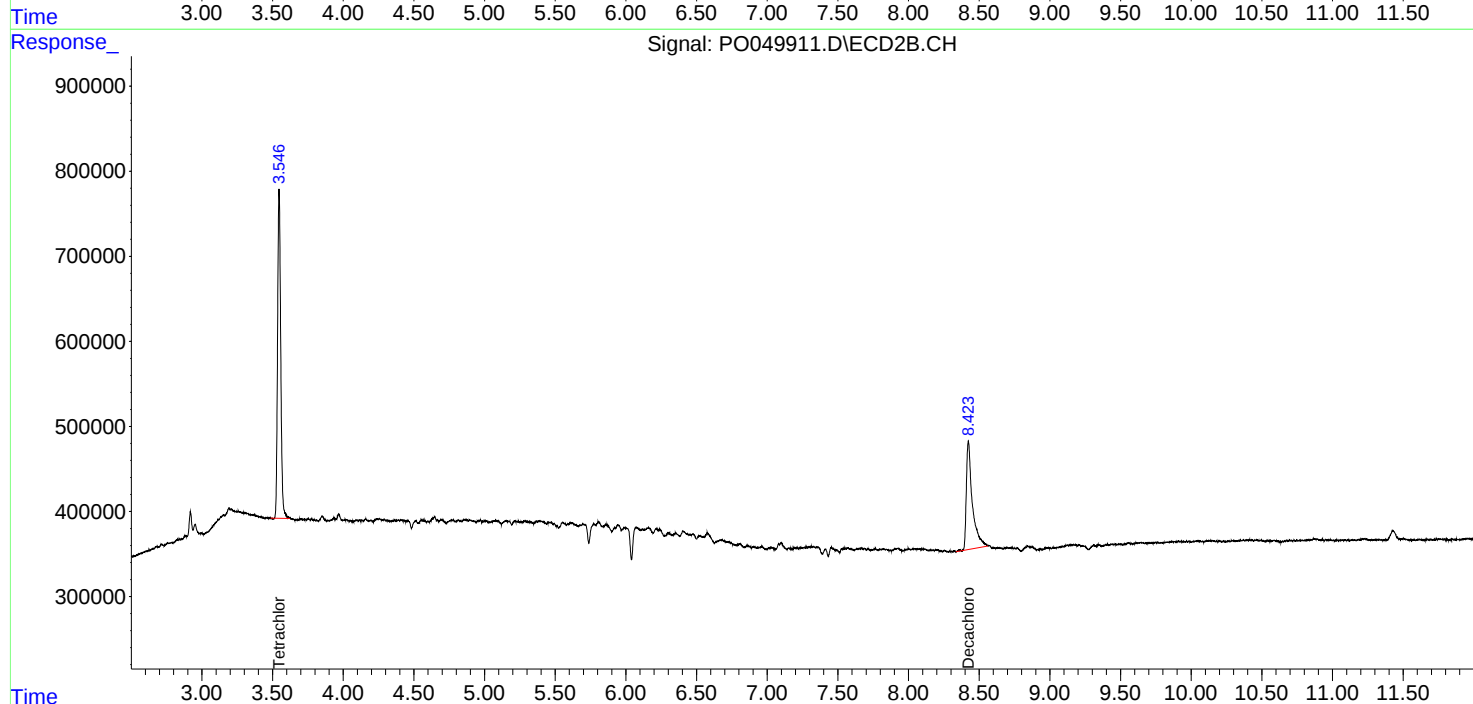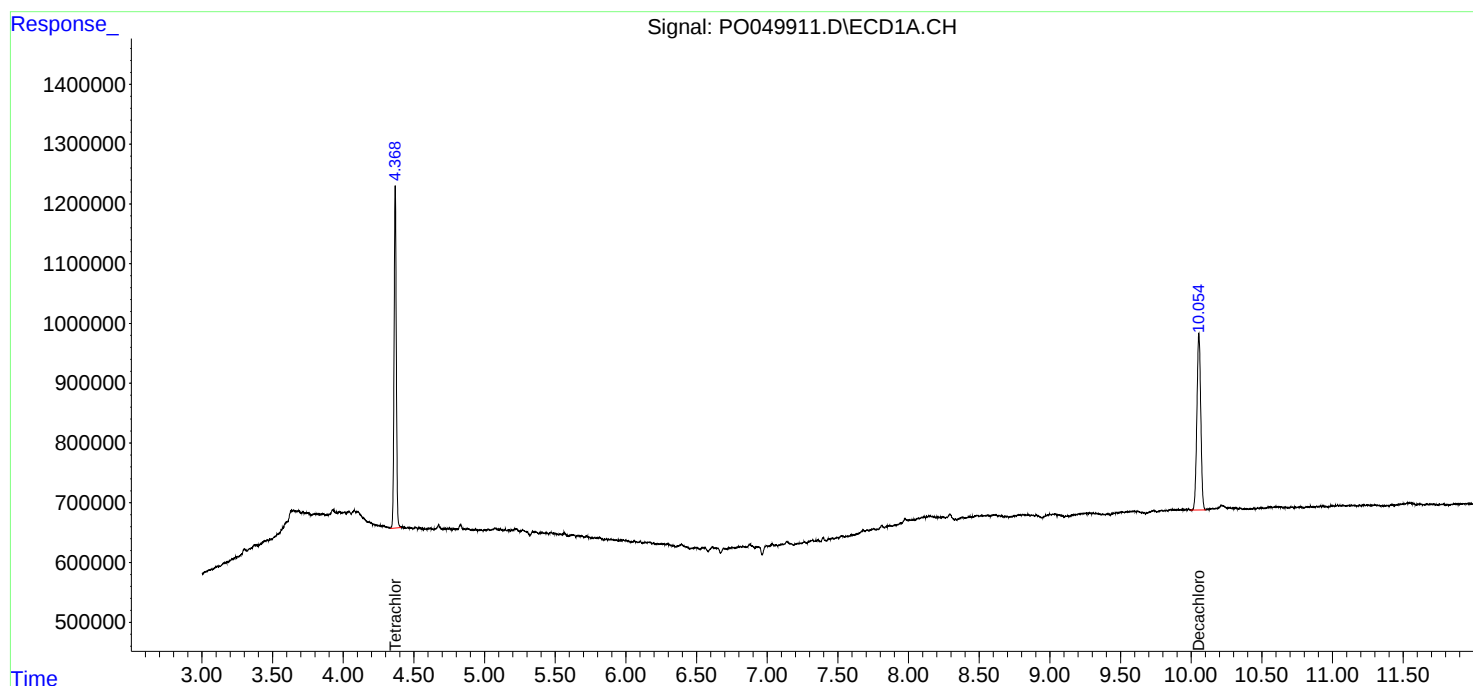


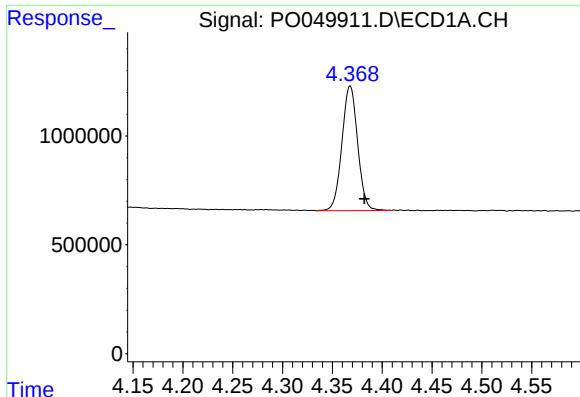

#1 Tetrachloro-m-xylene


R.T.: 4.368 min
Delta R.T.: -0.014 min
Response: 6269921
Conc: 27.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
FL-PIT-2

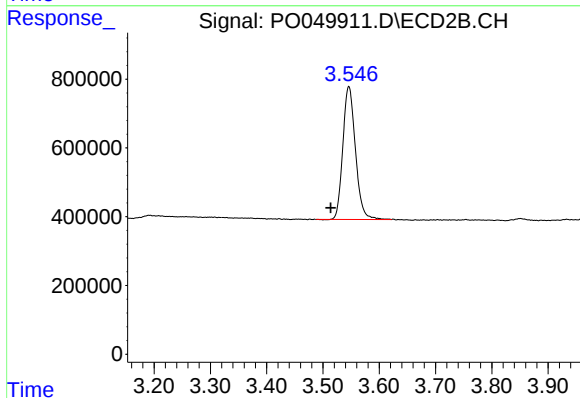


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.032 min
Response: 6013793
Conc: 24.93 ng/ml

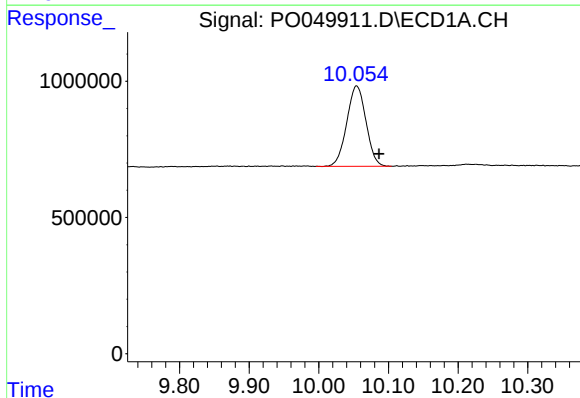

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: -0.033 min
Response: 5655297
Conc: 16.97 ng/ml

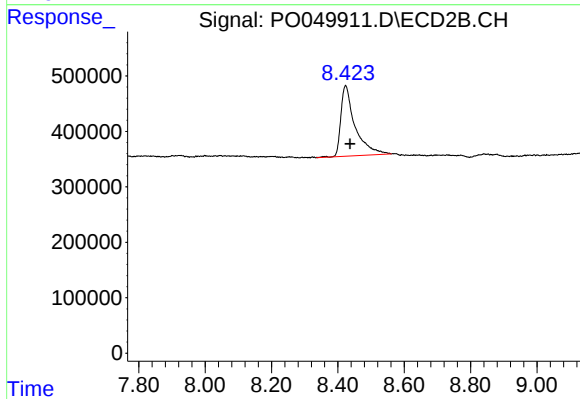

#2 Decachlorobiphenyl

R.T.: 8.423 min
Delta R.T.: -0.013 min
Response: 3779332
Conc: 14.45 ng/ml