

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101118\
 Data File : PO049919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2018 16:48
 Operator : SM/SJ
 Sample : J5367-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DS-VB-16202

Manual Integrations
 APPROVED

Sohil
 10/12/2018 1:38:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 11 17:14:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 08 15:27:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.363	3.544	5834760	5380148	25.811	22.307m
2) SA Decachlor...	10.045	8.414	2978930	1623738	8.940m	6.208 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101118\
Data File : P0049919.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2018 16:48
Operator : SM/SJ
Sample : J5367-01
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
DS-VB-16202


Manual Integrations
APPROVED

Sohil
10/12/2018 1:38:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 11 17:14:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100818.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 08 15:27:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

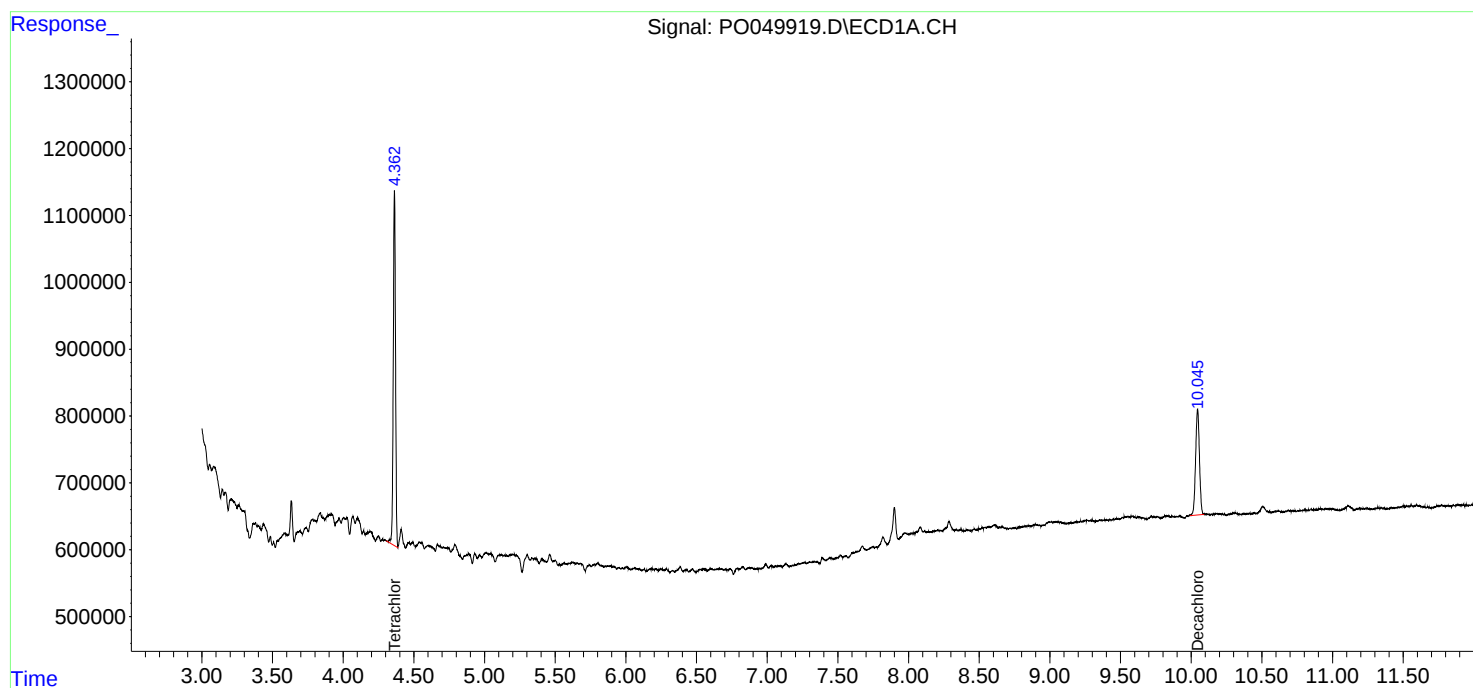

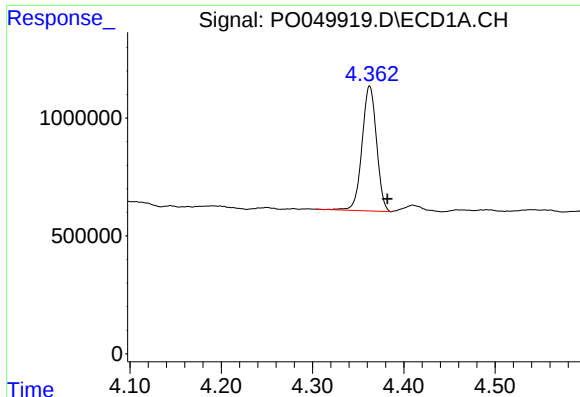


#1 Tetrachloro-m-xylene

R.T.: 4.363 min
Delta R.T.: -0.019 min
Response: 5834760
Conc: 25.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
DS-VB-16202


Manual Integrations
APPROVED

Sohil
10/12/2018 1:38:00 PM

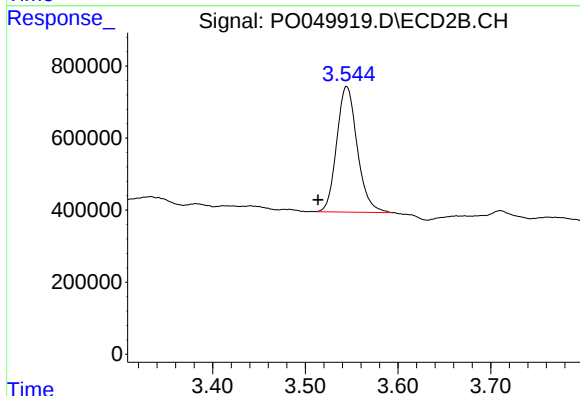


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: 0.030 min
Response: 5380148
Conc: 22.31 ng/ml m

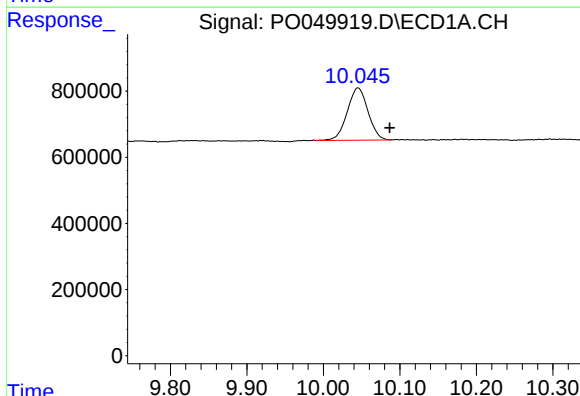

#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.042 min
Response: 2978930
Conc: 8.94 ng/ml m

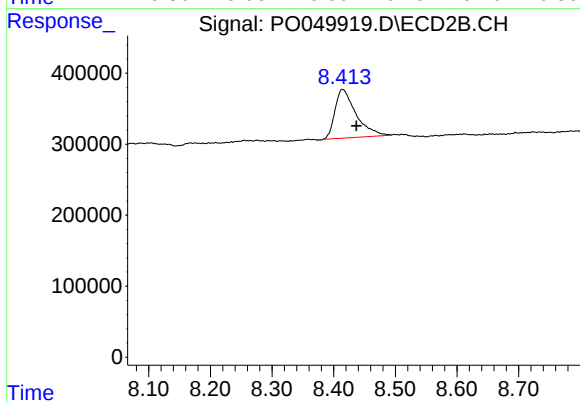

#2 Decachlorobiphenyl

R.T.: 8.414 min
Delta R.T.: -0.023 min
Response: 1623738
Conc: 6.21 ng/ml