

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101121\
 Data File : PO081994.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2021 23:51
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 02:40:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.987	3.976	1486034	637729	17.908	25.202 #
2)	SA Decachlor...	11.110	9.301f	1044255	626825	17.605	26.534 #
Target Compounds							
8)	L2 AR-1221-1	5.238	0.000	50224	0	52.591	N.D. #
9)	L2 AR-1221-2	5.342	0.000	21824	0	33.803	N.D. #
24)	L5 AR-1248-4	7.241f	0.000	28135	0	10.751	N.D. #
26)	L6 AR-1254-1	7.241	0.000	28135	0	10.285	N.D. #
28)	L6 AR-1254-3	7.871f	0.000	24969	0	6.119	N.D. #
32)	L7 AR-1260-2	8.308f	0.000	15190	0	4.113	N.D. #
33)	L7 AR-1260-3	0.000	7.188	0	23556	N.D.	14.404 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101121\
Data File : PO081994.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2021 23:51
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 02:40:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

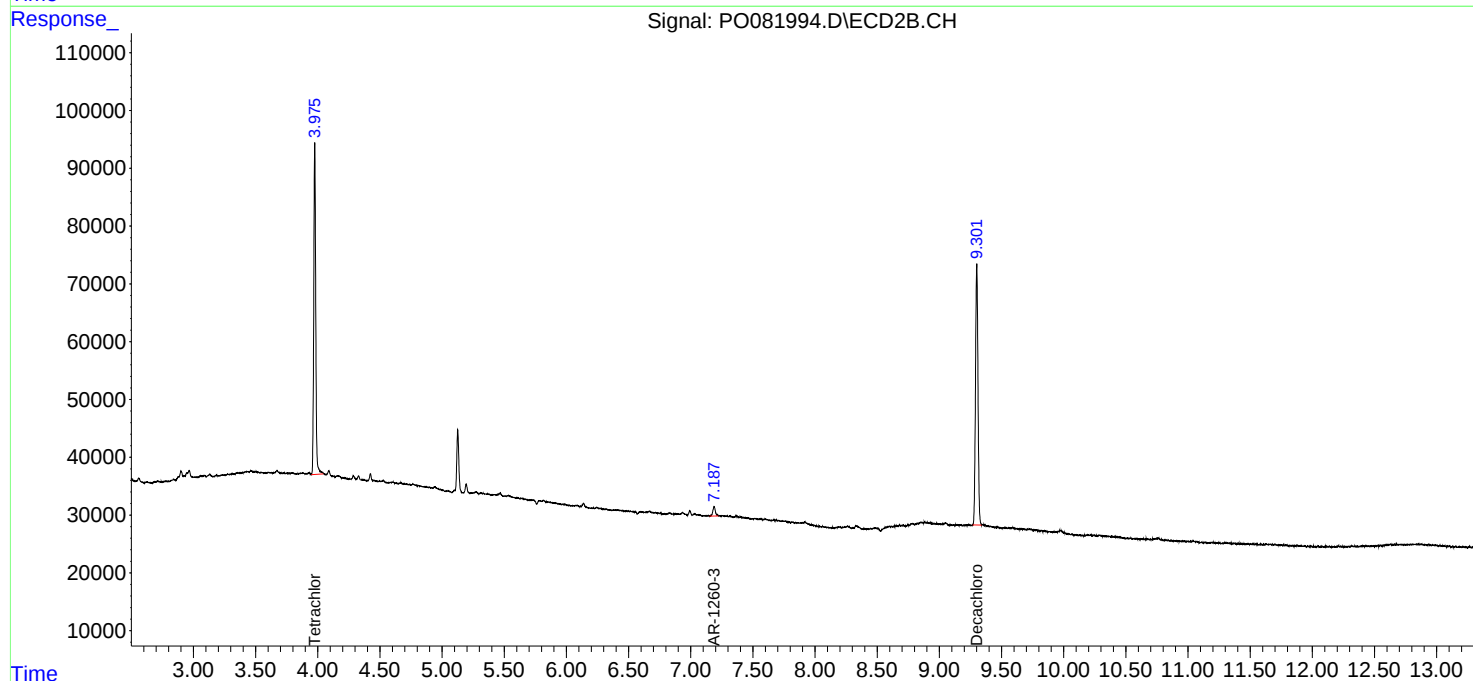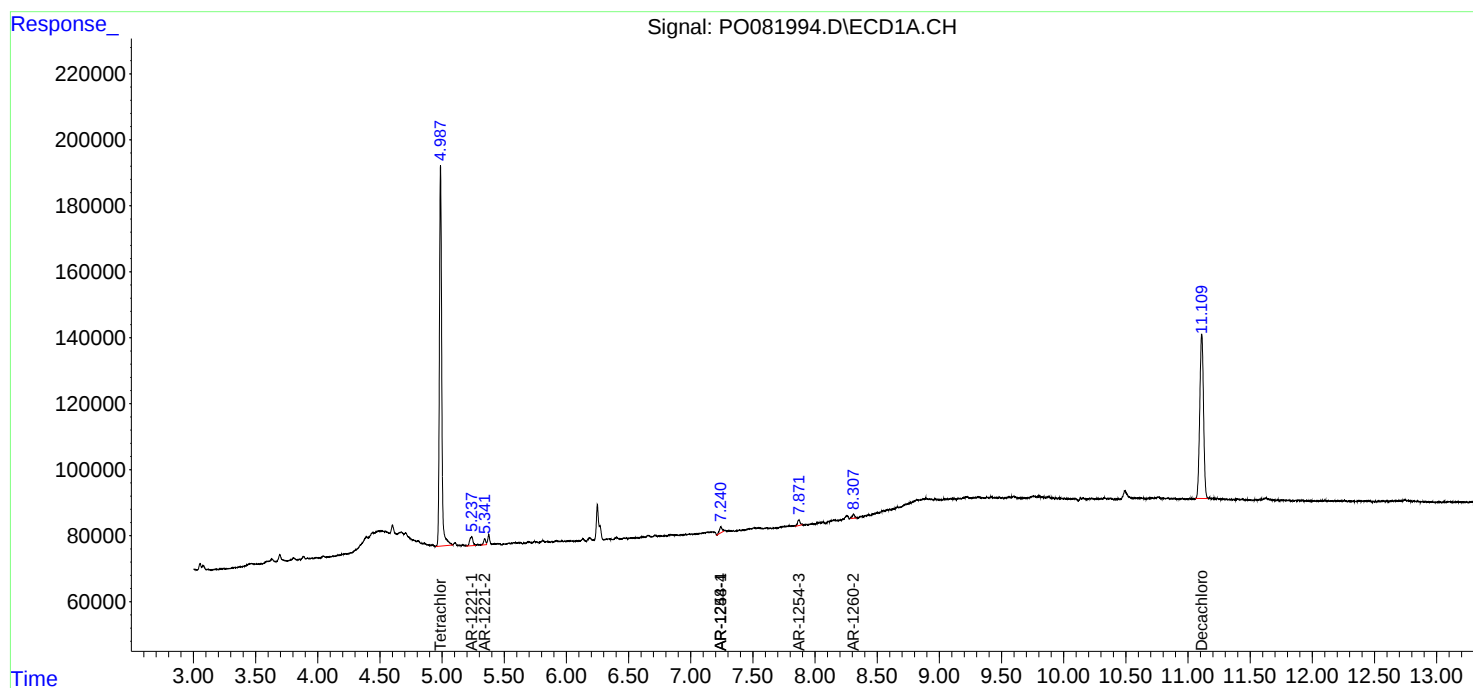


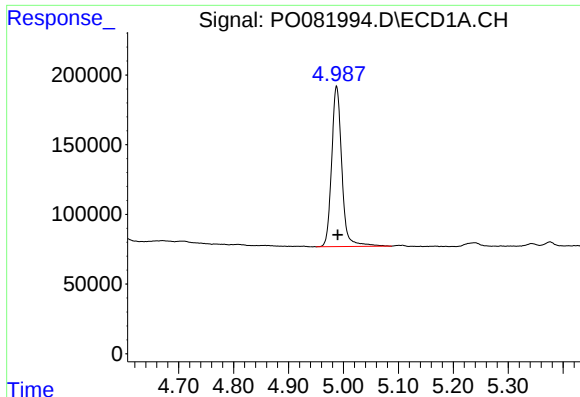

#1 Tetrachloro-m-xylene


R.T.: 4.987 min
Delta R.T.: -0.003 min
Response: 1486034
Conc: 17.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

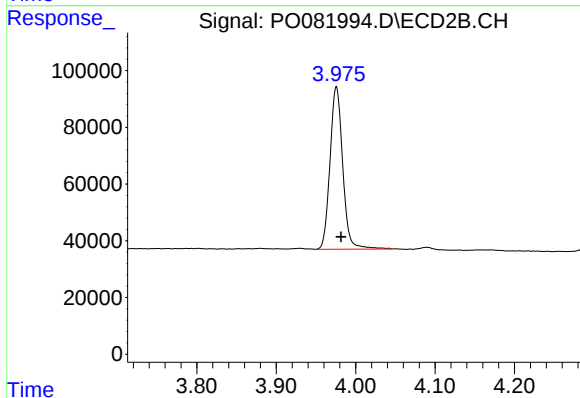


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.006 min
Response: 637729
Conc: 25.20 ng/ml

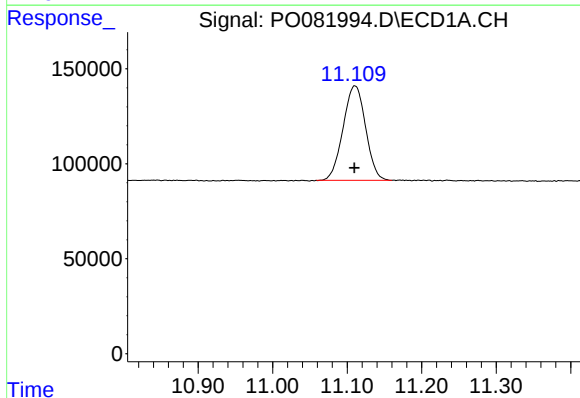


#2 Decachlorobiphenyl

R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 1044255
Conc: 17.61 ng/ml

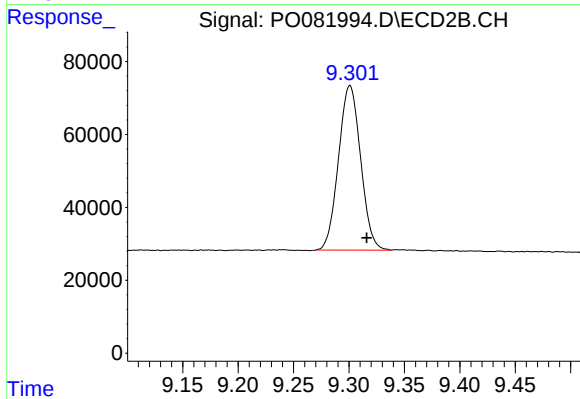

#2 Decachlorobiphenyl


R.T.: 9.301 min
Delta R.T.: -0.015 min
Response: 626825
Conc: 26.53 ng/ml

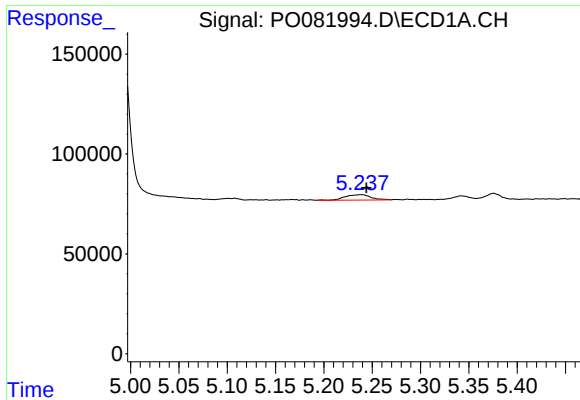

#8 AR-1221-1


R.T.: 5.238 min
Delta R.T.: -0.006 min
Response: 50224
Conc: 52.59 ng/ml

Instrument :
ECD_O
ClientSampleId :

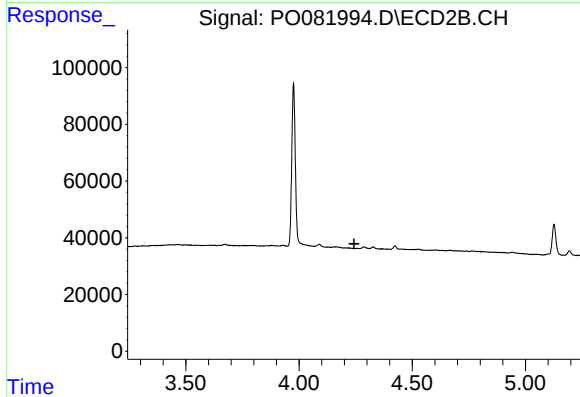


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.243 min
Response: 0
Conc: N.D.

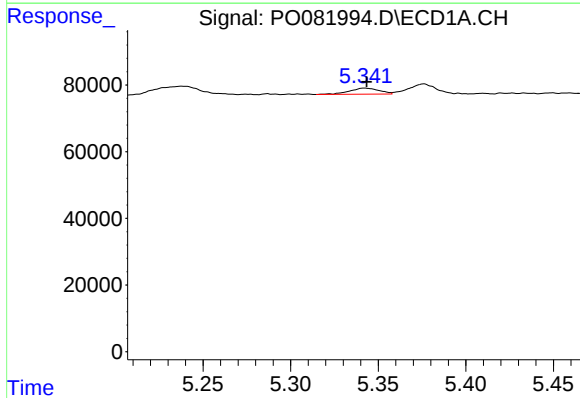


#9 AR-1221-2

R.T.: 5.342 min
Delta R.T.: -0.001 min
Response: 21824
Conc: 33.80 ng/ml

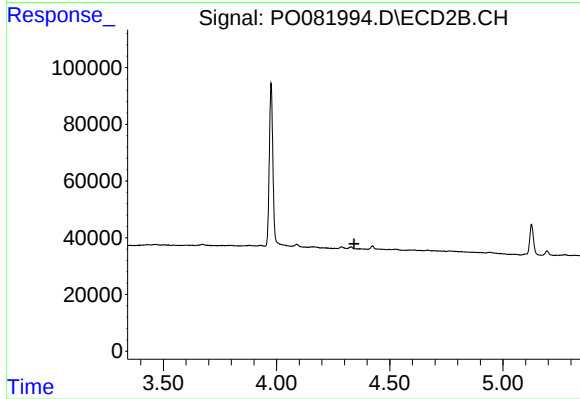

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.342 min
Response: 0
Conc: N.D.

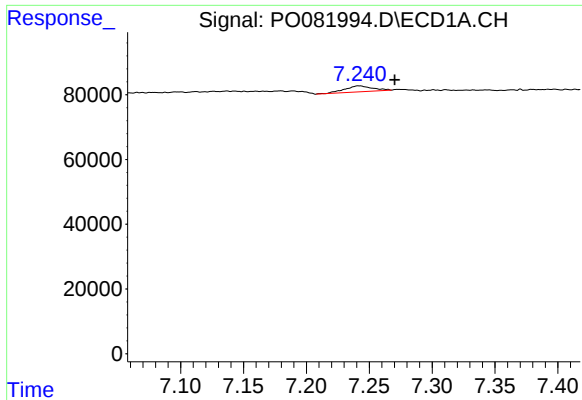

#24 AR-1248-4


R.T.: 7.241 min
Delta R.T.: -0.029 min
Response: 28135
Conc: 10.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

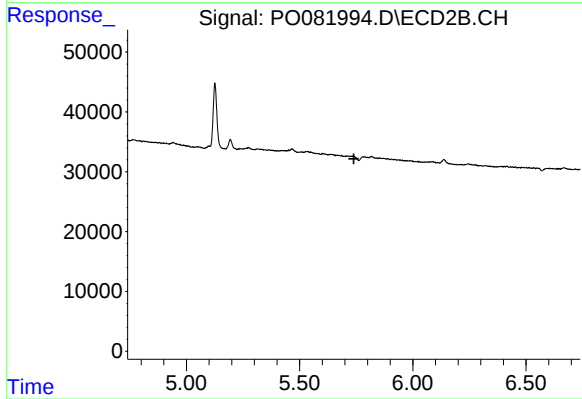


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.739 min
Response: 0
Conc: N.D.

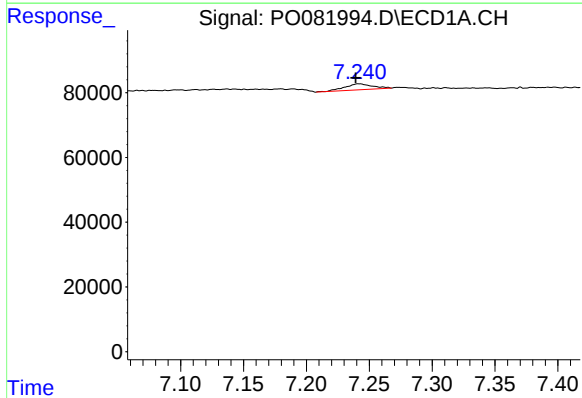


#26 AR-1254-1

R.T.: 7.241 min
Delta R.T.: 0.002 min
Response: 28135
Conc: 10.28 ng/ml

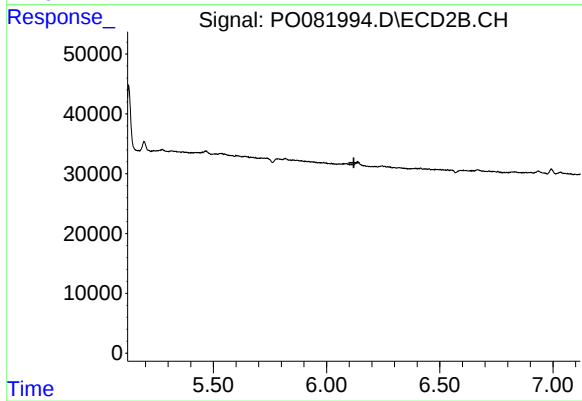

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

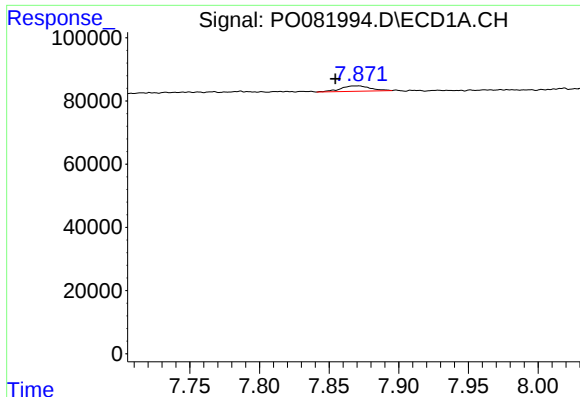

#28 AR-1254-3


R.T.: 7.871 min
Delta R.T.: 0.017 min
Response: 24969
Conc: 6.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

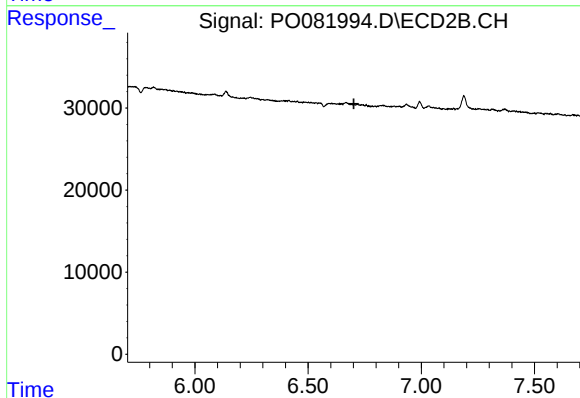


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.702 min
Response: 0
Conc: N.D.

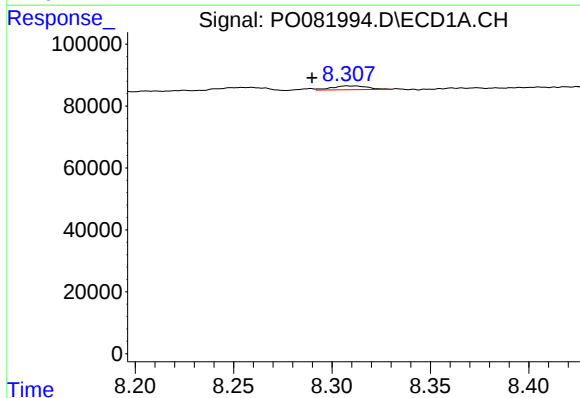


#32 AR-1260-2

R.T.: 8.308 min
Delta R.T.: 0.018 min
Response: 15190
Conc: 4.11 ng/ml

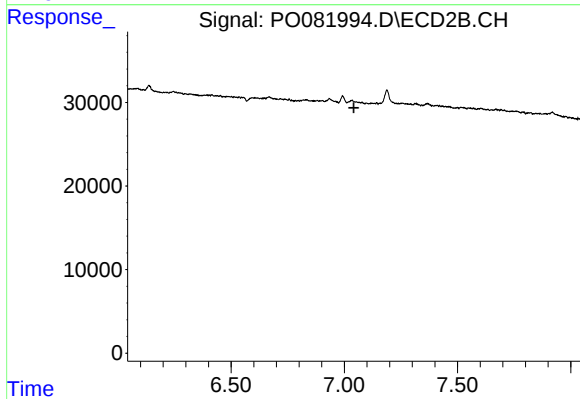

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.042 min
Response: 0
Conc: N.D.

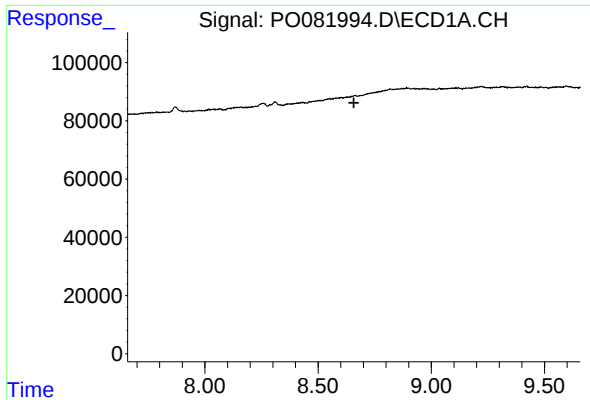

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

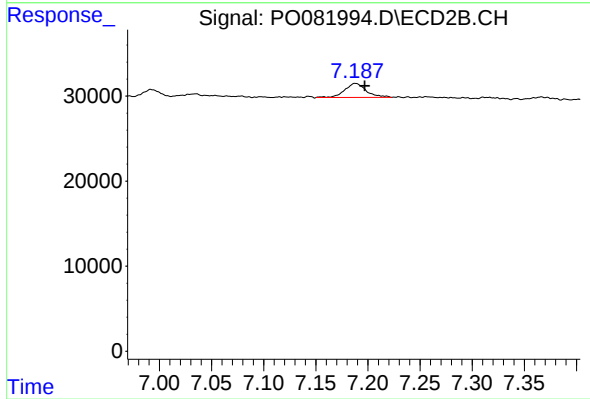

#33 AR-1260-3

R.T.: 7.188 min
Delta R.T.: -0.009 min
Response: 23556
Conc: 14.40 ng/ml