

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101121\
 Data File : PO081969.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Oct 2021 15:47
 Operator : AJ\MA
 Sample : M4164-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BU-03-100821

Manual Integrations
 APPROVED

mohammad
 10/13/2021 8:54:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 12 02:23:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 07 09:43:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.989	3.977	1509766	591685	18.194	23.383 #
2) SA Decachlor...	11.112	9.305	1060351	487726	17.877m	20.646

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101121\
Data File : P0081969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Oct 2021 15:47
Operator : AJ\MA
Sample : M4164-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BU-03-100821


Manual Integrations
APPROVED

mohammad
10/13/2021 8:54:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 12 02:23:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 07 09:43:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

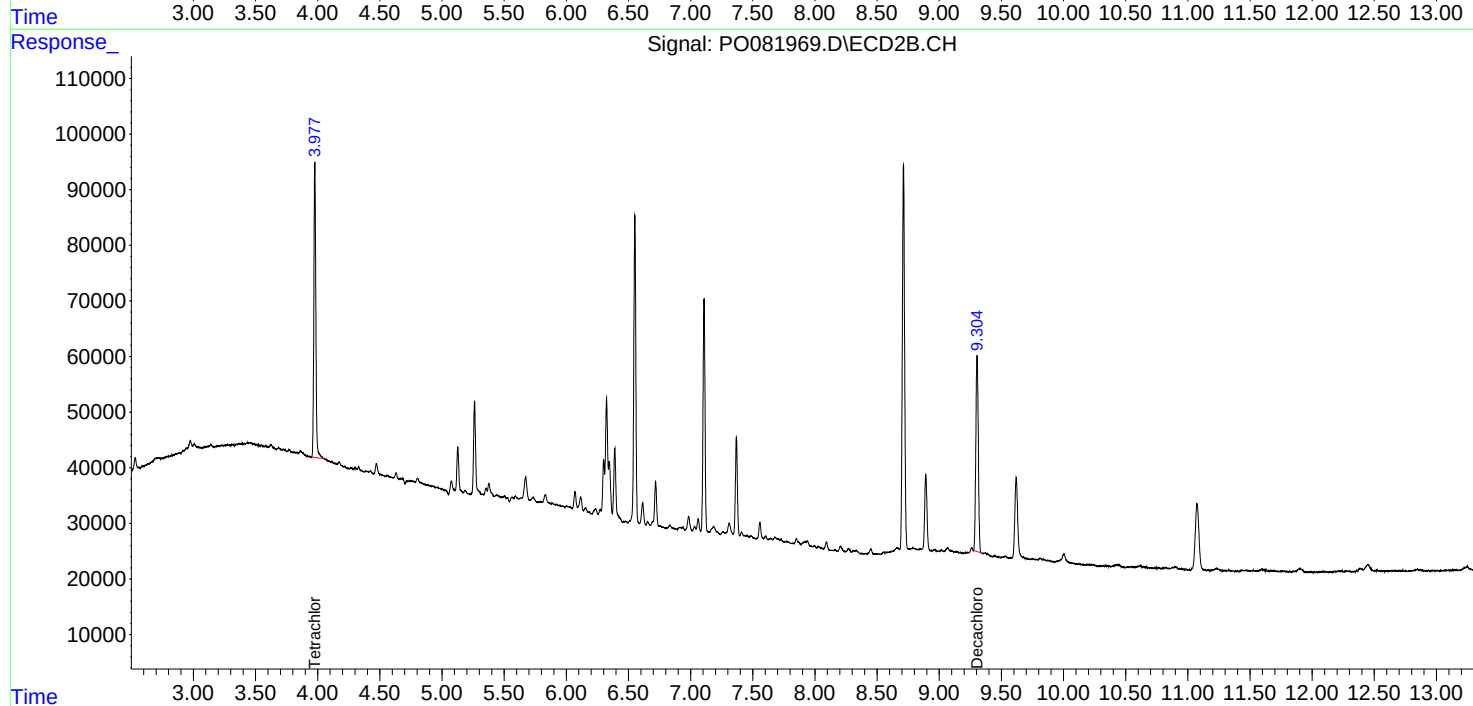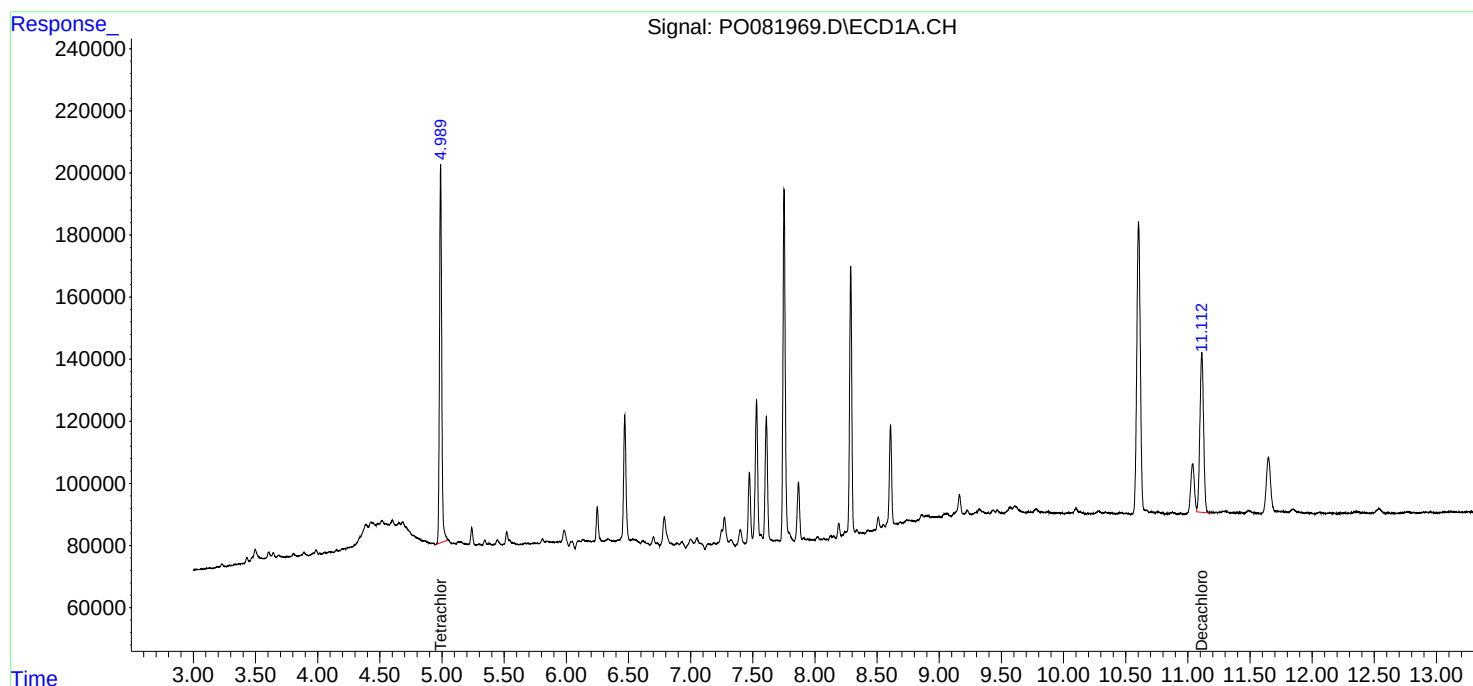

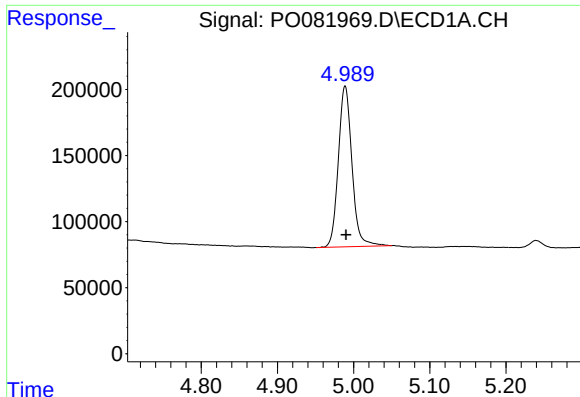


#1 Tetrachloro-m-xylene

R.T.: 4.989 min
Delta R.T.: -0.001 min
Response: 1509766
Conc: 18.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
BU-03-100821


Manual Integrations
APPROVED

mohammad
10/13/2021 8:54:56 AM

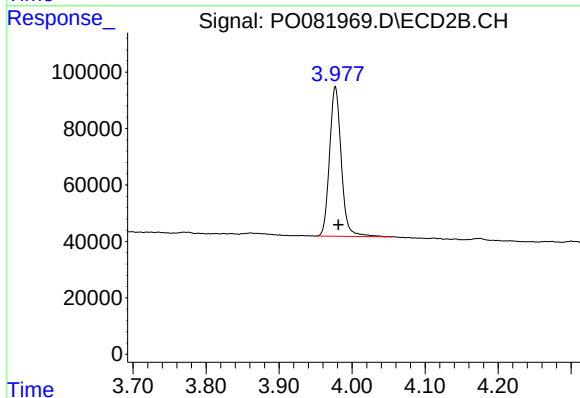


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 591685
Conc: 23.38 ng/ml

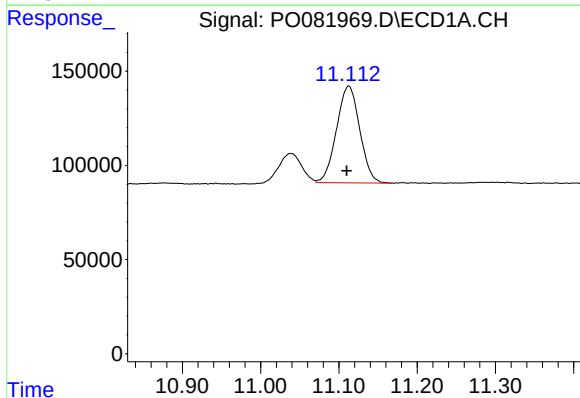

#2 Decachlorobiphenyl

R.T.: 11.112 min
Delta R.T.: 0.002 min
Response: 1060351
Conc: 17.88 ng/ml m

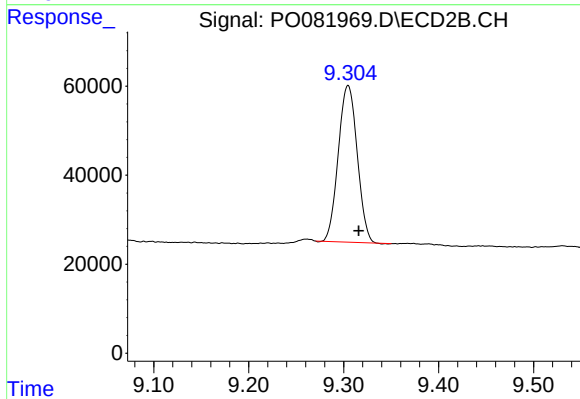

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: -0.011 min
Response: 487726
Conc: 20.65 ng/ml