

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101218\
 Data File : P0049952.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2018 1:08
 Operator : SM/SJ
 Sample : J5296-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100418-SIDI-E-U-M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 04:29:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101218.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 13 01:14:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.350	3.367	3632596	3089253	25.815	18.248 #
2)	SA Decachlor...	10.048	8.133	2614269	2543552	25.390	21.671

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101218\
Data File : P0049952.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2018 1:08
Operator : SM/SJ
Sample : J5296-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
100418-SIDI-E-U-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 04:29:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101218.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 13 01:14:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

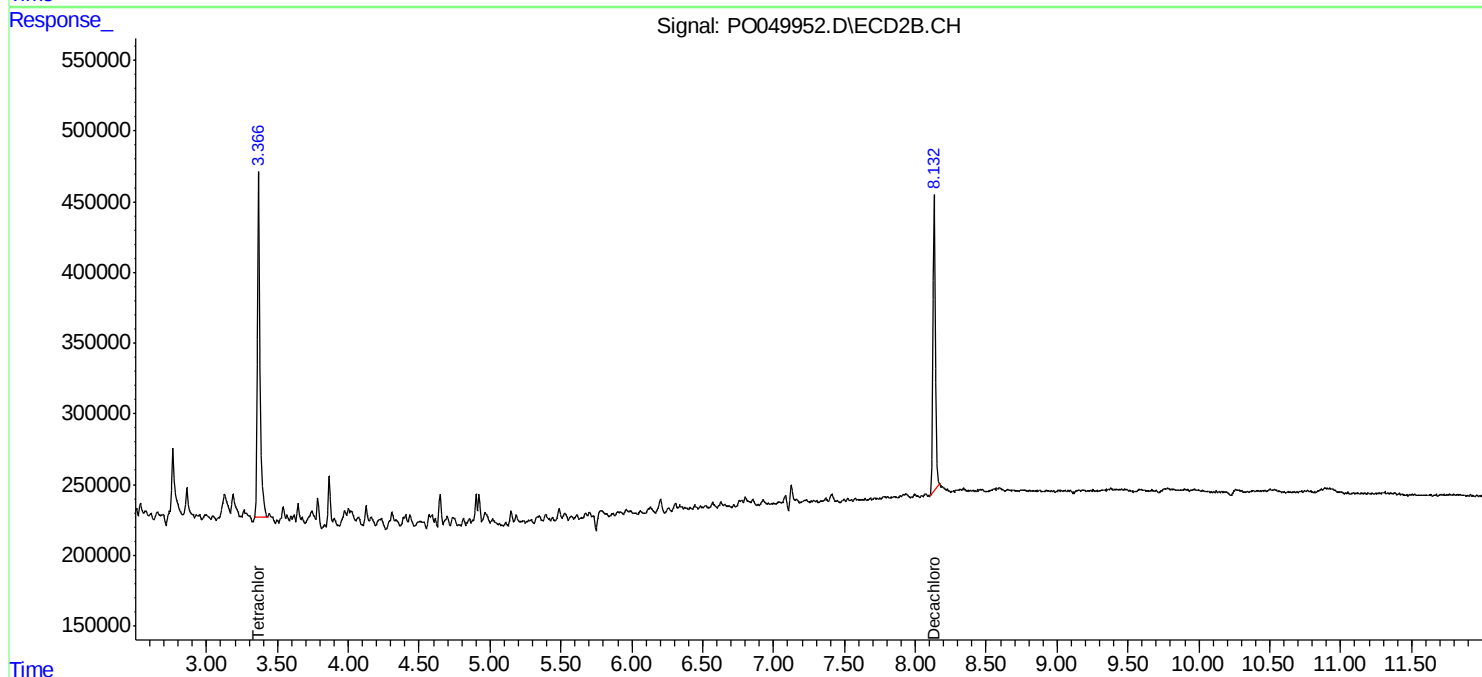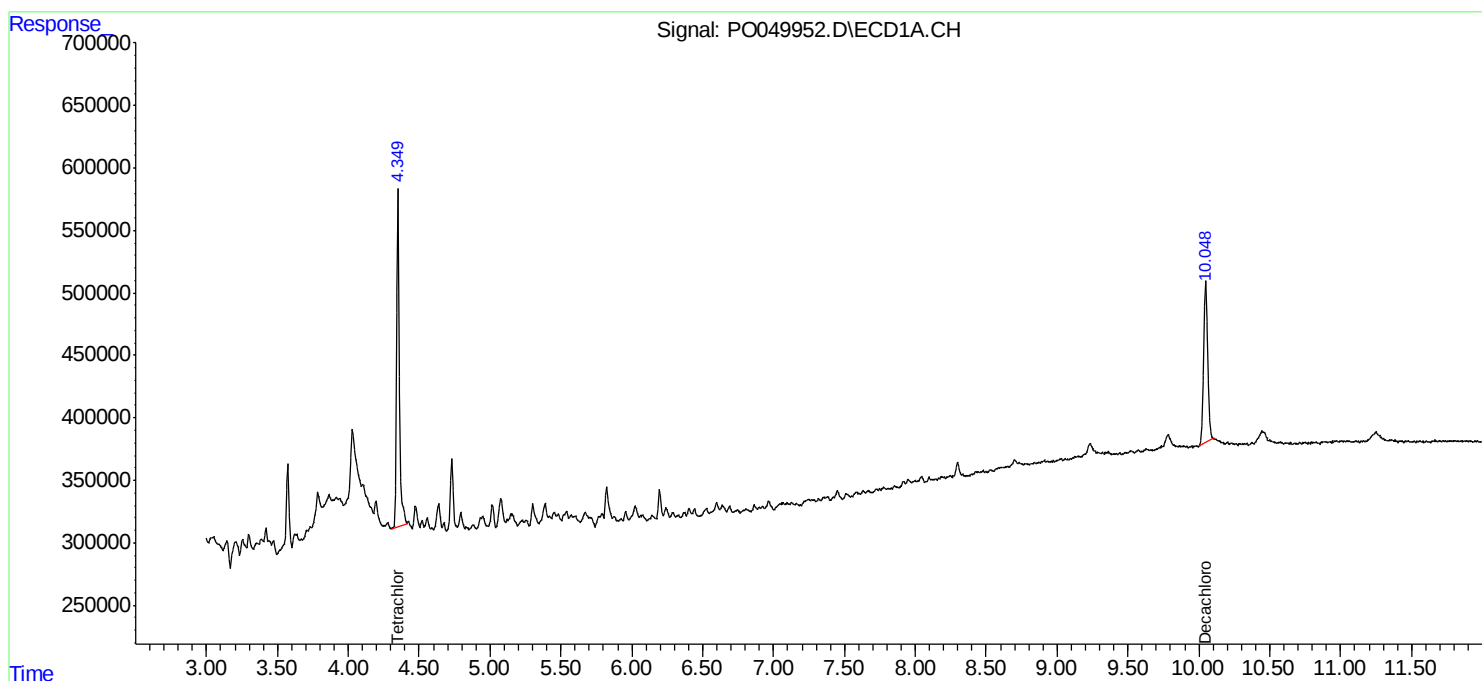


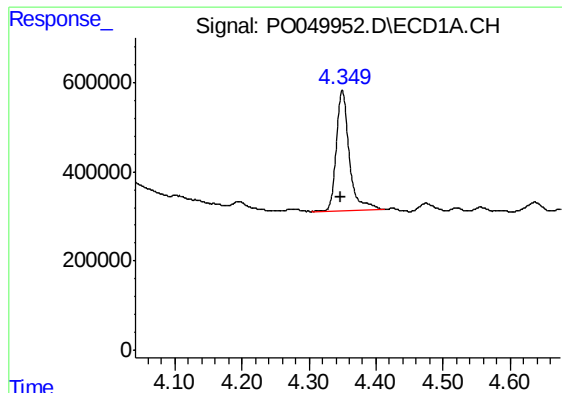

#1 Tetrachloro-m-xylene


R.T.: 4.350 min
Delta R.T.: 0.002 min
Response: 3632596
Conc: 25.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
100418-SIDI-E-U-M

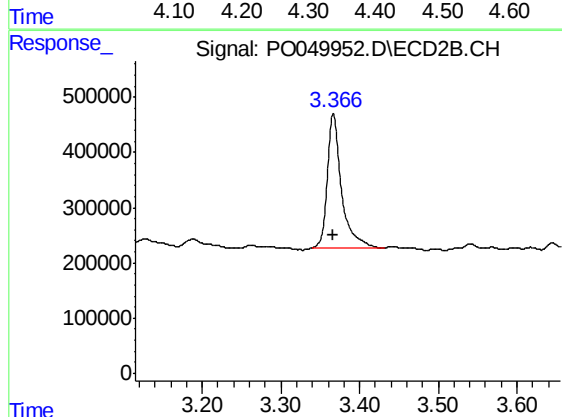


#1 Tetrachloro-m-xylene

R.T.: 3.367 min
Delta R.T.: 0.000 min
Response: 3089253
Conc: 18.25 ng/ml

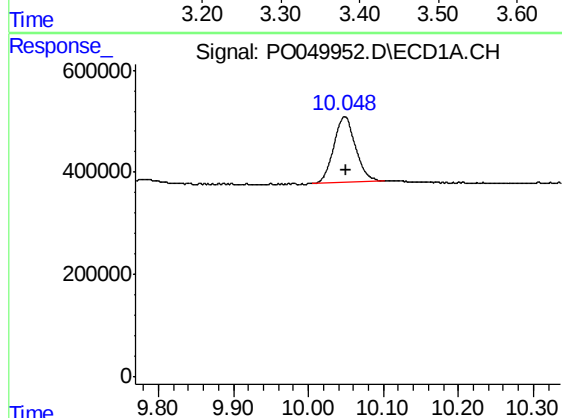

#2 Decachlorobiphenyl

R.T.: 10.048 min
Delta R.T.: -0.003 min
Response: 2614269
Conc: 25.39 ng/ml

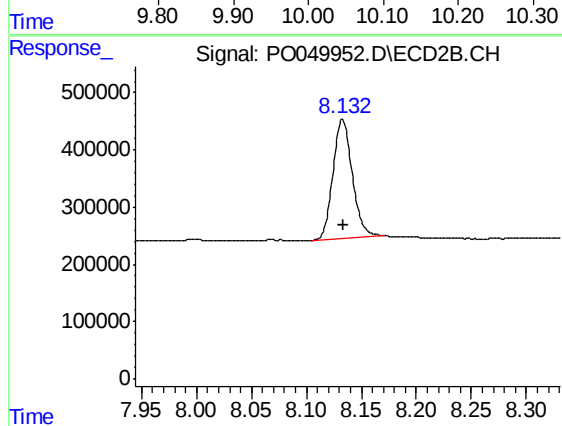

#2 Decachlorobiphenyl

R.T.: 8.133 min
Delta R.T.: -0.001 min
Response: 2543552
Conc: 21.67 ng/ml