

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101218\
 Data File : P0049969.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2018 8:05
 Operator : SM/SJ
 Sample : J5383-05
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100918-SIDI-F-U-M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 03:44:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101218.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 13 01:14:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.352	3.366	3730536	2934289	26.511	17.333 #
2)	SA Decachlor...	10.061	8.132	3048323	2601463	29.606	22.165 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101218\
Data File : PO049969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2018 8:05
Operator : SM/SJ
Sample : J5383-05
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
100918-SIDI-F-U-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 03:44:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101218.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 13 01:14:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

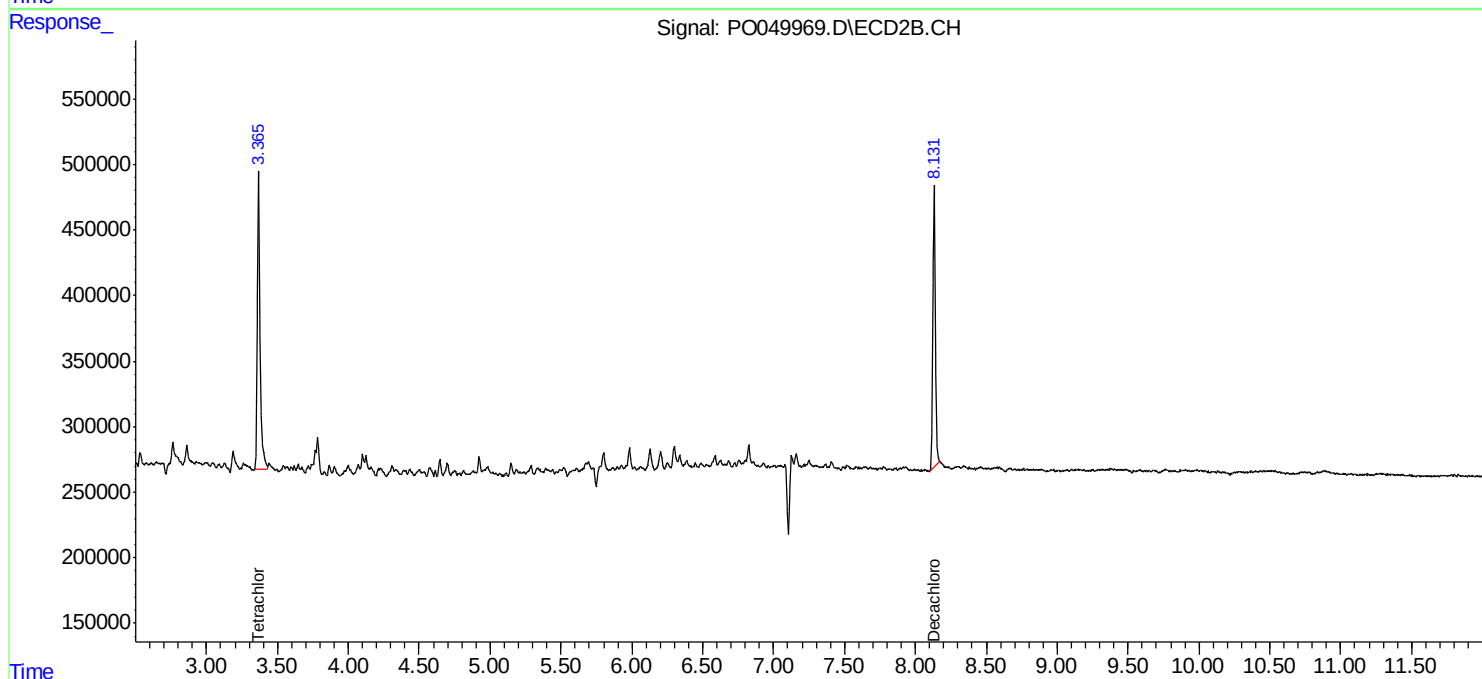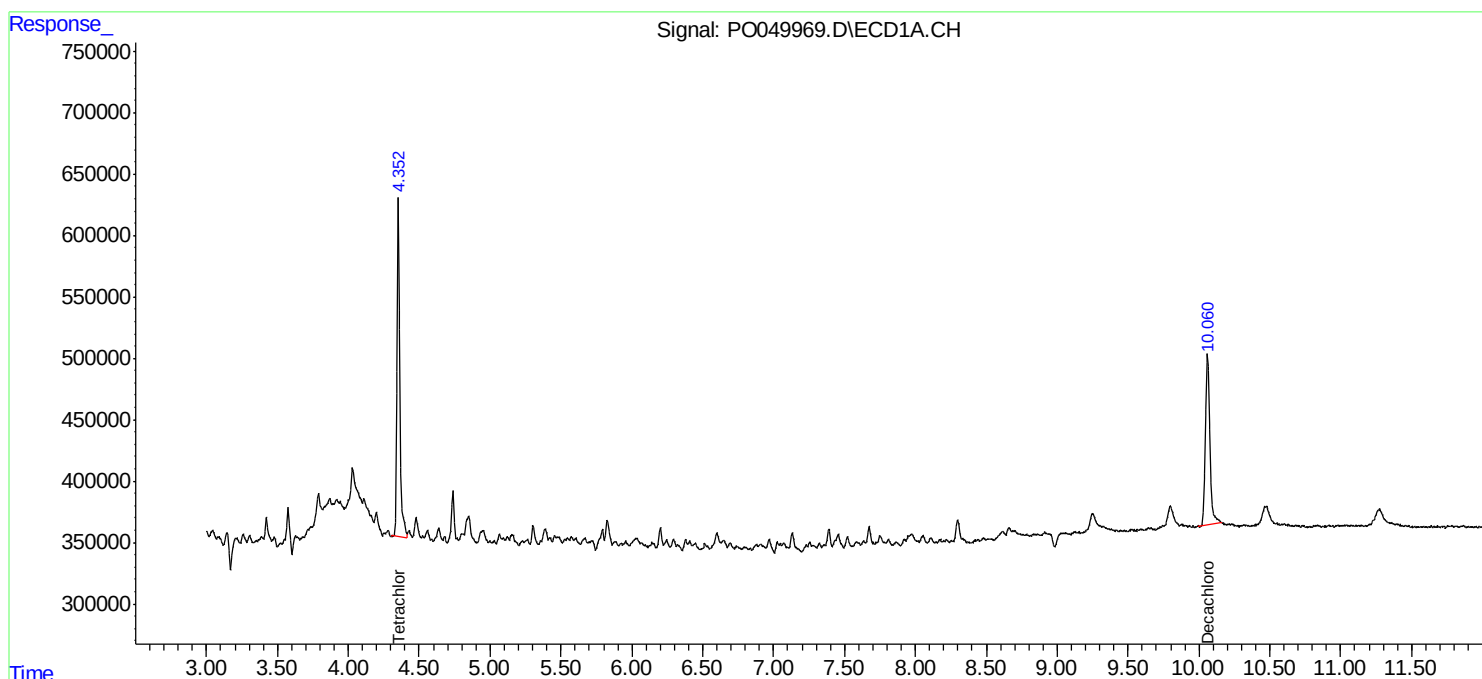


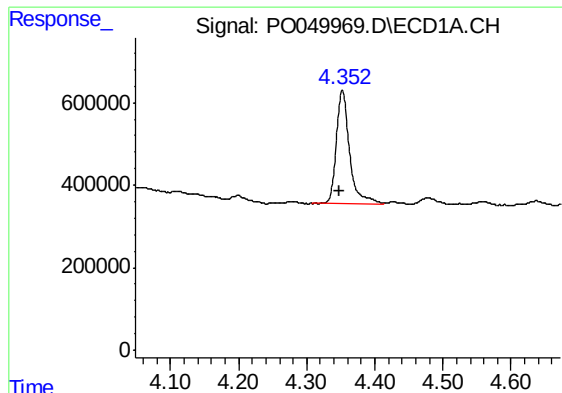

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: 0.004 min
Response: 3730536
Conc: 26.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
100918-SIDI-F-U-M

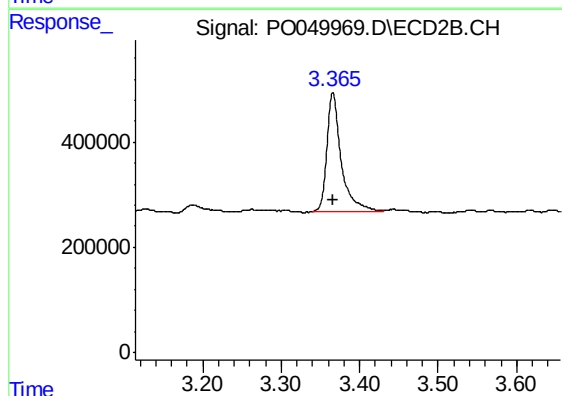


#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 2934289
Conc: 17.33 ng/ml

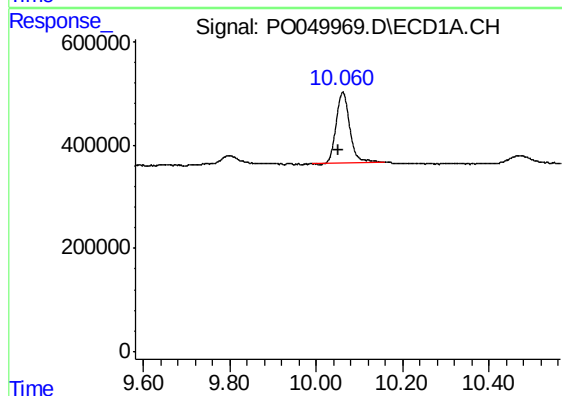

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: 0.010 min
Response: 3048323
Conc: 29.61 ng/ml

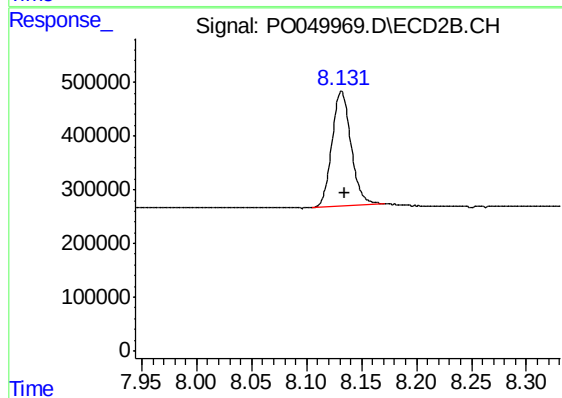

#2 Decachlorobiphenyl

R.T.: 8.132 min
Delta R.T.: -0.002 min
Response: 2601463
Conc: 22.16 ng/ml