

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101218\
 Data File : P0050002.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2018 19:14
 Operator : SM/SJ
 Sample : PB113727BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB113727BL

Manual Integrations
 APPROVED

Sohil
 10/15/2018 11:24:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 04:02:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101218.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 13 01:14:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.346	3.366	4169462	3210315	29.630	18.963 #
2)	SA Decachlor...	10.156f	8.129	3109096	2880995	30.196m	24.546

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101218\
Data File : PO050002.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2018 19:14
Operator : SM/SJ
Sample : PB113727BL
Misc :
ALS Vial : 73 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB113727BL


Manual Integrations
APPROVED

Sohil
10/15/2018 11:24:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 04:02:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101218.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 13 01:14:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

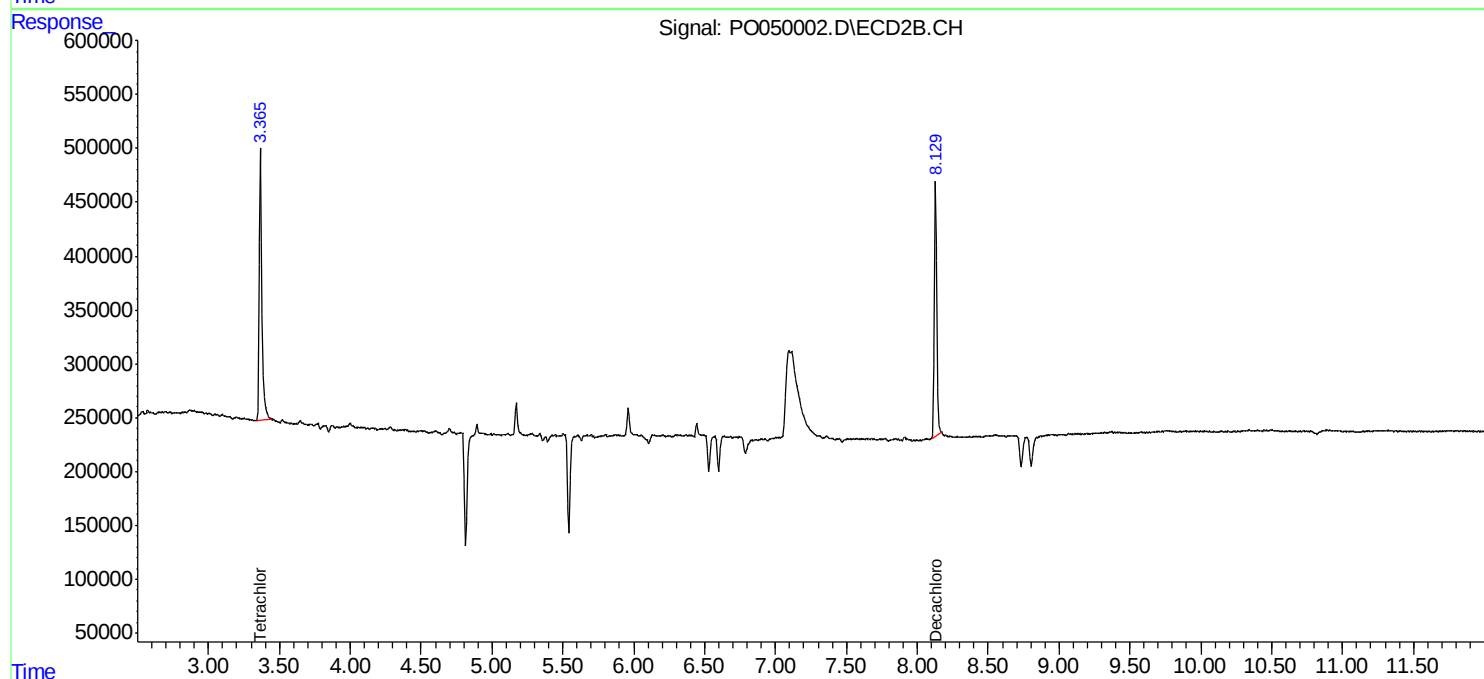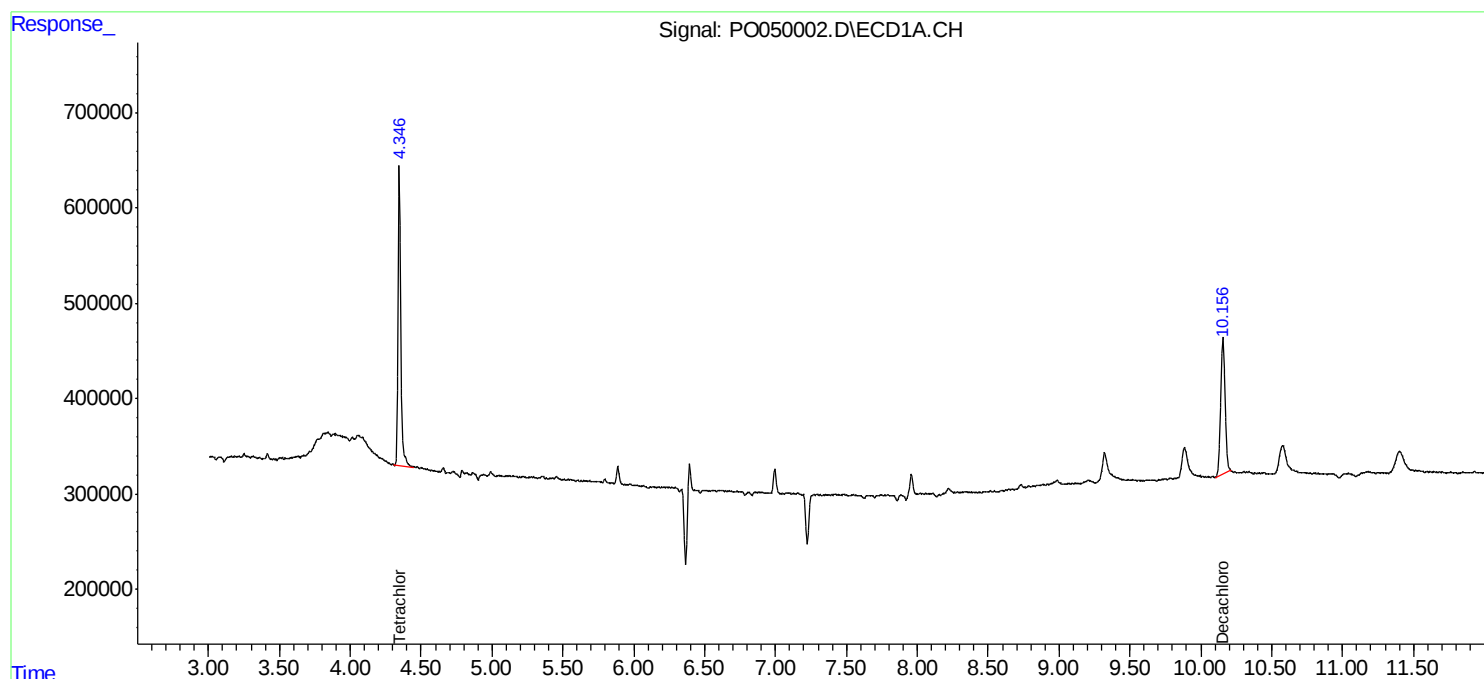

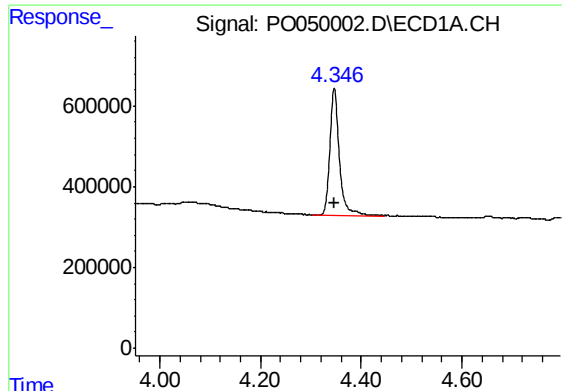


#1 Tetrachloro-m-xylene

R.T.: 4.346 min
Delta R.T.: -0.002 min
Response: 4169462
Conc: 29.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB113727BL


Manual Integrations
APPROVED

Sohil
10/15/2018 11:24:27 AM

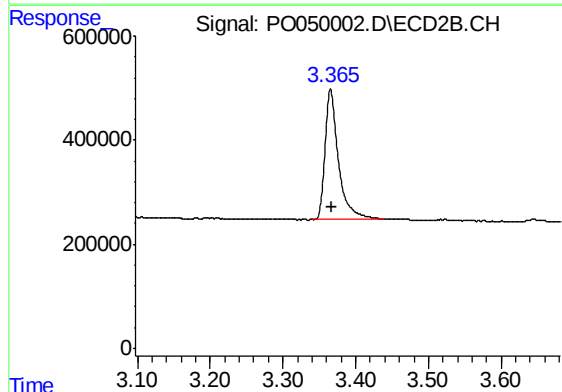


#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: -0.001 min
Response: 3210315
Conc: 18.96 ng/ml

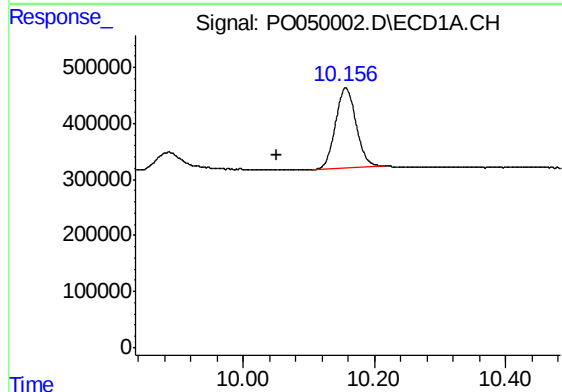

#2 Decachlorobiphenyl

R.T.: 10.156 min
Delta R.T.: 0.105 min
Response: 3109096
Conc: 30.20 ng/ml m

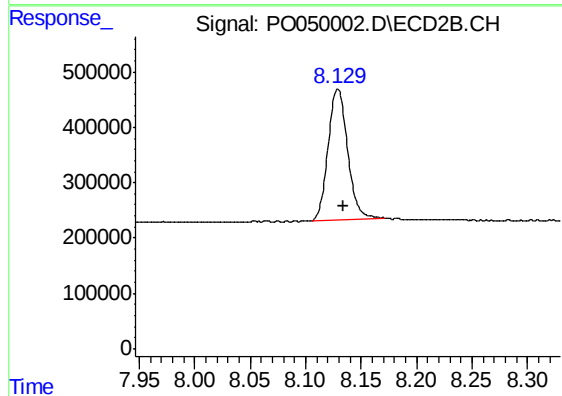

#2 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: -0.005 min
Response: 2880995
Conc: 24.55 ng/ml