

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101220\
 Data File : P0072296.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Oct 2020 19:42
 Operator : DD\AJ
 Sample : L4340-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A-2332-MH12

Manual Integrations
 APPROVED

Ankita
 10/13/2020 12:32:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 06:14:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.508	1721309	864936	23.965	23.092
2) SA Decachlor...	9.929	8.676	1541831	839049	14.003	14.751m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101220\
Data File : PO072296.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Oct 2020 19:42
Operator : DD\AJ
Sample : L4340-03
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
A-2332-MH12


Manual Integrations
APPROVED

Ankita
10/13/2020 12:32:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 06:14:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

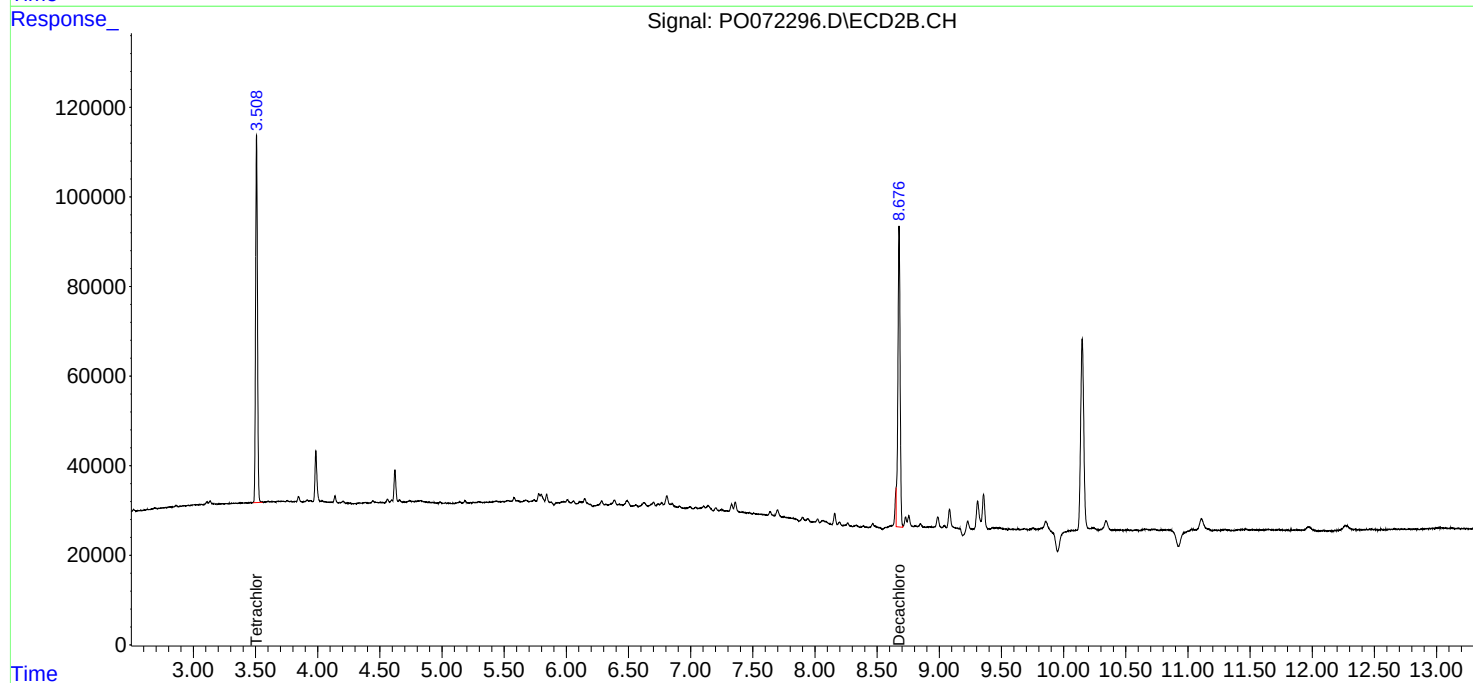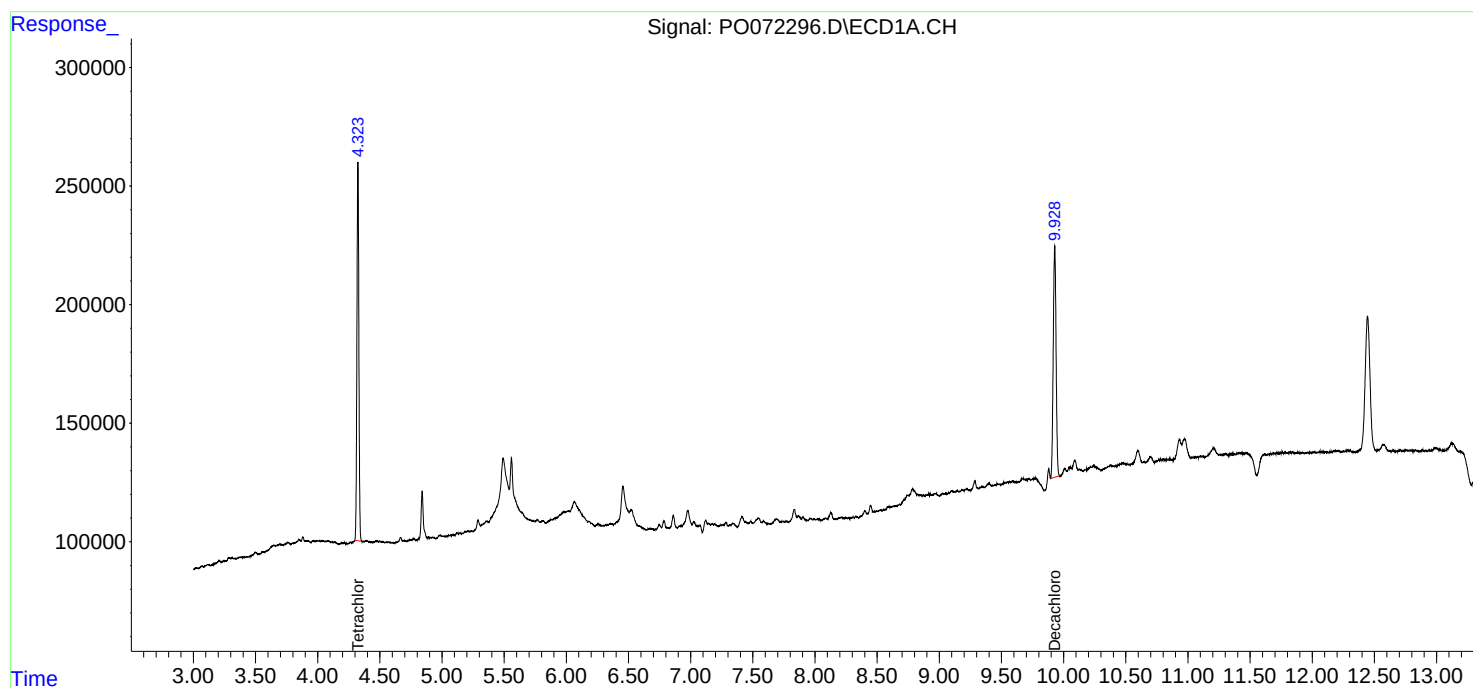

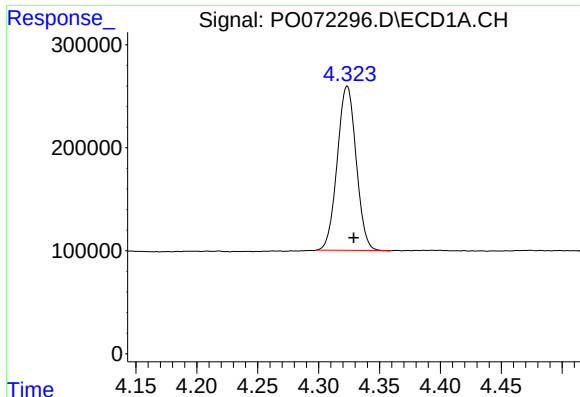


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.005 min
Response: 1721309
Conc: 23.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
A-2332-MH12


Manual Integrations
APPROVED

Ankita
10/13/2020 12:32:12 PM

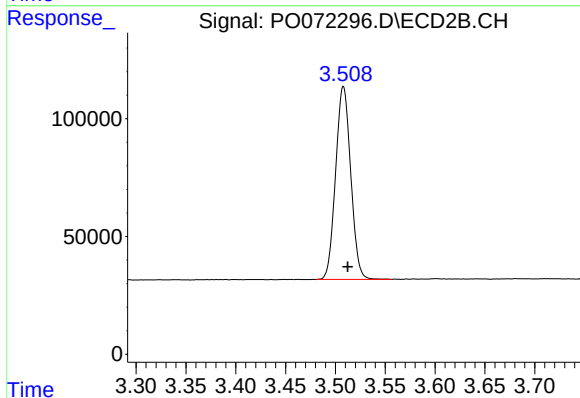


#1 Tetrachloro-m-xylene

R.T.: 3.508 min
Delta R.T.: -0.004 min
Response: 864936
Conc: 23.09 ng/ml

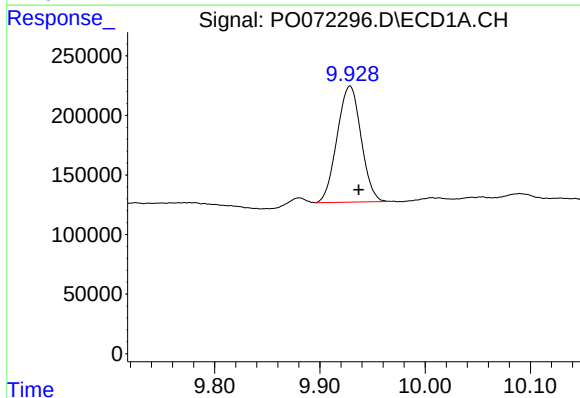

#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.008 min
Response: 1541831
Conc: 14.00 ng/ml

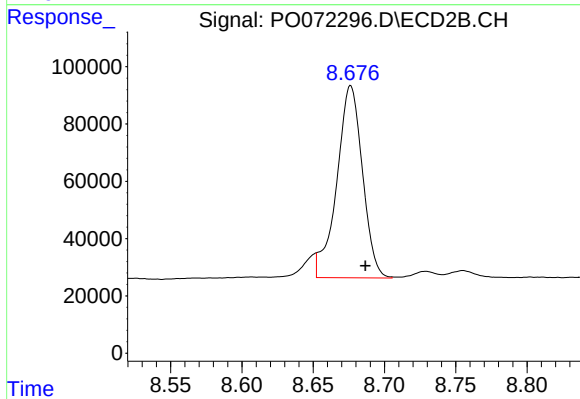

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.011 min
Response: 839049
Conc: 14.75 ng/ml m