

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101221\
 Data File : PO081996.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Oct 2021 15:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 06:42:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 06:41:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.987	3.975	1222241	575693	21.884	21.255
2)	SA Decachlor...	11.109	9.300	827481	525604	22.816	21.978
Target Compounds							
8)	L2 AR-1221-1	5.240	0.000	33765	0	48.902	N.D. #
9)	L2 AR-1221-2	5.345	0.000	16383	0	33.145	N.D. #
21)	L5 AR-1248-1	0.000	5.194f	0	20905	N.D.	30.535 #
27)	L6 AR-1254-2	7.458	0.000	9614	0	3.499	N.D. #
30)	L6 AR-1254-5	8.585	0.000	6138	0	2.753	N.D. #
32)	L7 AR-1260-2	8.310f	0.000	42422	0	17.032	N.D. #
33)	L7 AR-1260-3	8.641	7.186	10702	32521	6.302	18.768 #
36)	L8 AR-1262-1	8.671	0.000	10665	0	2.288	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101221\
Data File : P0081996.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Oct 2021 15:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 06:42:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 06:41:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

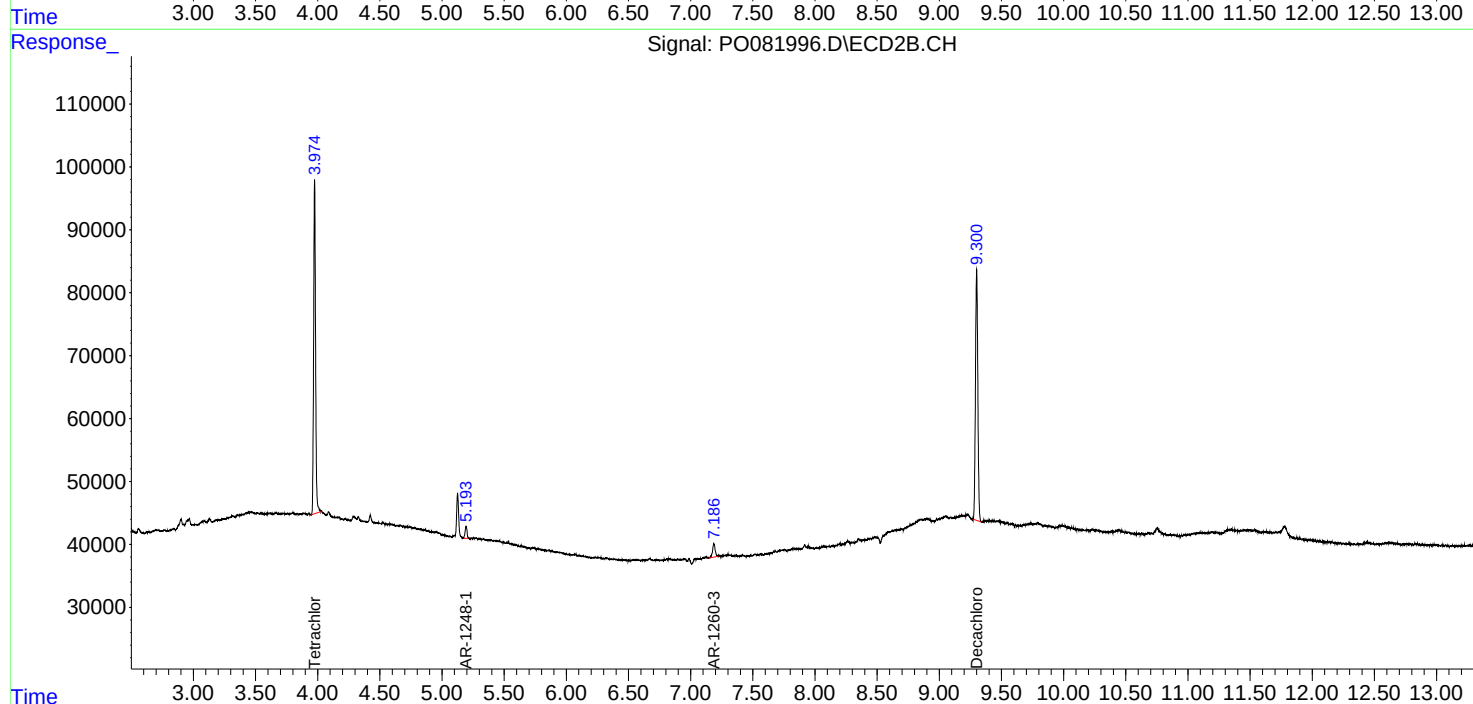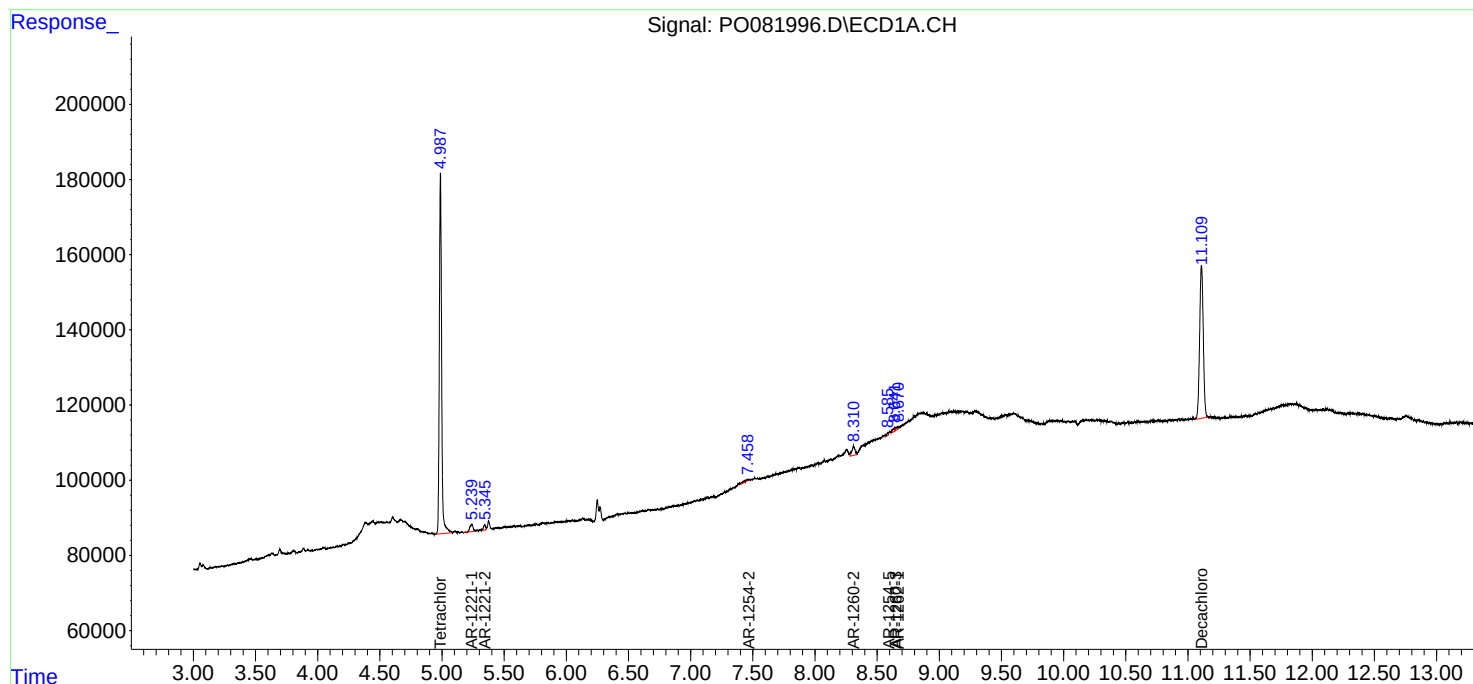


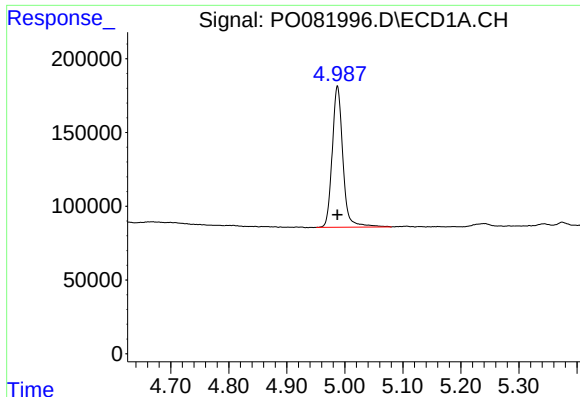

#1 Tetrachloro-m-xylene


R.T.: 4.987 min
Delta R.T.: 0.000 min
Response: 1222241
Conc: 21.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

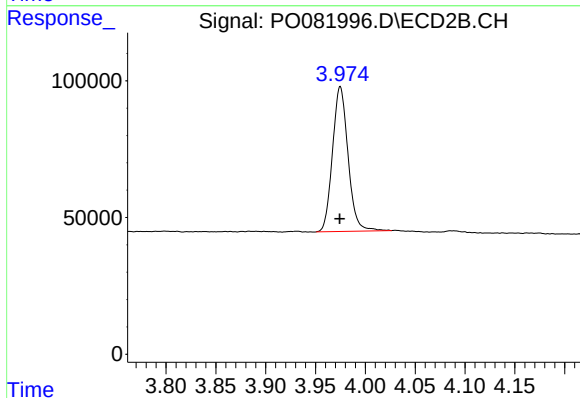


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: 0.000 min
Response: 575693
Conc: 21.26 ng/ml

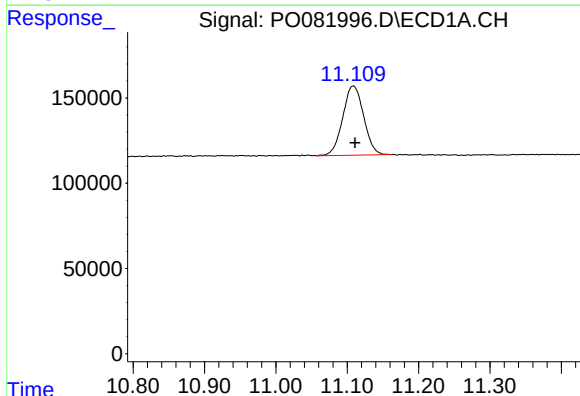


#2 Decachlorobiphenyl

R.T.: 11.109 min
Delta R.T.: -0.002 min
Response: 827481
Conc: 22.82 ng/ml

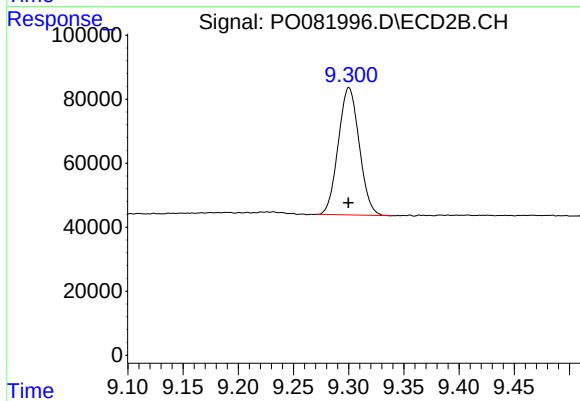

#2 Decachlorobiphenyl


R.T.: 9.300 min
Delta R.T.: 0.000 min
Response: 525604
Conc: 21.98 ng/ml

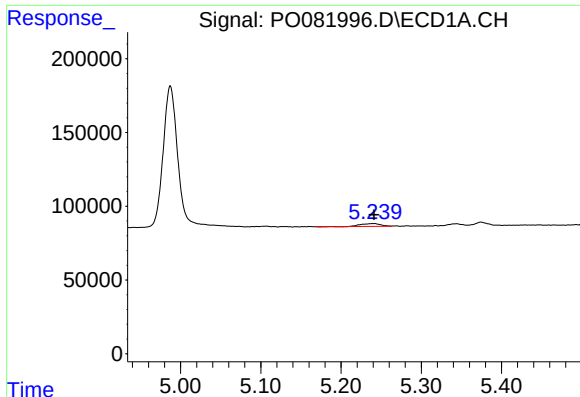

#8 AR-1221-1


R.T.: 5.240 min
Delta R.T.: -0.001 min
Response: 33765
Conc: 48.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

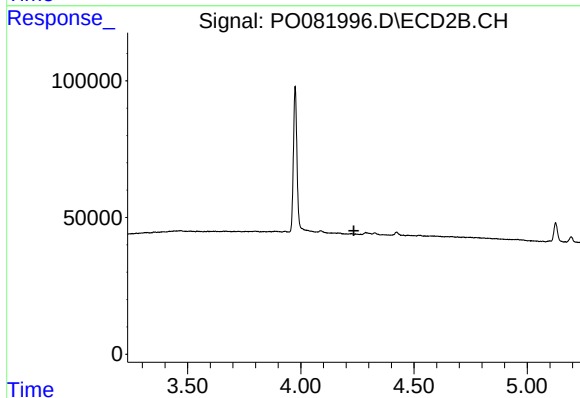


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.234 min
Response: 0
Conc: N.D.

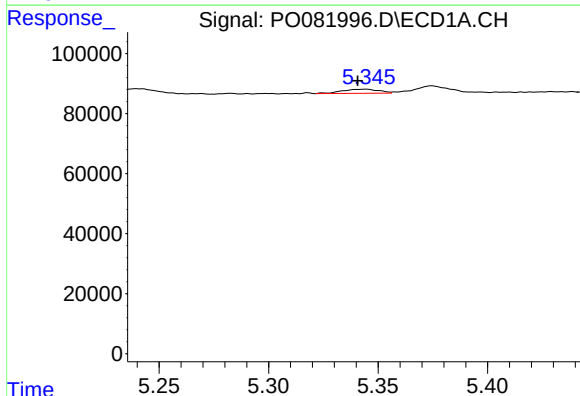


#9 AR-1221-2

R.T.: 5.345 min
Delta R.T.: 0.004 min
Response: 16383
Conc: 33.14 ng/ml

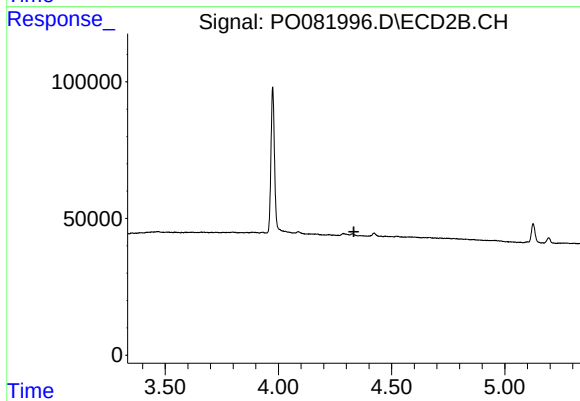

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.334 min
Response: 0
Conc: N.D.

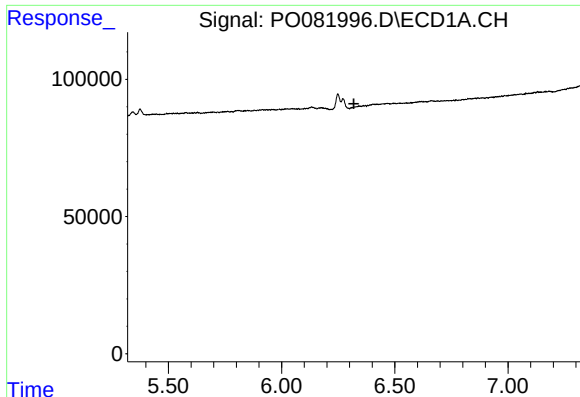

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 6.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

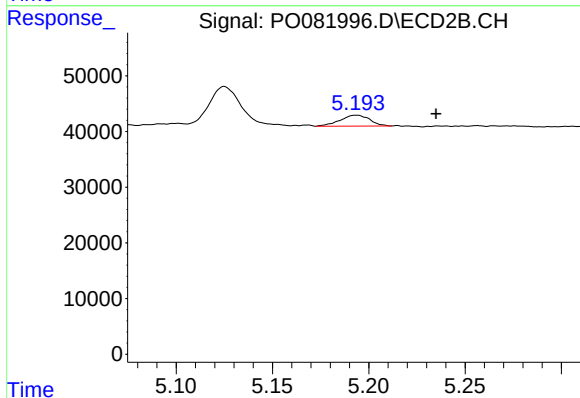


#21 AR-1248-1

R.T.: 5.194 min
Delta R.T.: -0.041 min
Response: 20905
Conc: 30.53 ng/ml

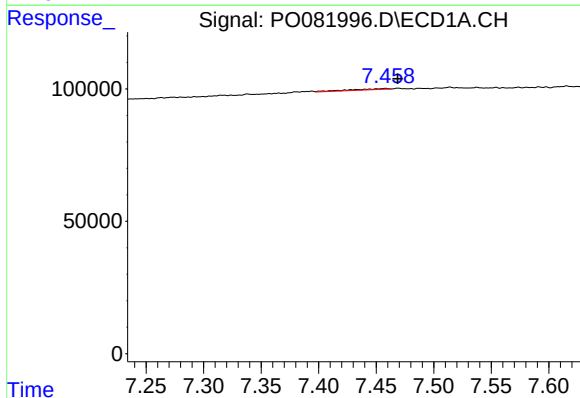


#27 AR-1254-2

R.T.: 7.458 min
Delta R.T.: -0.010 min
Response: 9614
Conc: 3.50 ng/ml

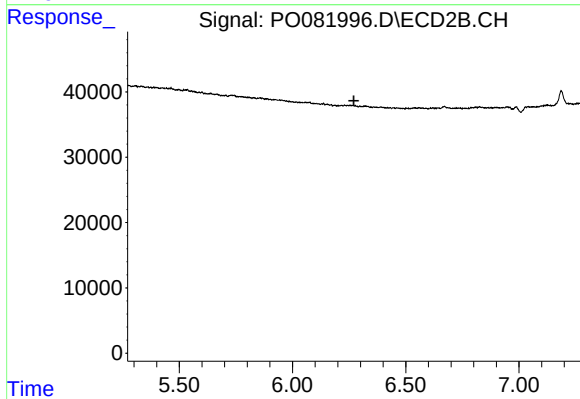

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.271 min
Response: 0
Conc: N.D.

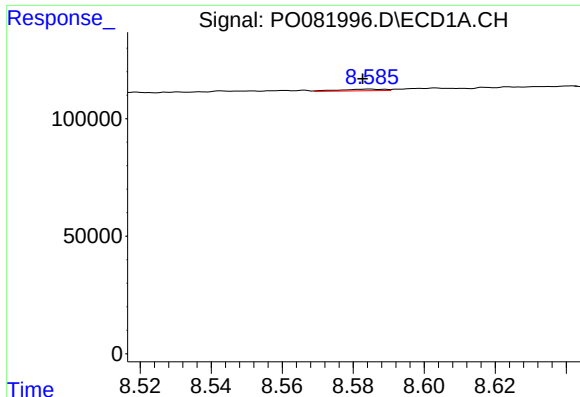

#30 AR-1254-5


R.T.: 8.585 min
Delta R.T.: 0.002 min
Response: 6138
Conc: 2.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

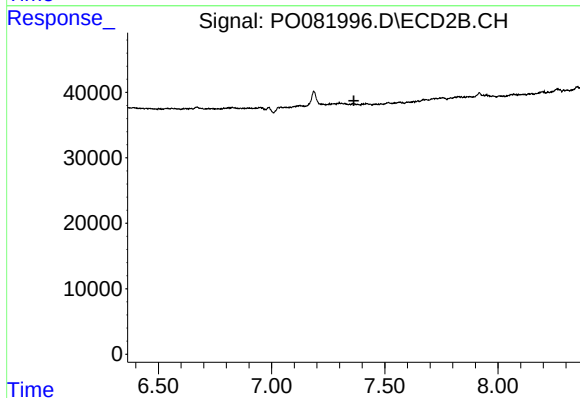


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

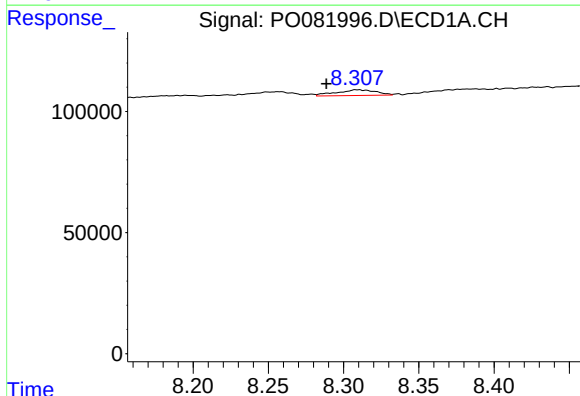


#32 AR-1260-2

R.T.: 8.310 min
Delta R.T.: 0.022 min
Response: 42422
Conc: 17.03 ng/ml

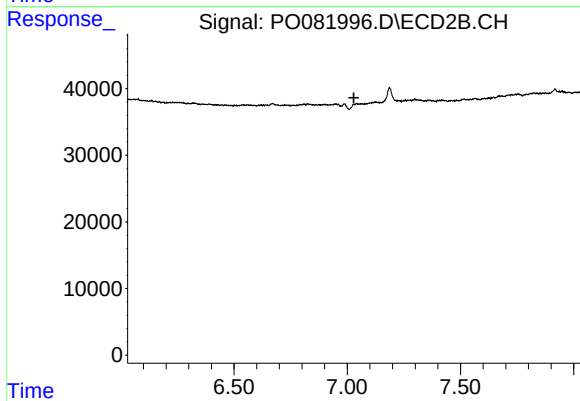

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.029 min
Response: 0
Conc: N.D.

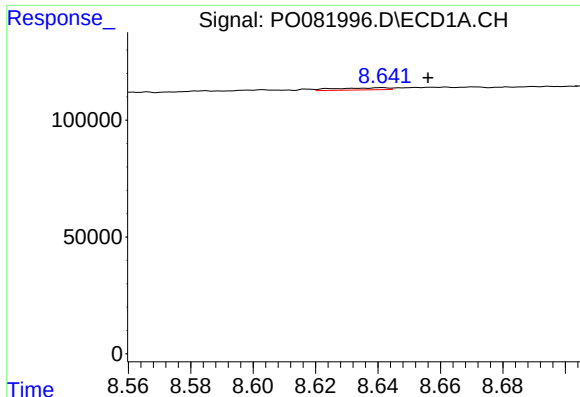

#33 AR-1260-3


R.T.: 8.641 min
Delta R.T.: -0.015 min
Response: 10702
Conc: 6.30 ng/ml

Instrument :
ECD_O
ClientSampleId :

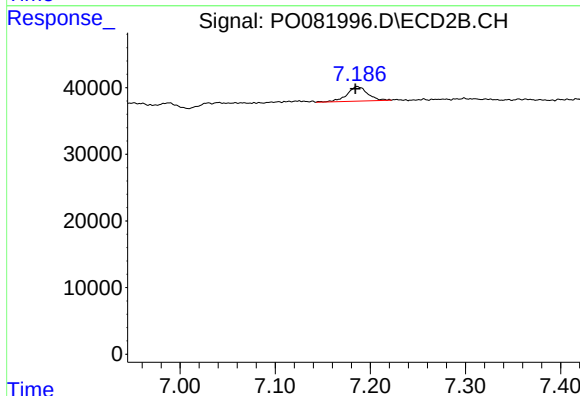


#33 AR-1260-3

R.T.: 7.186 min
Delta R.T.: 0.002 min
Response: 32521
Conc: 18.77 ng/ml

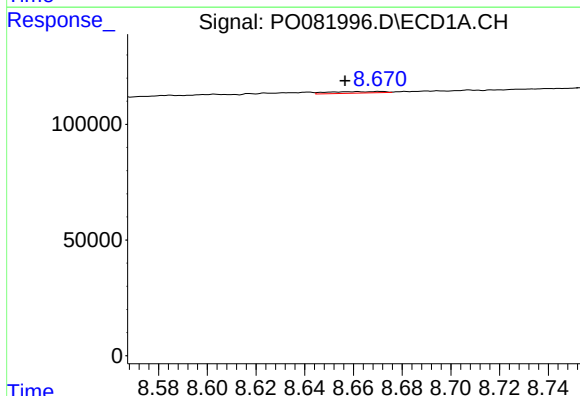

#36 AR-1262-1

R.T.: 8.671 min
Delta R.T.: 0.014 min
Response: 10665
Conc: 2.29 ng/ml

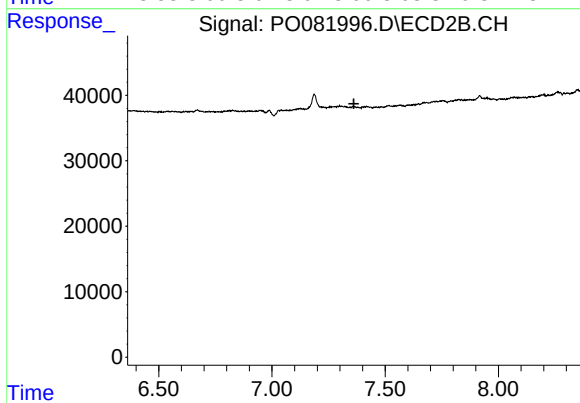

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.