

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0101223\  
 Data File : P0098734.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 12 Oct 2023 12:12  
 Operator : YP/AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 12 15:18:05 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0092723.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Sep 28 01:18:56 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 4.479  | 3.633 | 41891000 | 16118453 | 21.816 | 20.695 |
| 2)                          | SA Decachlor... | 10.293 | 8.641 | 28711582 | 12752992 | 23.653 | 23.803 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO101223\  
Data File : PO098734.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Oct 2023 12:12  
Operator : YP/AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 12 15:18:05 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO092723.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Sep 28 01:18:56 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

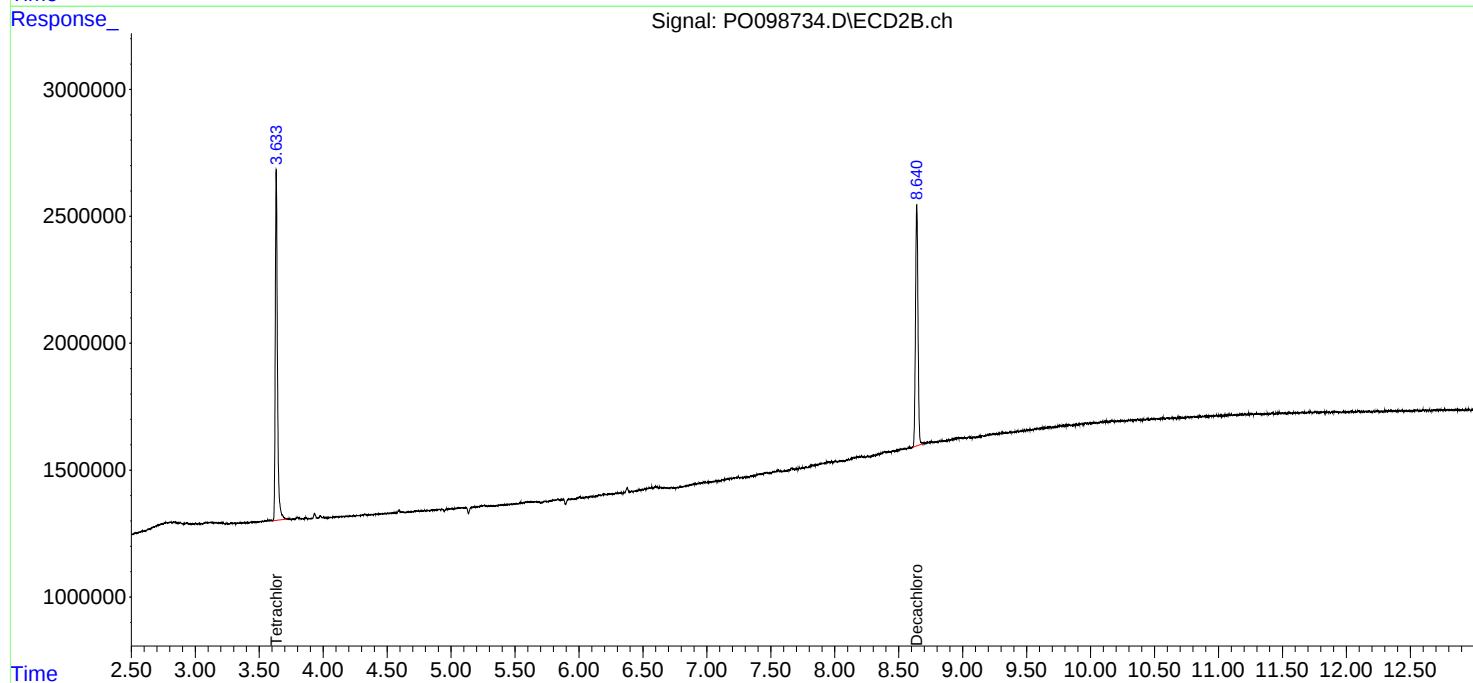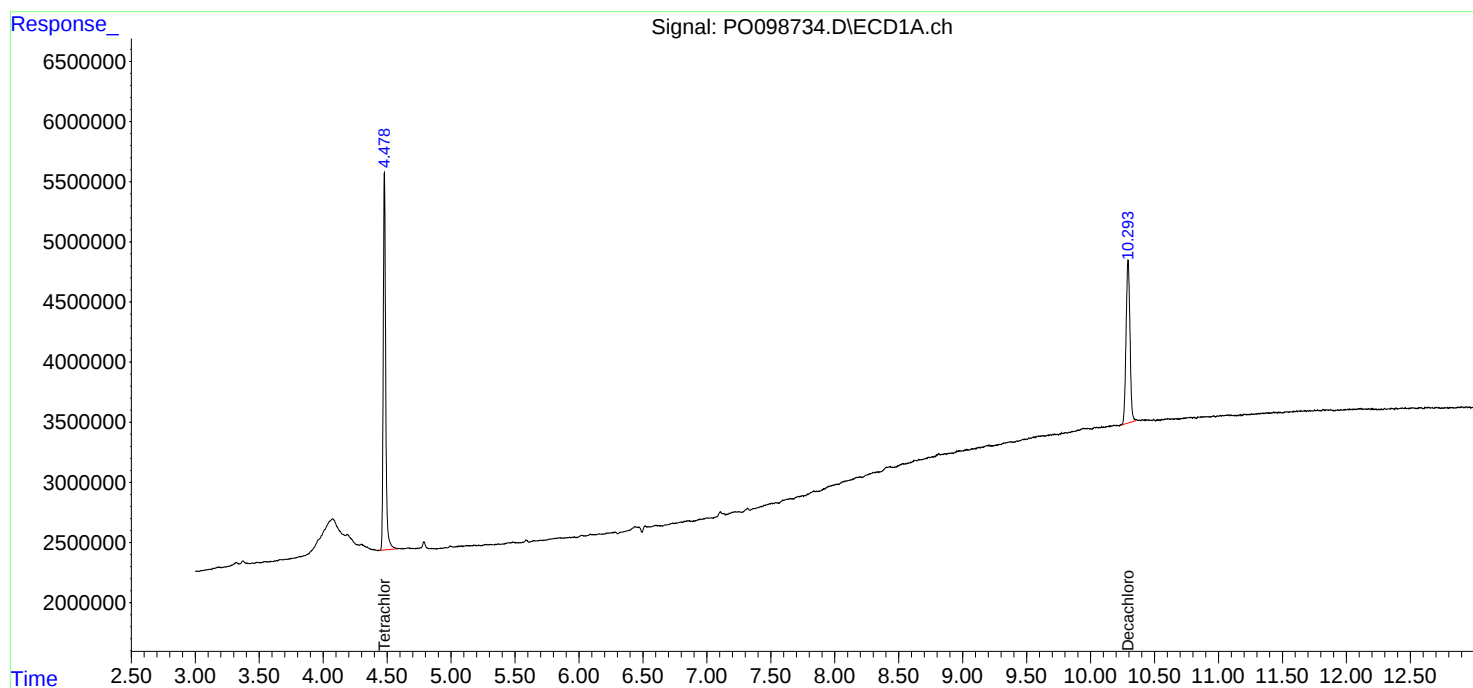


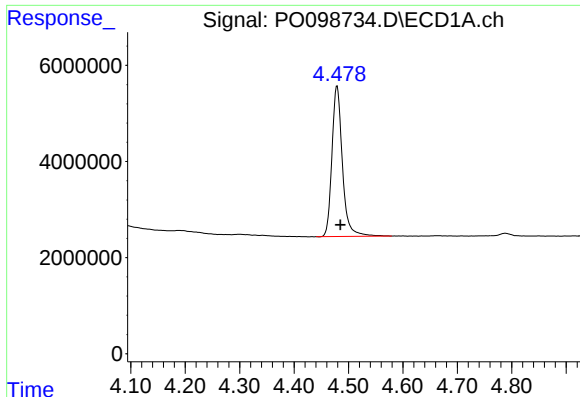

#1 Tetrachloro-m-xylene


R.T.: 4.479 min  
Delta R.T.: -0.006 min  
Response: 41891000  
Conc: 21.82 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

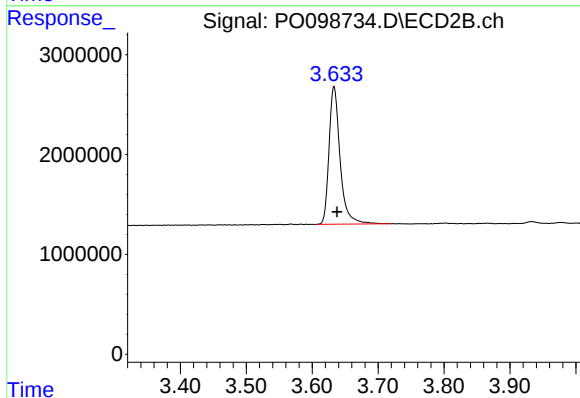


#1 Tetrachloro-m-xylene

R.T.: 3.633 min  
Delta R.T.: -0.005 min  
Response: 16118453  
Conc: 20.69 ng/ml

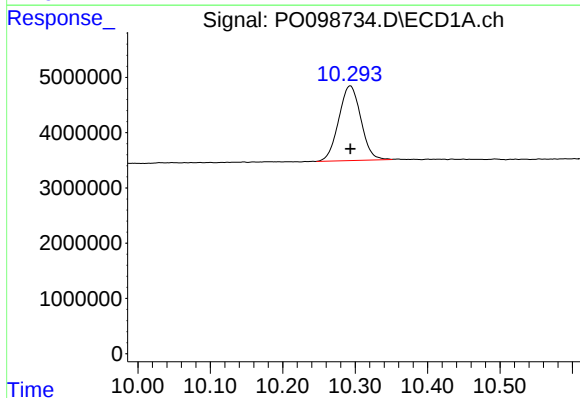

#2 Decachlorobiphenyl

R.T.: 10.293 min  
Delta R.T.: 0.000 min  
Response: 28711582  
Conc: 23.65 ng/ml

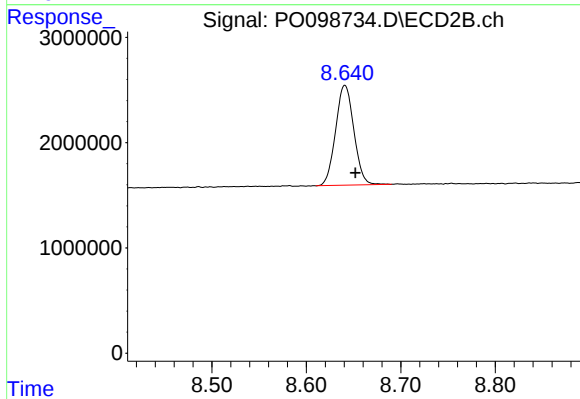

#2 Decachlorobiphenyl

R.T.: 8.641 min  
Delta R.T.: -0.011 min  
Response: 12752992  
Conc: 23.80 ng/ml