

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101223\
 Data File : P0098749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2023 17:20
 Operator : YP/AJ
 Sample : 04728-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K242-25B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/13/2023
 Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:15:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.633	32142016	13348558	16.739	17.139
2) SA Decachlor...	10.293	8.641	17855720	8072060	14.710	15.066

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101223\
Data File : PO098749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2023 17:20
Operator : YP/AJ
Sample : 04728-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K242-25B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:15:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

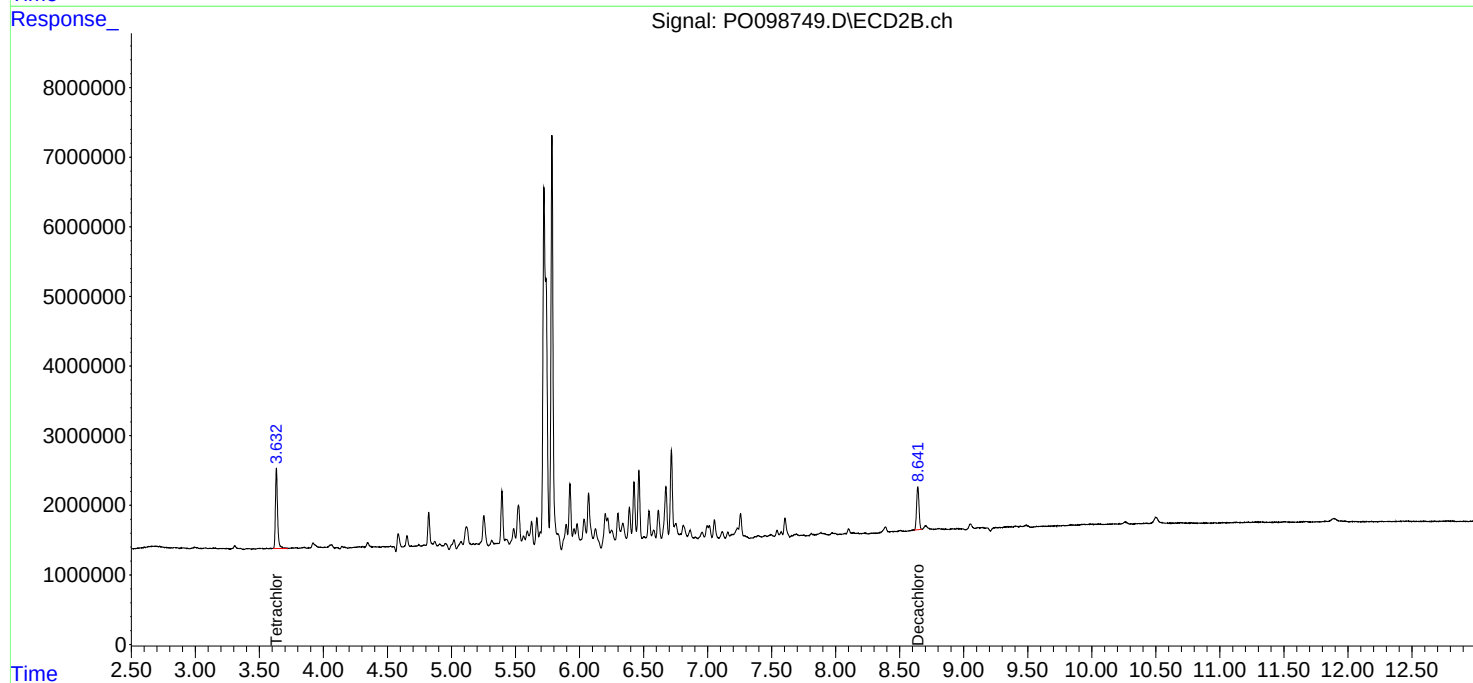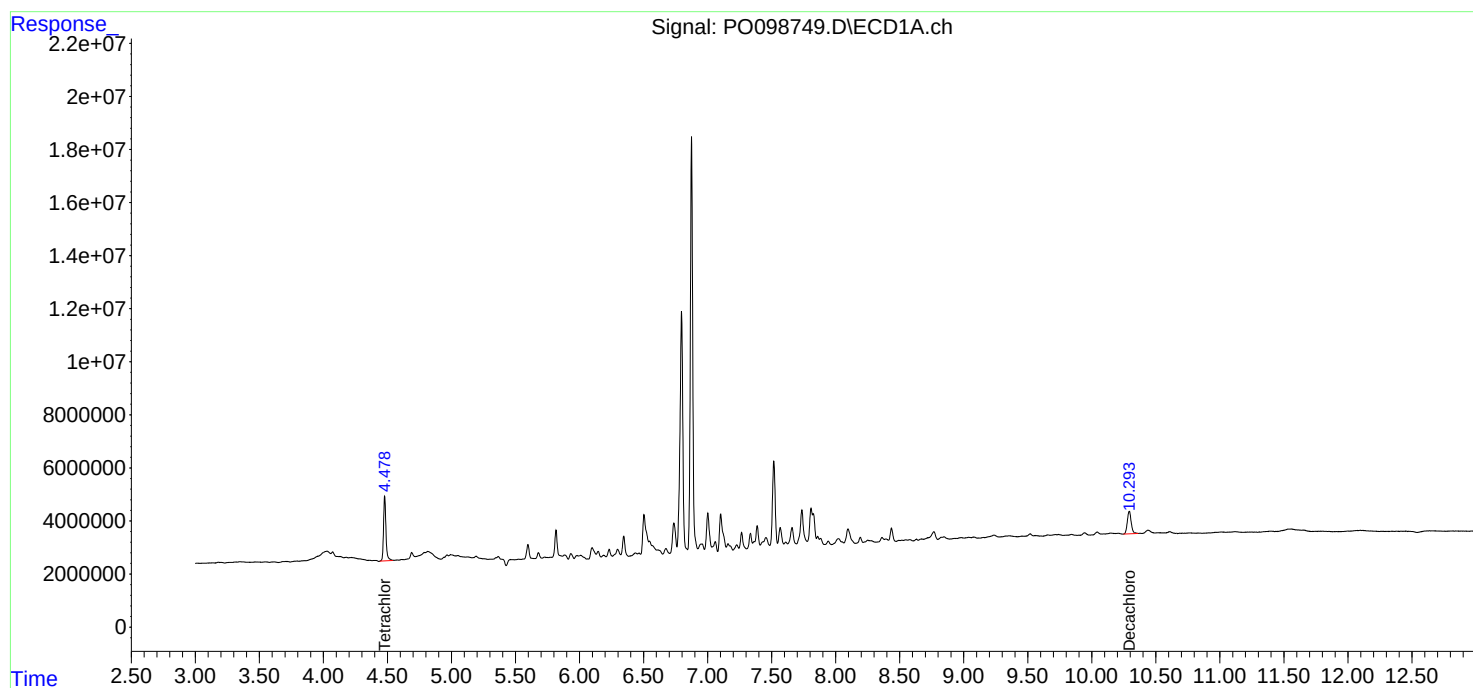

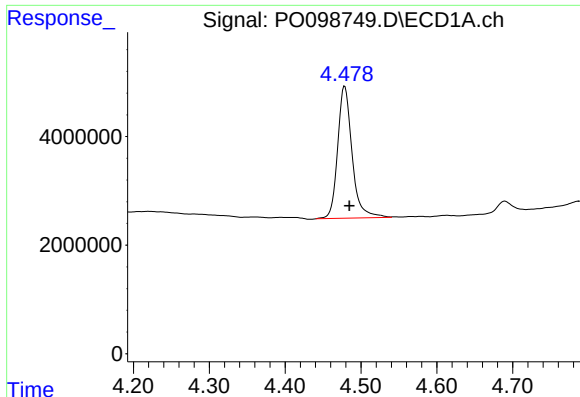


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: -0.006 min
Response: 32142016
Conc: 16.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-25B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

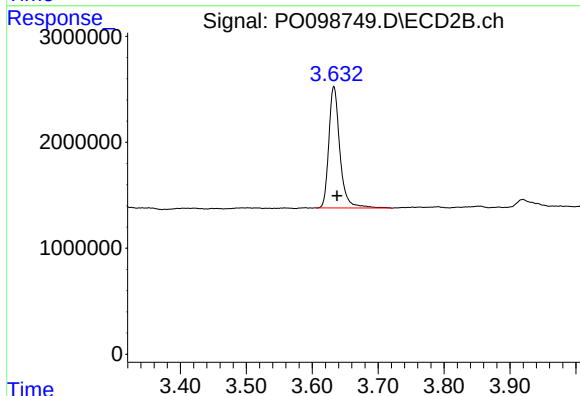


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.005 min
Response: 13348558
Conc: 17.14 ng/ml

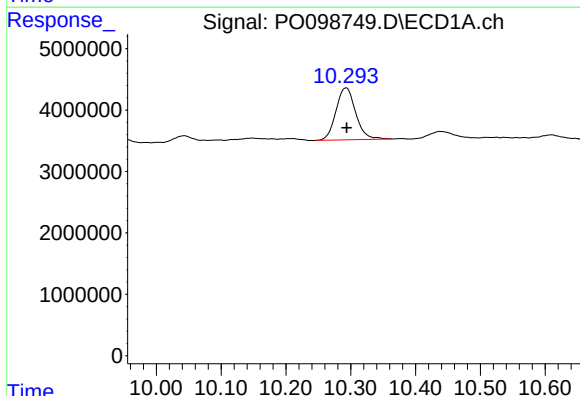

#2 Decachlorobiphenyl

R.T.: 10.293 min
Delta R.T.: 0.000 min
Response: 17855720
Conc: 14.71 ng/ml

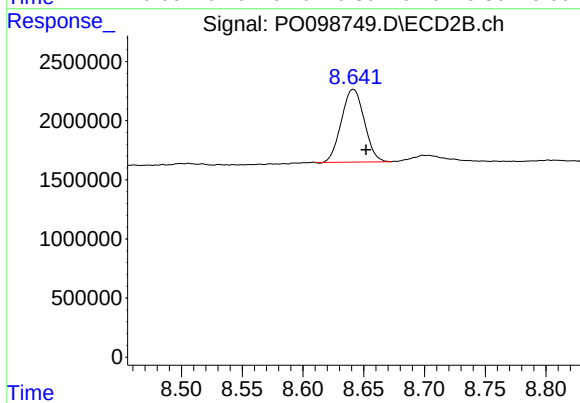

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: -0.011 min
Response: 8072060
Conc: 15.07 ng/ml