

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101223\
 Data File : P0098754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2023 18:44
 Operator : YP/AJ
 Sample : 04730-23
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/13/2023
 Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:20:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.634	34096154	13910048	17.757	17.859
2) SA Decachlor...	10.292	8.638	16132870	6784200	13.291	12.663

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101223\
Data File : PO098754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2023 18:44
Operator : YP/AJ
Sample : 04730-23
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DUP-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:20:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

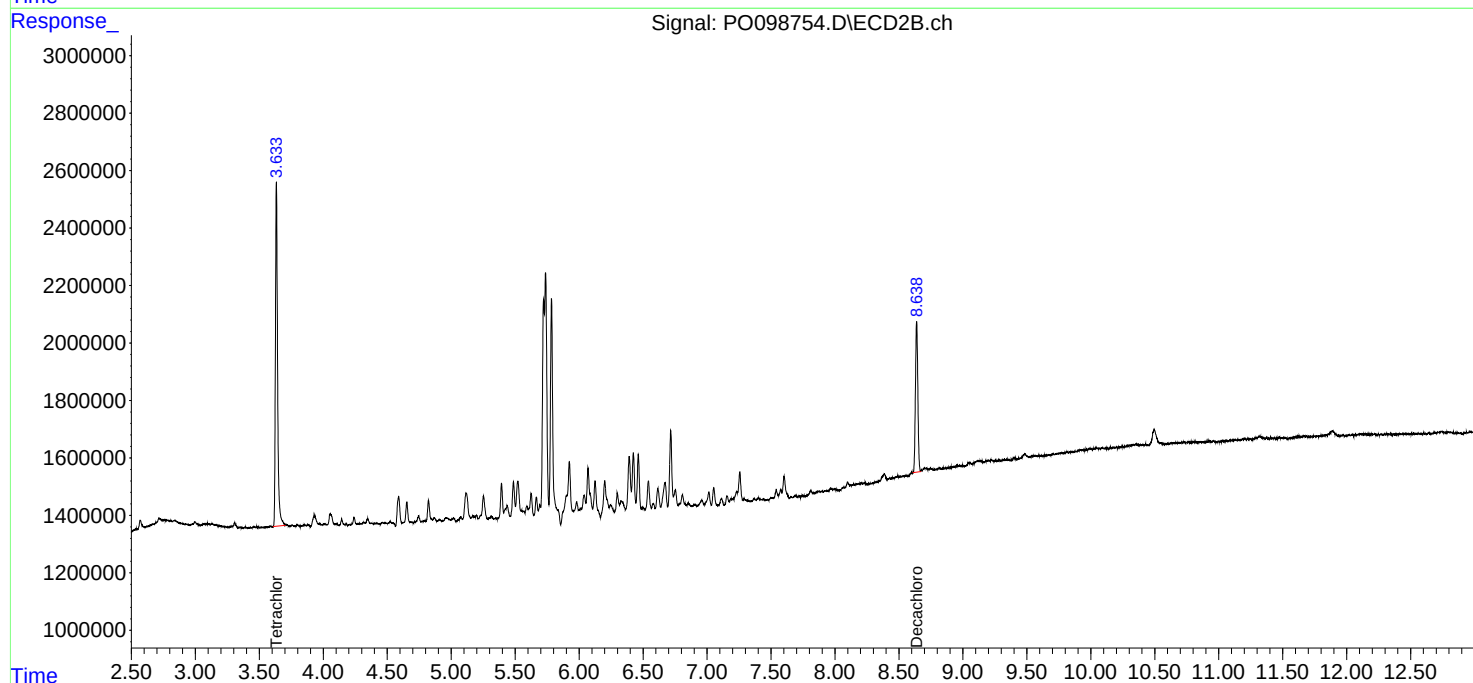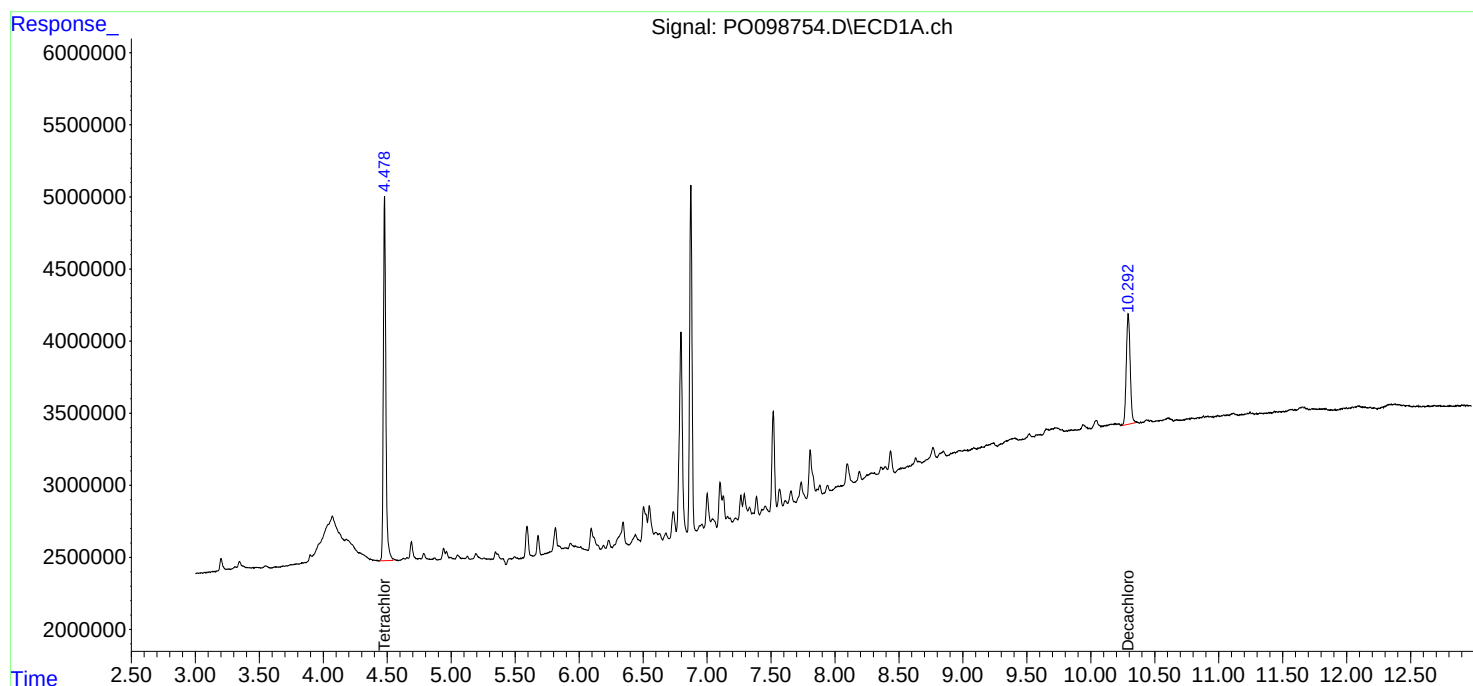

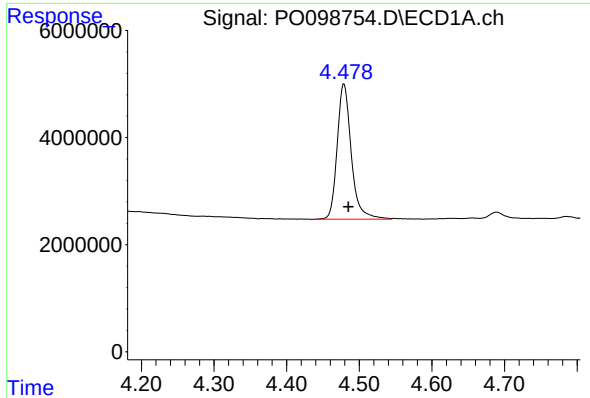


#1 Tetrachloro-m-xylene

R.T.: 4.479 min
Delta R.T.: -0.006 min
Response: 34096154
Conc: 17.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

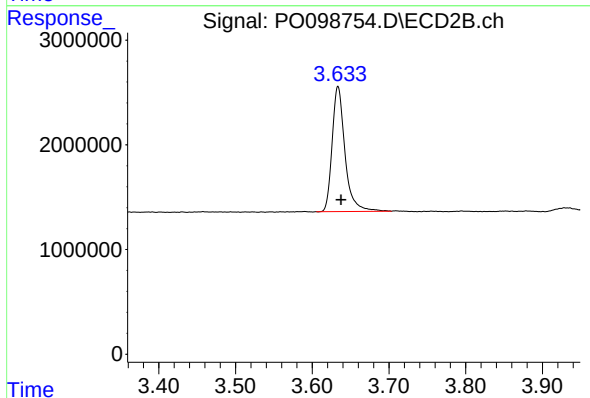


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.004 min
Response: 13910048
Conc: 17.86 ng/ml

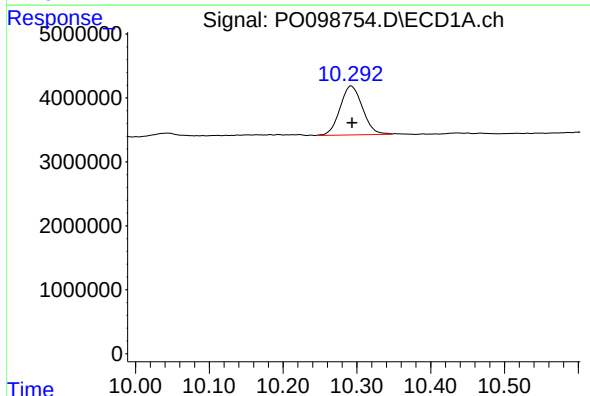

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: -0.001 min
Response: 16132870
Conc: 13.29 ng/ml

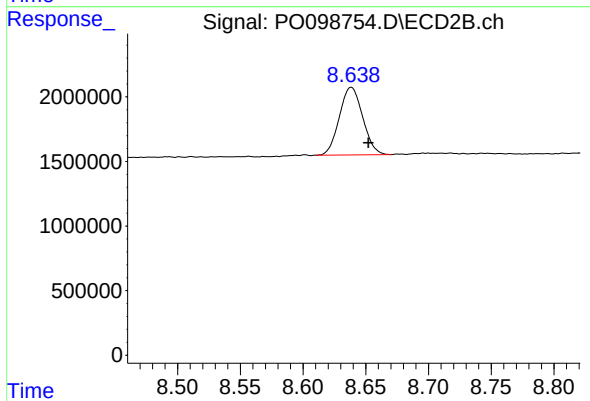

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: -0.014 min
Response: 6784200
Conc: 12.66 ng/ml