

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO101223\
 Data File : PO098765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Oct 2023 21:51
 Operator : YP/AJ
 Sample : 04726-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 K242-11C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/13/2023
 Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 01:26:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.632	34354513	13415376	17.891	17.224
2) SA Decachlor...	10.290	8.637	17542603	8406128	14.452	15.690
Target Compounds						
26) L6 AR-1254-1	6.511	5.518	4638785	1976266	73.441	51.540m#
27) L6 AR-1254-2	6.734	5.665	4344413	1010179	45.270	29.342m#
28) L6 AR-1254-3	7.101	6.069	4679907	2691898	49.737	51.805m
29) L6 AR-1254-4	7.386	6.298	2599710	1082413	44.650	39.435m
30) L6 AR-1254-5	7.806	6.715	5820109	4046111	83.329m	93.405

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101223\
Data File : PO098765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Oct 2023 21:51
Operator : YP/AJ
Sample : 04726-05
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
K242-11C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 01:26:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

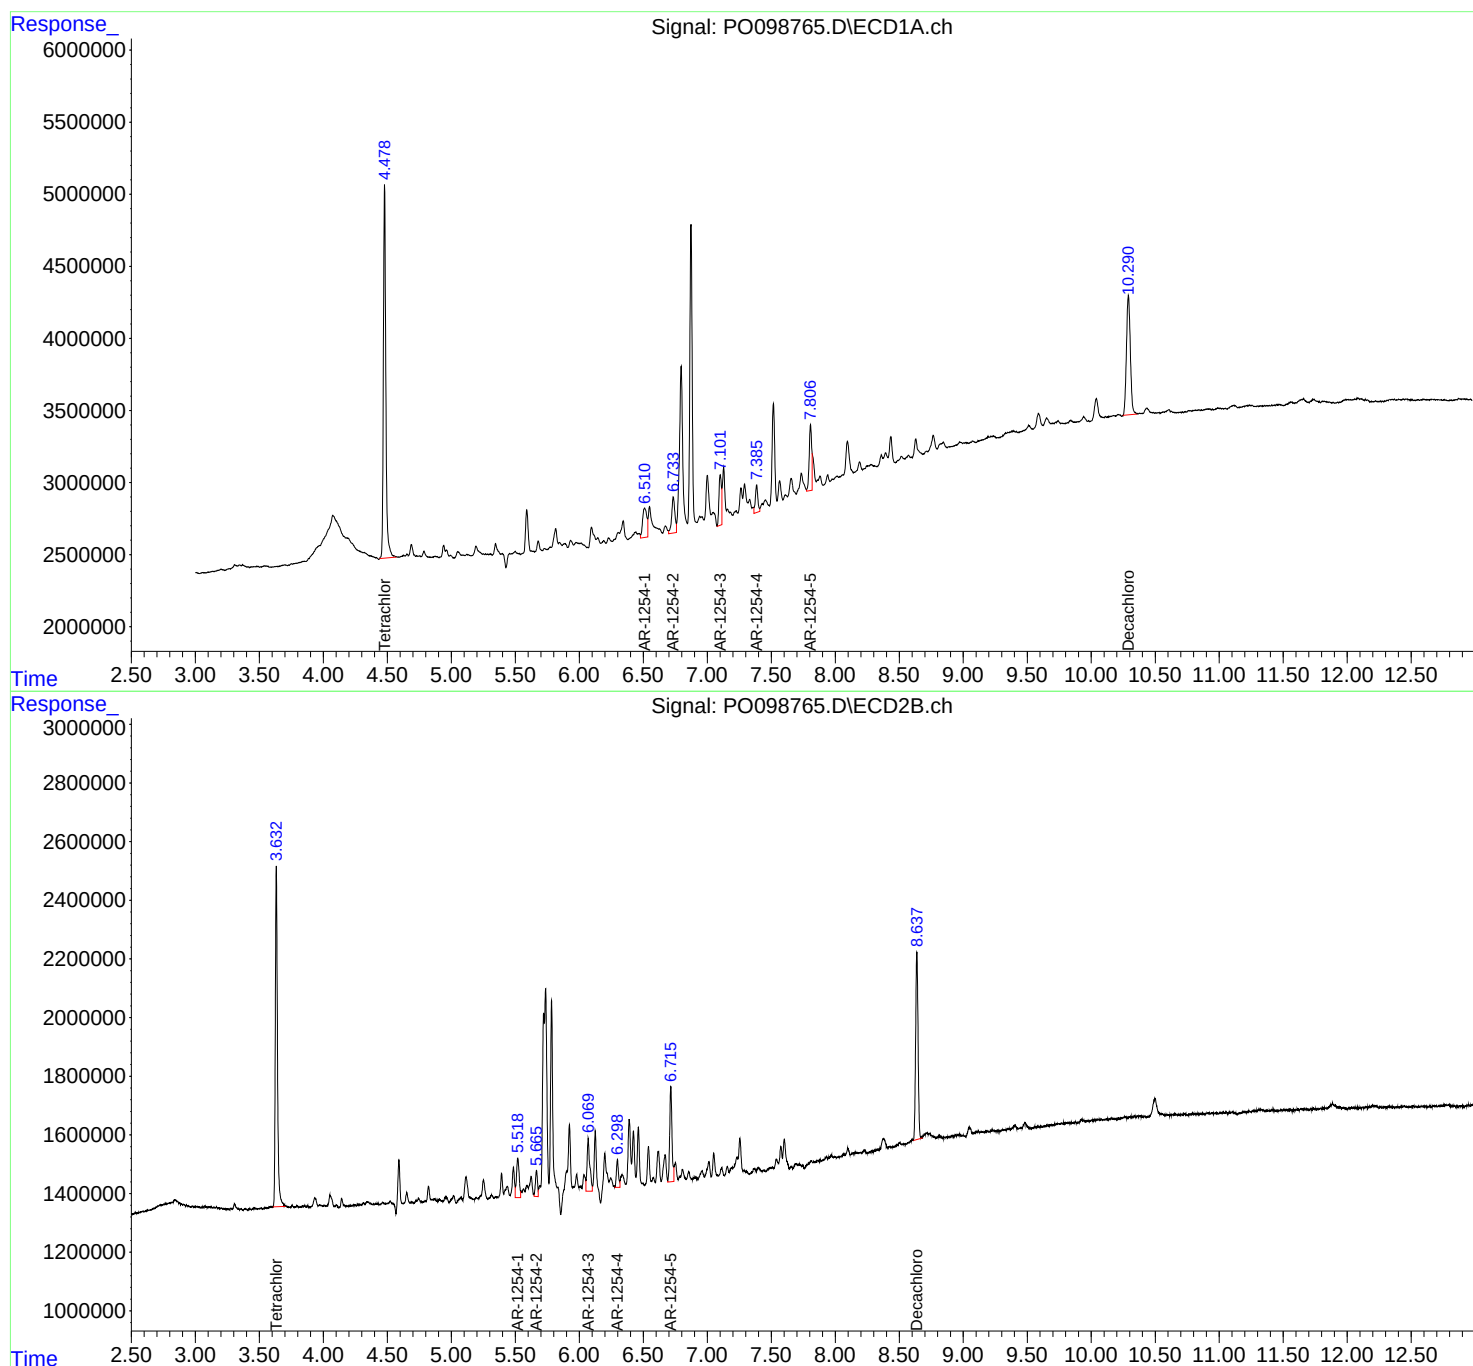

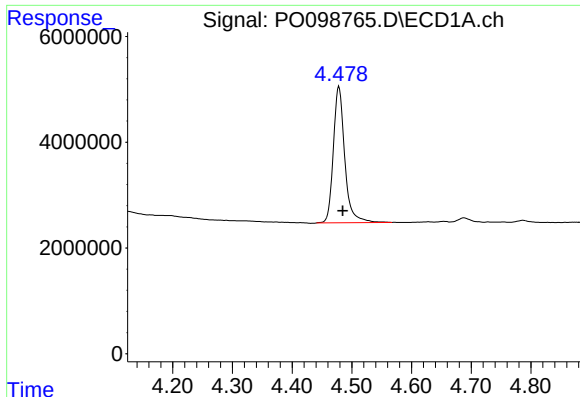


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.007 min
Response: 34354513
Conc: 17.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-11C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

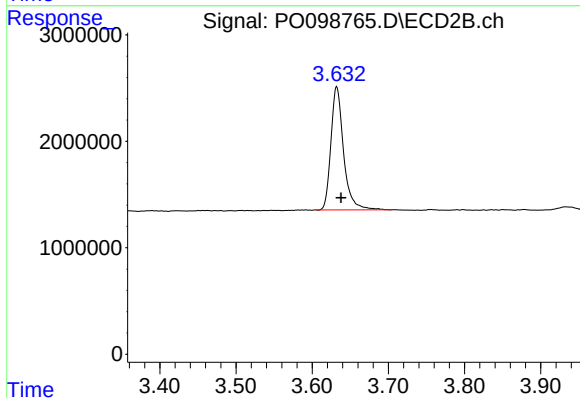


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.006 min
Response: 13415376
Conc: 17.22 ng/ml

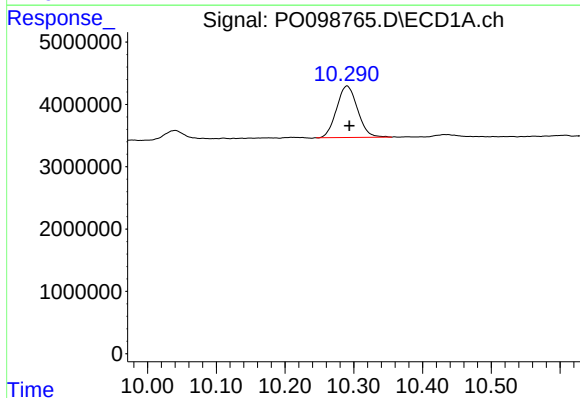


#2 Decachlorobiphenyl

R.T.: 10.290 min
Delta R.T.: -0.003 min
Response: 17542603
Conc: 14.45 ng/ml

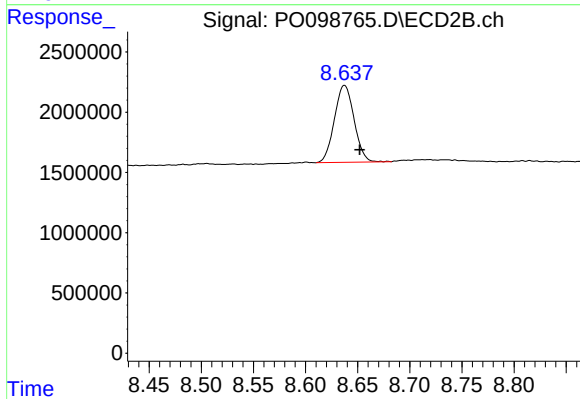

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.015 min
Response: 8406128
Conc: 15.69 ng/ml

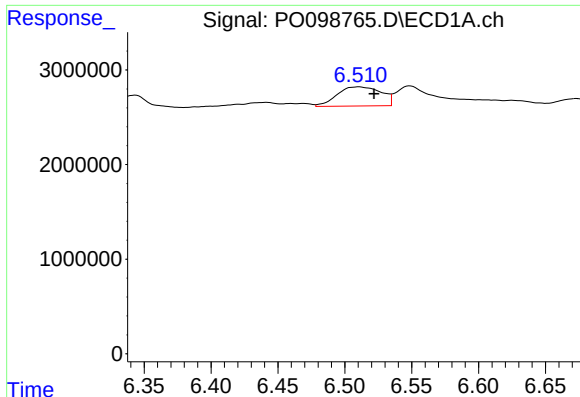


#26 AR-1254-1

R.T.: 6.511 min
Delta R.T.: -0.011 min
Response: 4638785
Conc: 73.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-11C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

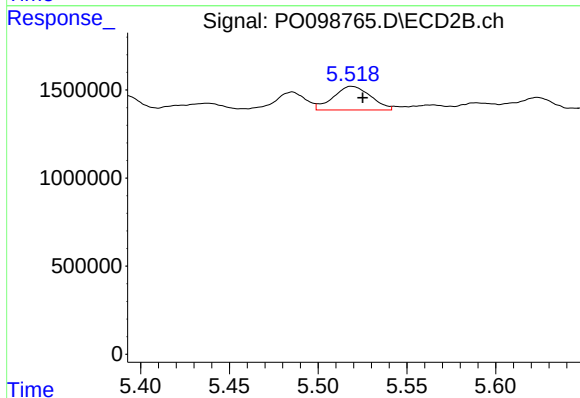


#26 AR-1254-1

R.T.: 5.518 min
Delta R.T.: -0.007 min
Response: 1976266
Conc: 51.54 ng/ml m

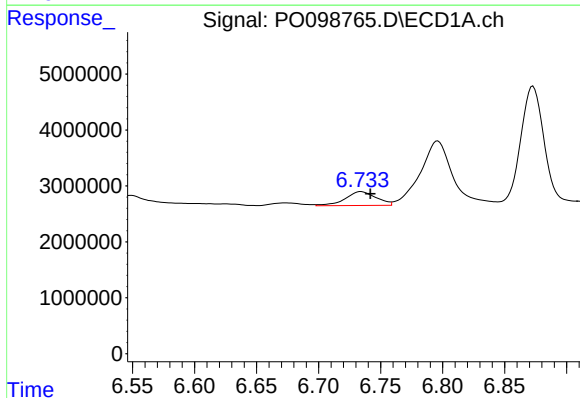


#27 AR-1254-2

R.T.: 6.734 min
Delta R.T.: -0.008 min
Response: 4344413
Conc: 45.27 ng/ml

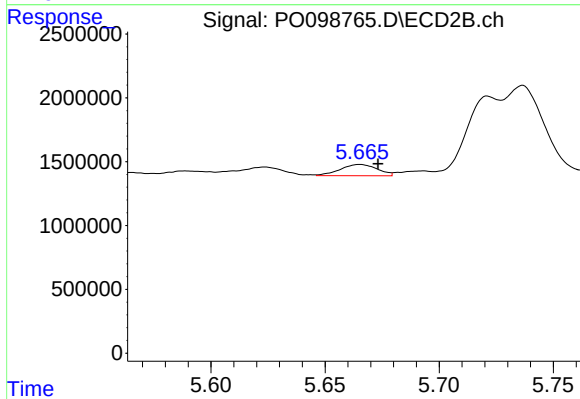

#27 AR-1254-2

R.T.: 5.665 min
Delta R.T.: -0.008 min
Response: 1010179
Conc: 29.34 ng/ml m

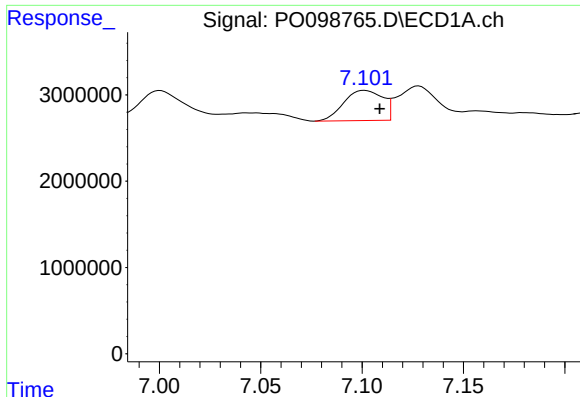


#28 AR-1254-3

R.T.: 7.101 min
Delta R.T.: -0.007 min
Response: 4679907
Conc: 49.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-11C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

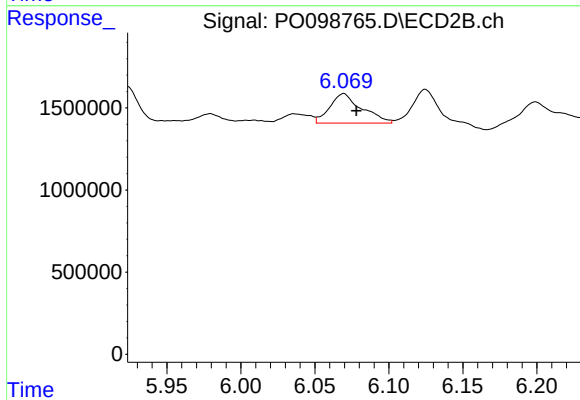


#28 AR-1254-3

R.T.: 6.069 min
Delta R.T.: -0.009 min
Response: 2691898
Conc: 51.81 ng/ml m

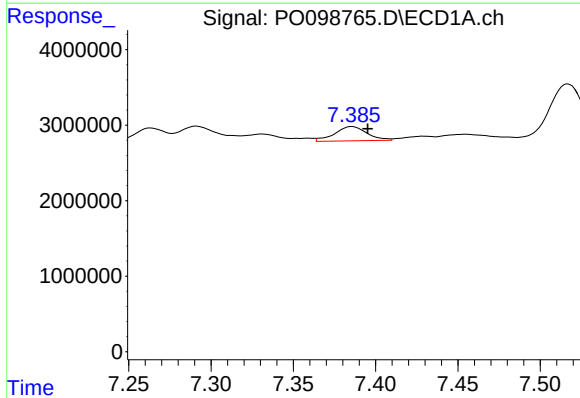


#29 AR-1254-4

R.T.: 7.386 min
Delta R.T.: -0.010 min
Response: 2599710
Conc: 44.65 ng/ml

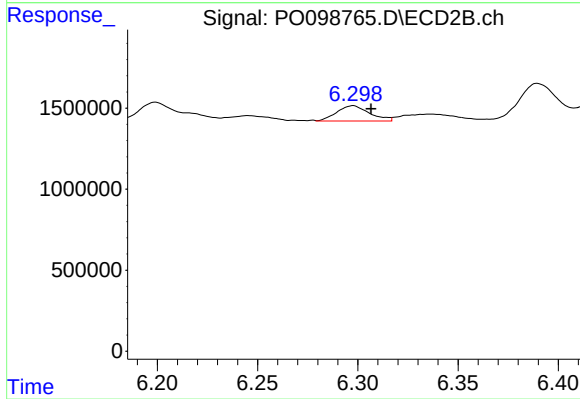

#29 AR-1254-4

R.T.: 6.298 min
Delta R.T.: -0.009 min
Response: 1082413
Conc: 39.43 ng/ml m

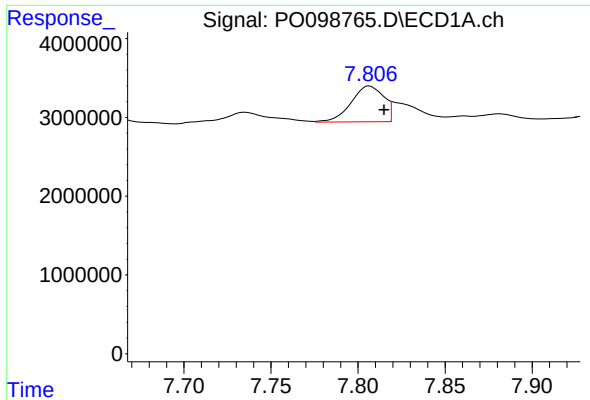


#30 AR-1254-5

R.T.: 7.806 min
Delta R.T.: -0.009 min
Response: 5820109
Conc: 83.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-11C

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

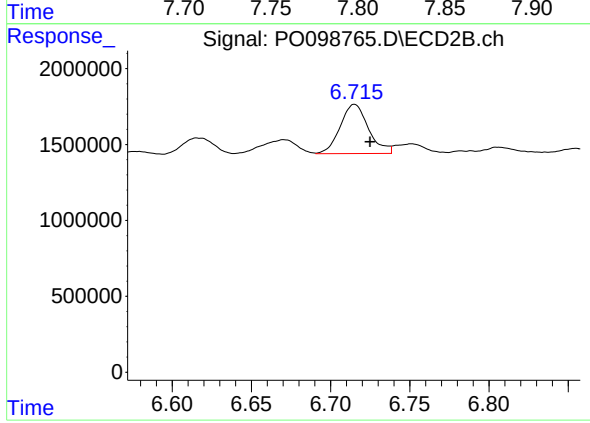

#30 AR-1254-5

R.T.: 6.715 min
Delta R.T.: -0.010 min
Response: 4046111
Conc: 93.40 ng/ml