

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101223\
 Data File : P0098781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 02:36
 Operator : YP/AJ
 Sample : 04727-13
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K242-21B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/13/2023
 Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 02:53:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.631	34363823	13630193	17.896	17.500
2) SA Decachlor...	10.288	8.635	19678288	7845290	16.211	14.643

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101223\
Data File : PO098781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 02:36
Operator : YP/AJ
Sample : 04727-13
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K242-21B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 02:53:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

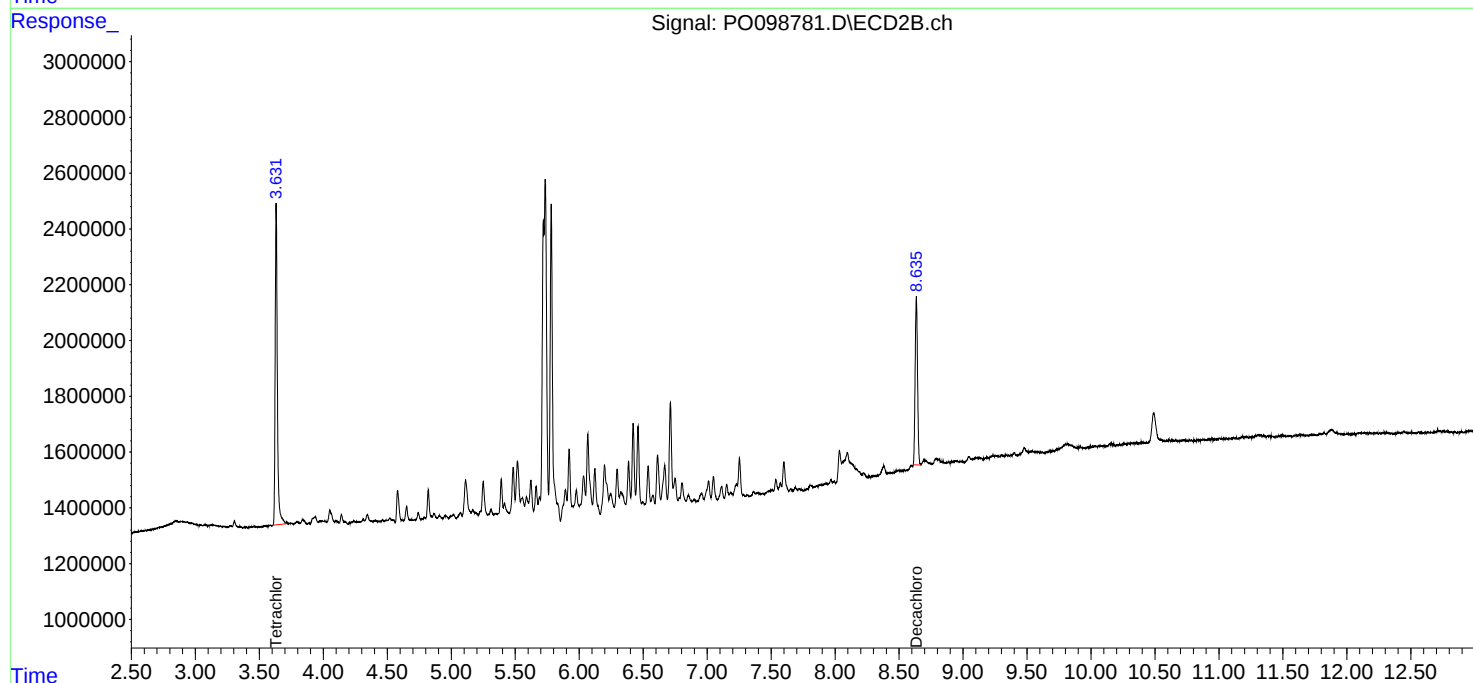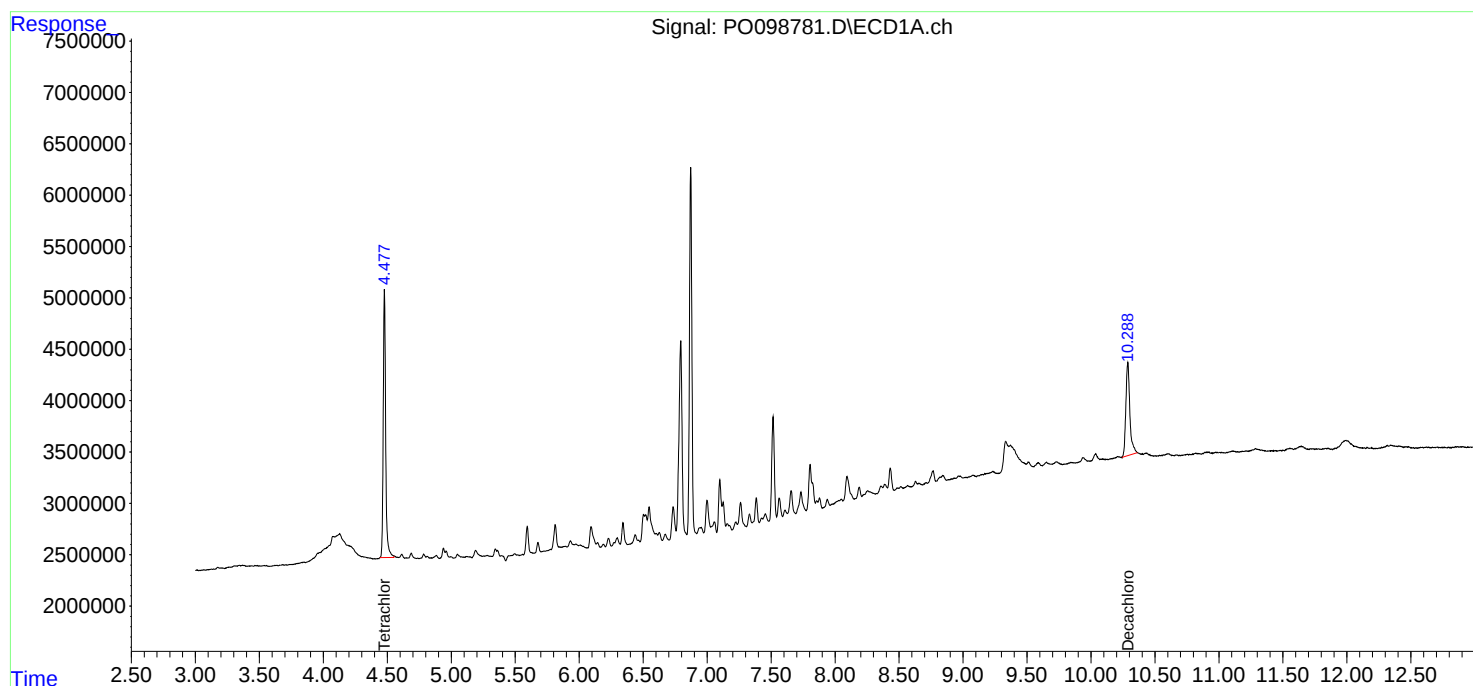

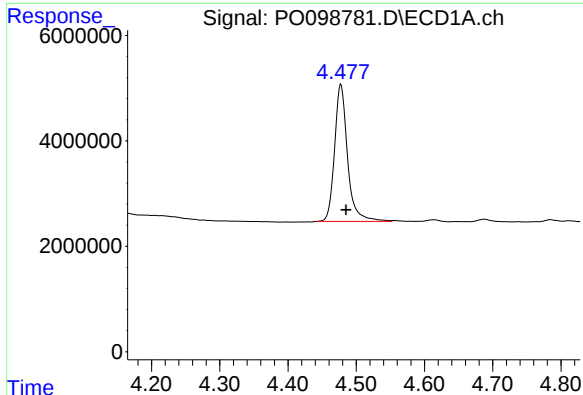


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.007 min
Response: 34363823
Conc: 17.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
K242-21B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/13/2023
Supervised By :Ankita Jodhani 10/13/2023

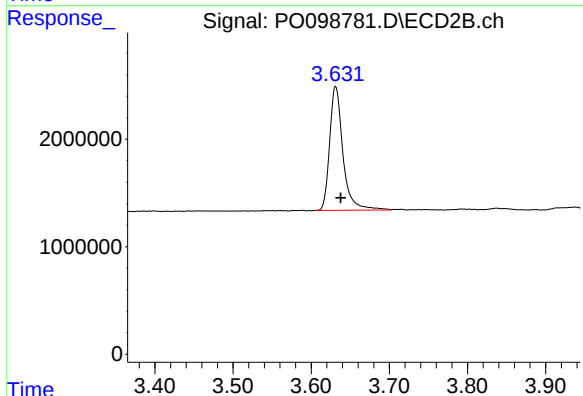


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.006 min
Response: 13630193
Conc: 17.50 ng/ml

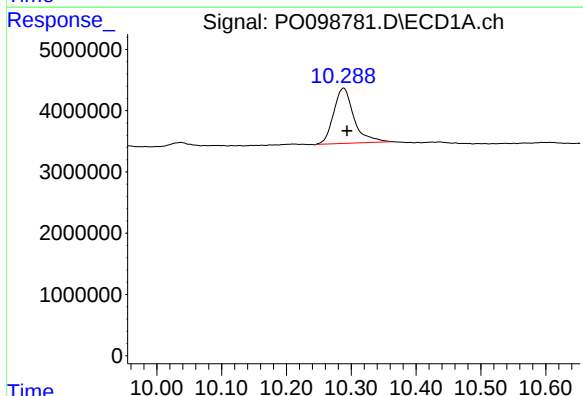

#2 Decachlorobiphenyl

R.T.: 10.288 min
Delta R.T.: -0.005 min
Response: 19678288
Conc: 16.21 ng/ml

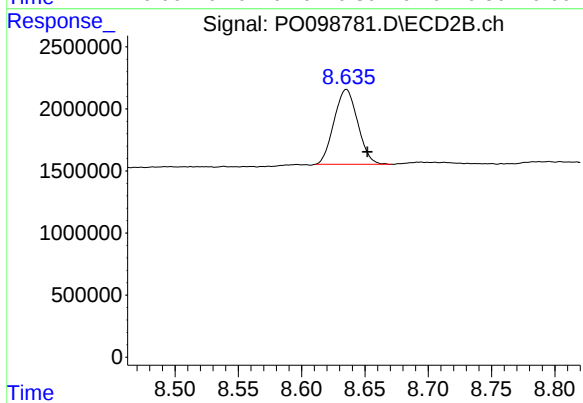

#2 Decachlorobiphenyl

R.T.: 8.635 min
Delta R.T.: -0.017 min
Response: 7845290
Conc: 14.64 ng/ml