

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101320\
 Data File : PO072315.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2020 16:09
 Operator : DD\AJ
 Sample : L4369-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-4

Manual Integrations
 APPROVED

Ankita
 10/14/2020 12:02:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:24:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.509	1984772	1011570	27.633	27.007
2) SA Decachlor...	9.931	8.679	1997602	986163	18.142	17.338
Target Compounds						
26) L6 AR-1254-1	6.518	5.581	2968229	1659154	849.582	694.254
27) L6 AR-1254-2	6.746	5.742	4496247	1578764	816.679	738.096
28) L6 AR-1254-3	7.122	6.151	5405285	2880954	935.952	848.548
29) L6 AR-1254-4	7.417	6.392	5142821	1653615	882.743	681.012
30) L6 AR-1254-5	7.838	6.812	5673970	3292537	1054.277m	1006.243

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101320\
Data File : PO072315.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2020 16:09
Operator : DD\AJ
Sample : L4369-08
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-4


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:24:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

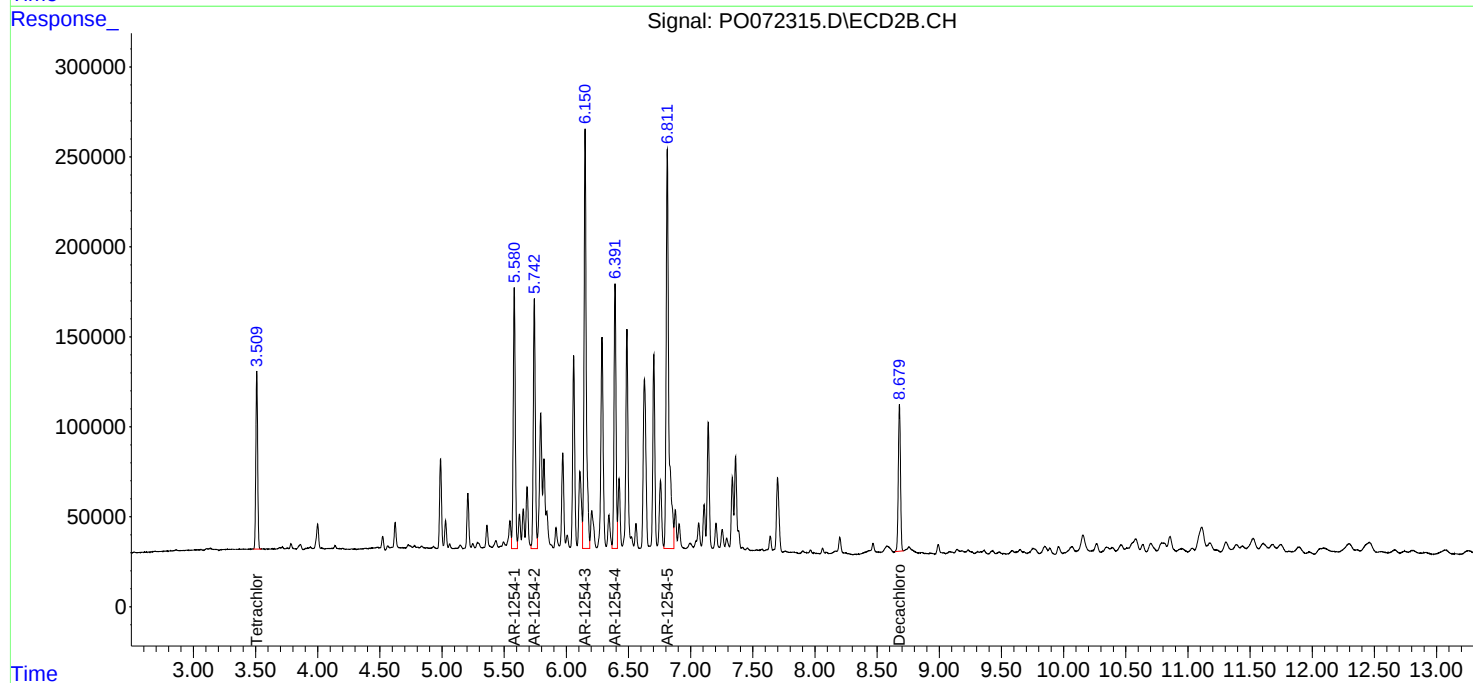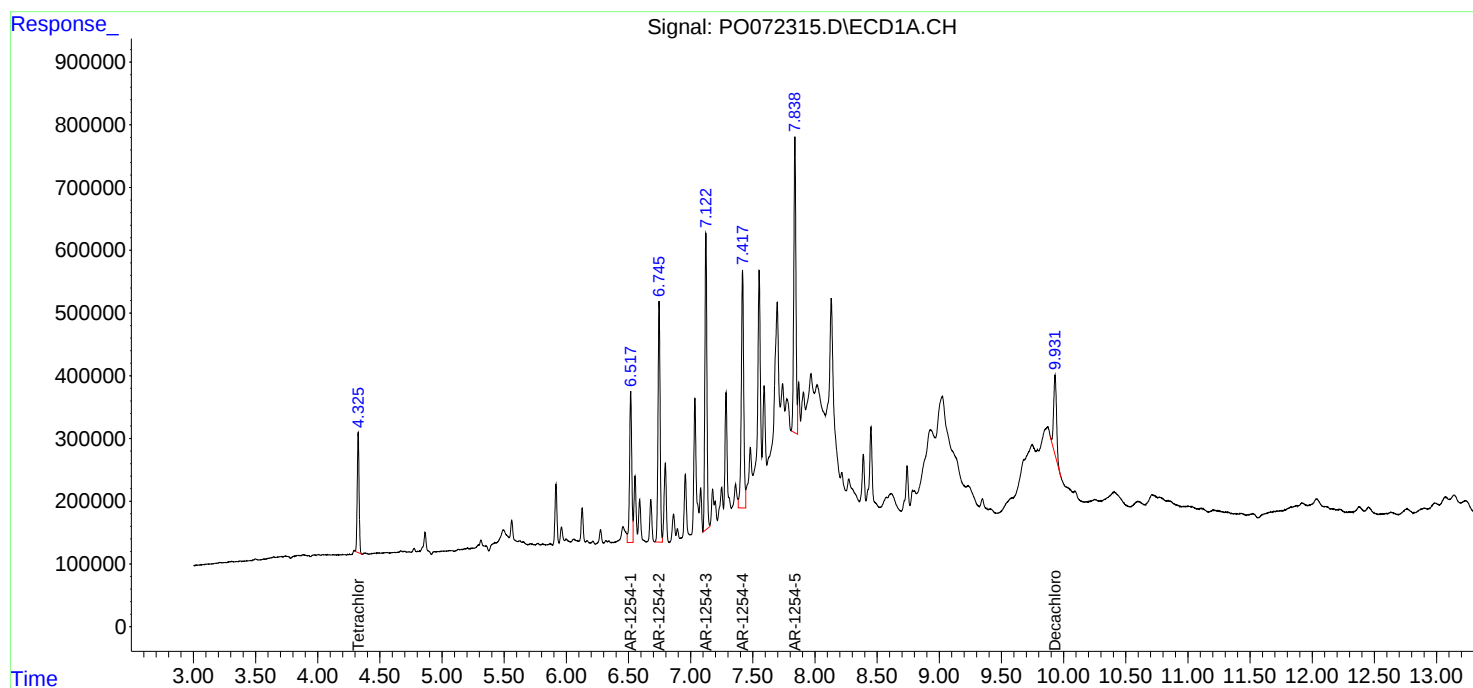

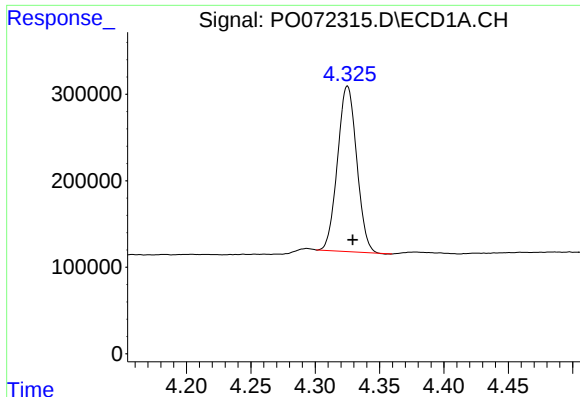


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.004 min
Response: 1984772
Conc: 27.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-4


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:38 PM

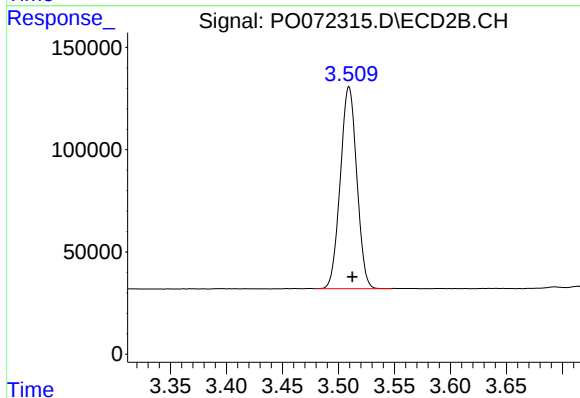


#1 Tetrachloro-m-xylene

R.T.: 3.509 min
Delta R.T.: -0.003 min
Response: 1011570
Conc: 27.01 ng/ml

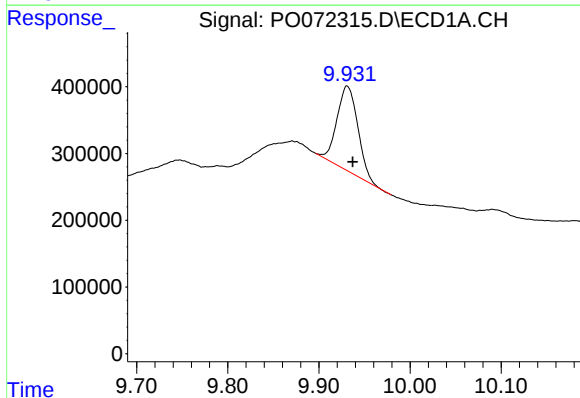


#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.006 min
Response: 1997602
Conc: 18.14 ng/ml

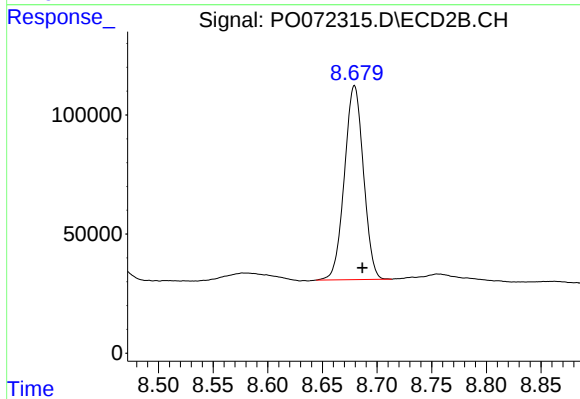

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.007 min
Response: 986163
Conc: 17.34 ng/ml

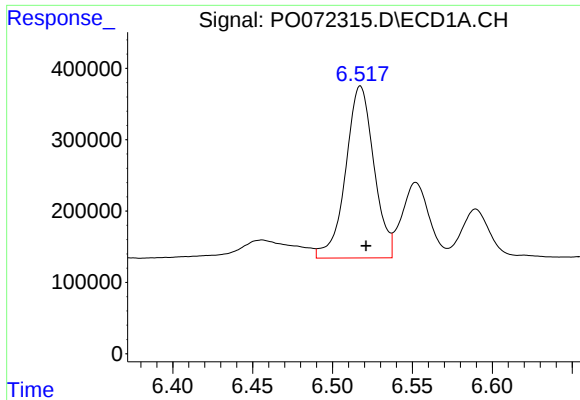


#26 AR-1254-1

R.T.: 6.518 min
Delta R.T.: -0.004 min
Response: 2968229
Conc: 849.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-4


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:38 PM

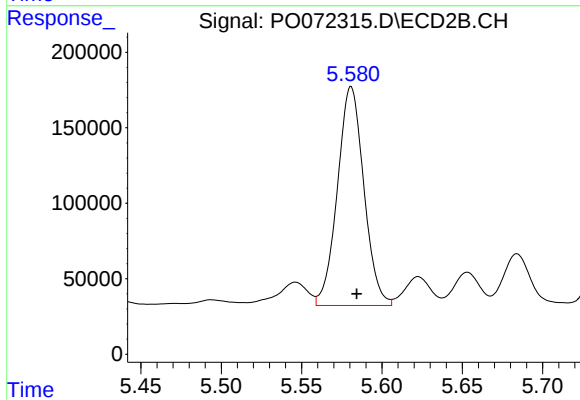


#26 AR-1254-1

R.T.: 5.581 min
Delta R.T.: -0.003 min
Response: 1659154
Conc: 694.25 ng/ml

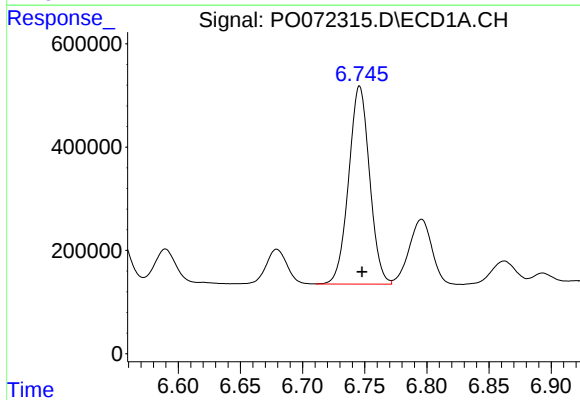


#27 AR-1254-2

R.T.: 6.746 min
Delta R.T.: -0.002 min
Response: 4496247
Conc: 816.68 ng/ml

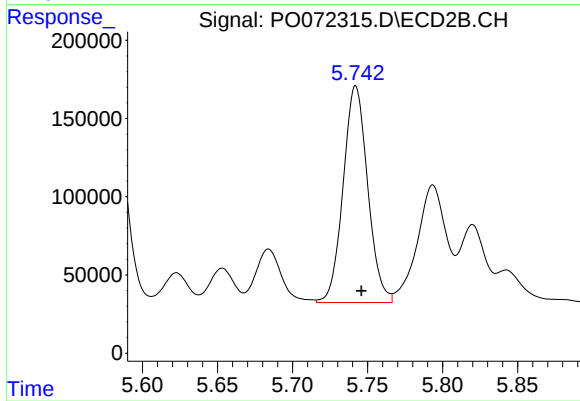

#27 AR-1254-2

R.T.: 5.742 min
Delta R.T.: -0.004 min
Response: 1578764
Conc: 738.10 ng/ml

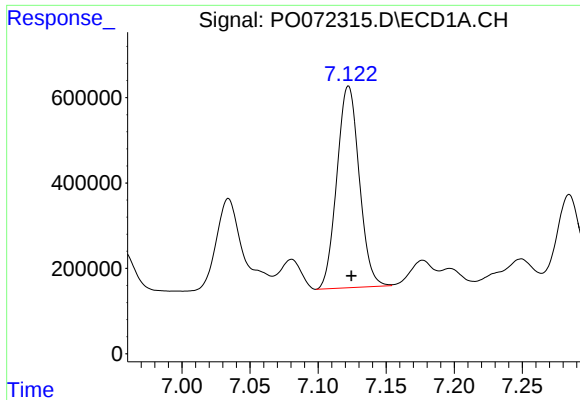


#28 AR-1254-3

R.T.: 7.122 min
Delta R.T.: -0.002 min
Response: 5405285
Conc: 935.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-4


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:38 PM

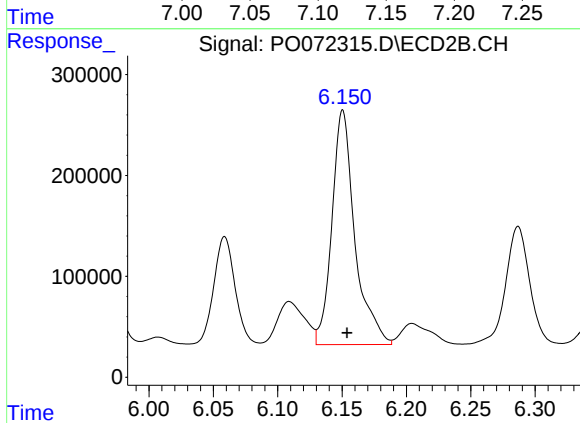


#28 AR-1254-3

R.T.: 6.151 min
Delta R.T.: -0.003 min
Response: 2880954
Conc: 848.55 ng/ml

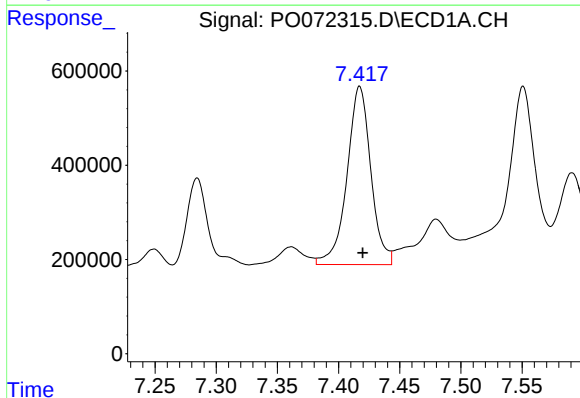


#29 AR-1254-4

R.T.: 7.417 min
Delta R.T.: -0.002 min
Response: 5142821
Conc: 882.74 ng/ml

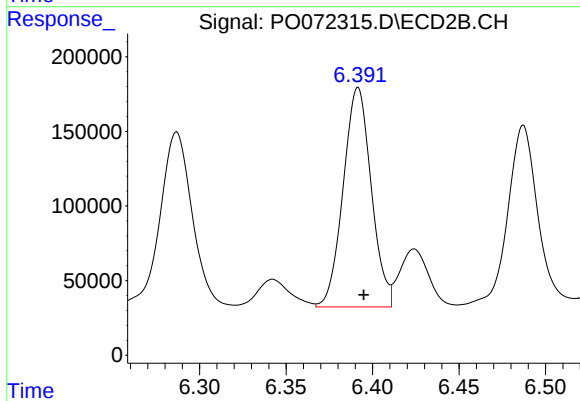

#29 AR-1254-4

R.T.: 6.392 min
Delta R.T.: -0.003 min
Response: 1653615
Conc: 681.01 ng/ml

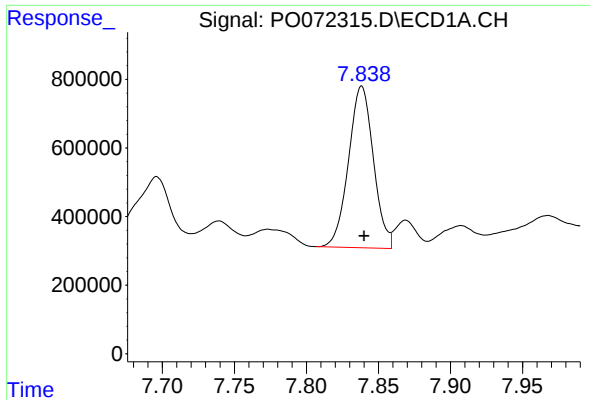


#30 AR-1254-5

R.T.: 7.838 min
Delta R.T.: -0.002 min
Response: 5673970
Conc: 1054.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HD-4

Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:38 PM

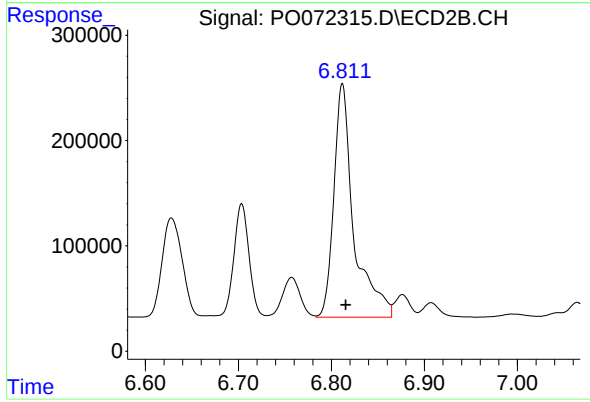

#30 AR-1254-5

R.T.: 6.812 min
Delta R.T.: -0.004 min
Response: 3292537
Conc: 1006.24 ng/ml