

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101320\
 Data File : PO072330.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2020 20:26
 Operator : DD\AJ
 Sample : L4375-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:30:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.508	1972566	1009049	27.463	26.939
2) SA Decachlor...	9.929	8.677	1721359	875468	15.634	15.392

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101320\
Data File : PO072330.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2020 20:26
Operator : DD\AJ
Sample : L4375-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:30:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

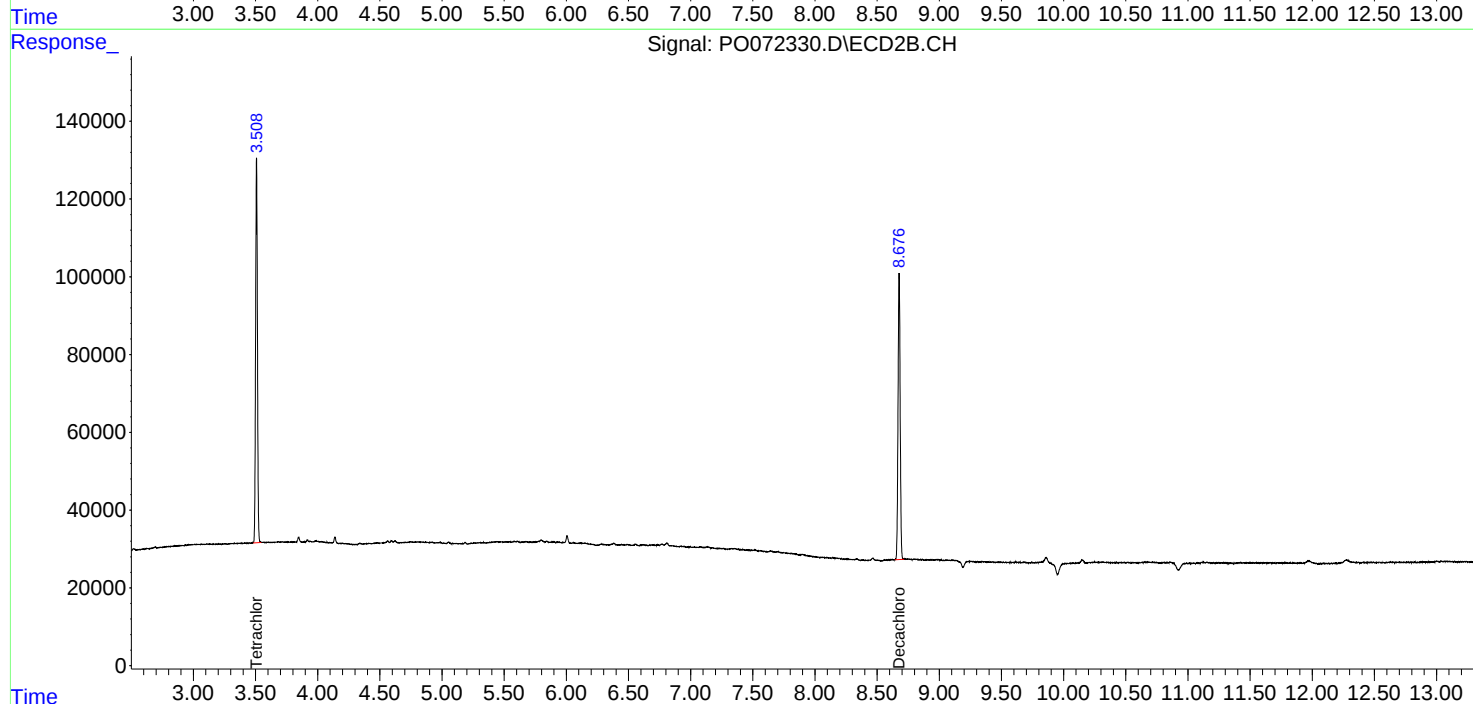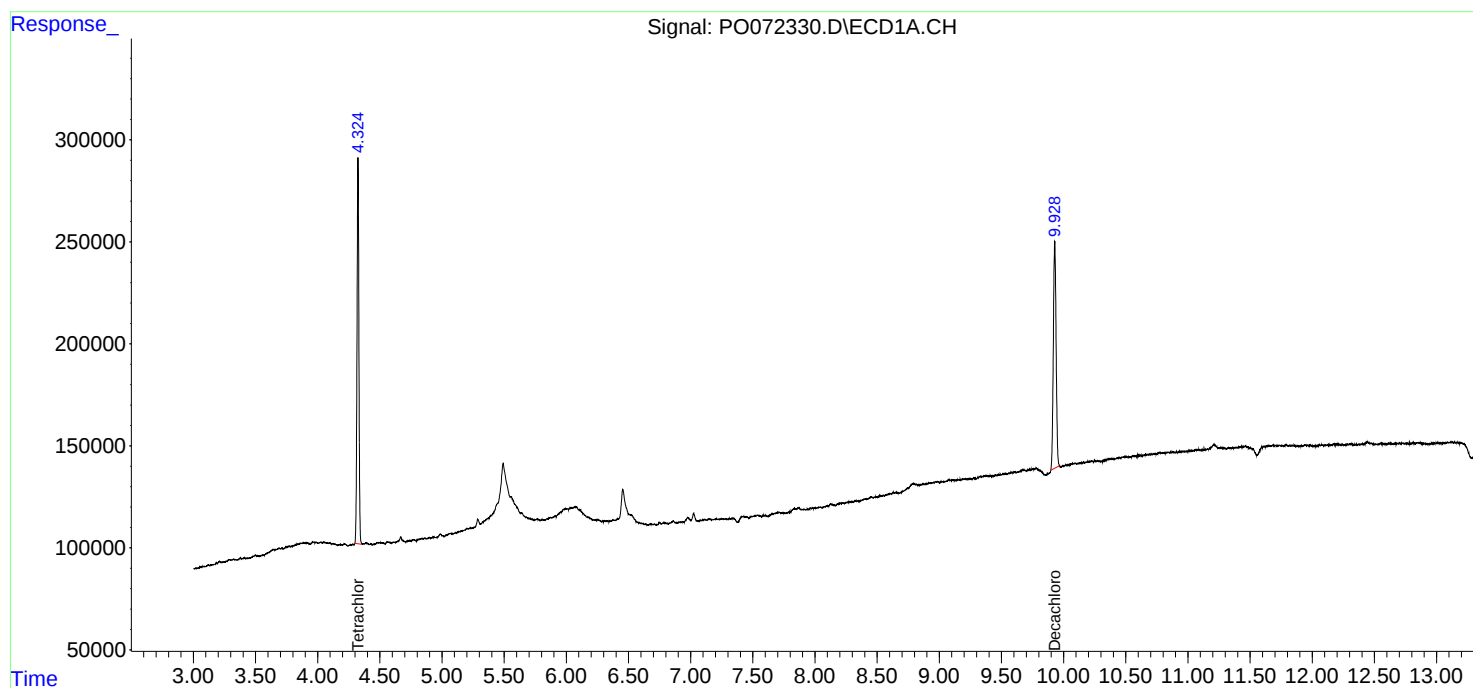


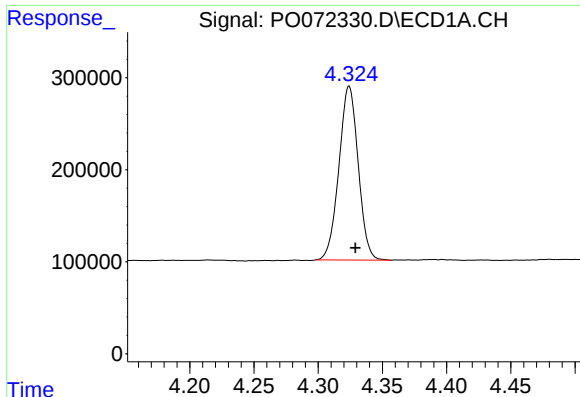

#1 Tetrachloro-m-xylene


R.T.: 4.324 min
Delta R.T.: -0.005 min
Response: 1972566
Conc: 27.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4

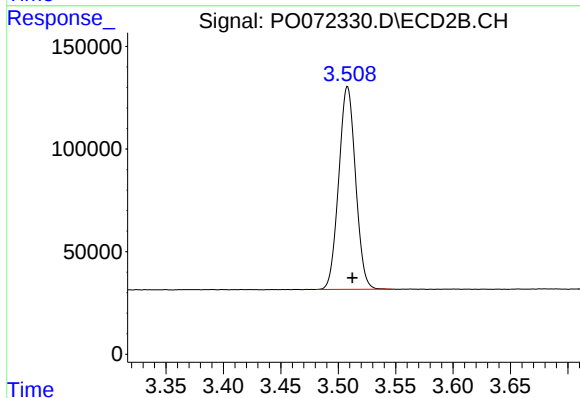


#1 Tetrachloro-m-xylene

R.T.: 3.508 min
Delta R.T.: -0.004 min
Response: 1009049
Conc: 26.94 ng/ml

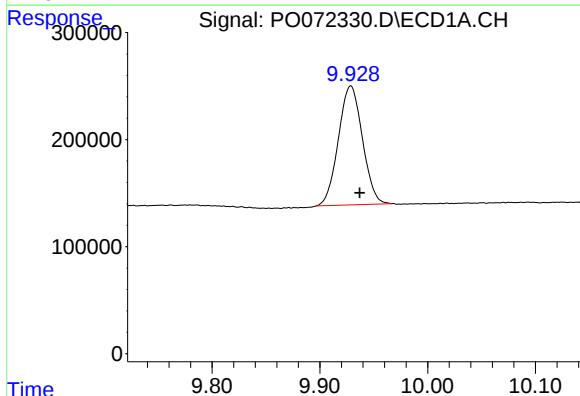

#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.008 min
Response: 1721359
Conc: 15.63 ng/ml

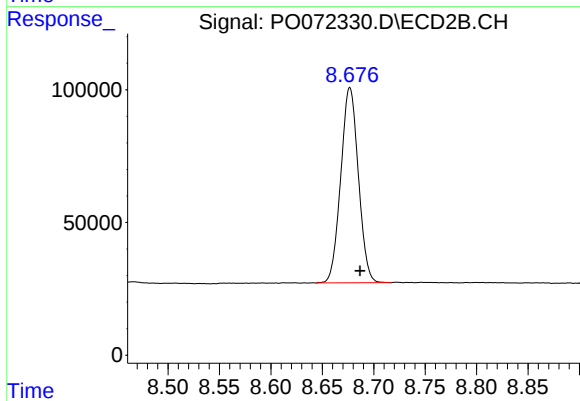

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.010 min
Response: 875468
Conc: 15.39 ng/ml