

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101320\
 Data File : PO072334.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2020 22:08
 Operator : DD\AJ
 Sample : L4369-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-3

Manual Integrations
 APPROVED

Ankita
 10/14/2020 12:02:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:31:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 05 11:48:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.323	3.508	1855061	945082	25.827	25.232
2) SA Decachlor...	9.929	8.676	1627986	830483	14.786	14.601m
Target Compounds						
26) L6 AR-1254-1	6.516	5.579	1385854	789180	396.666	330.223
27) L6 AR-1254-2	6.744	5.740	2148448	796050	390.235	372.166
28) L6 AR-1254-3	7.120	6.149	2918126	1633888	505.288	481.241
29) L6 AR-1254-4	7.416	6.389	2069876	792036	355.285	326.186
30) L6 AR-1254-5	7.836	6.810	3493587	1838647	649.141	561.915

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101320\
Data File : PO072334.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2020 22:08
Operator : DD\AJ
Sample : L4369-06
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-3


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:31:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100320.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 05 11:48:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

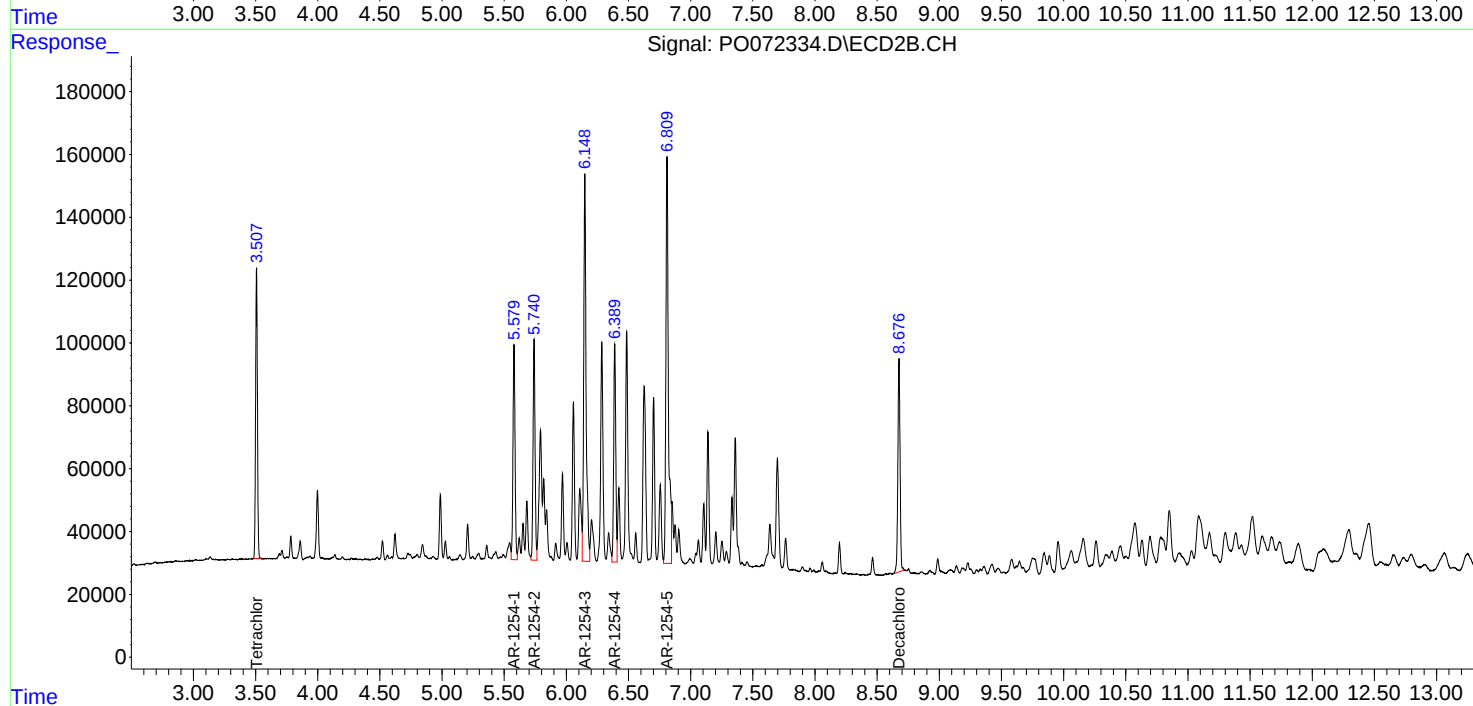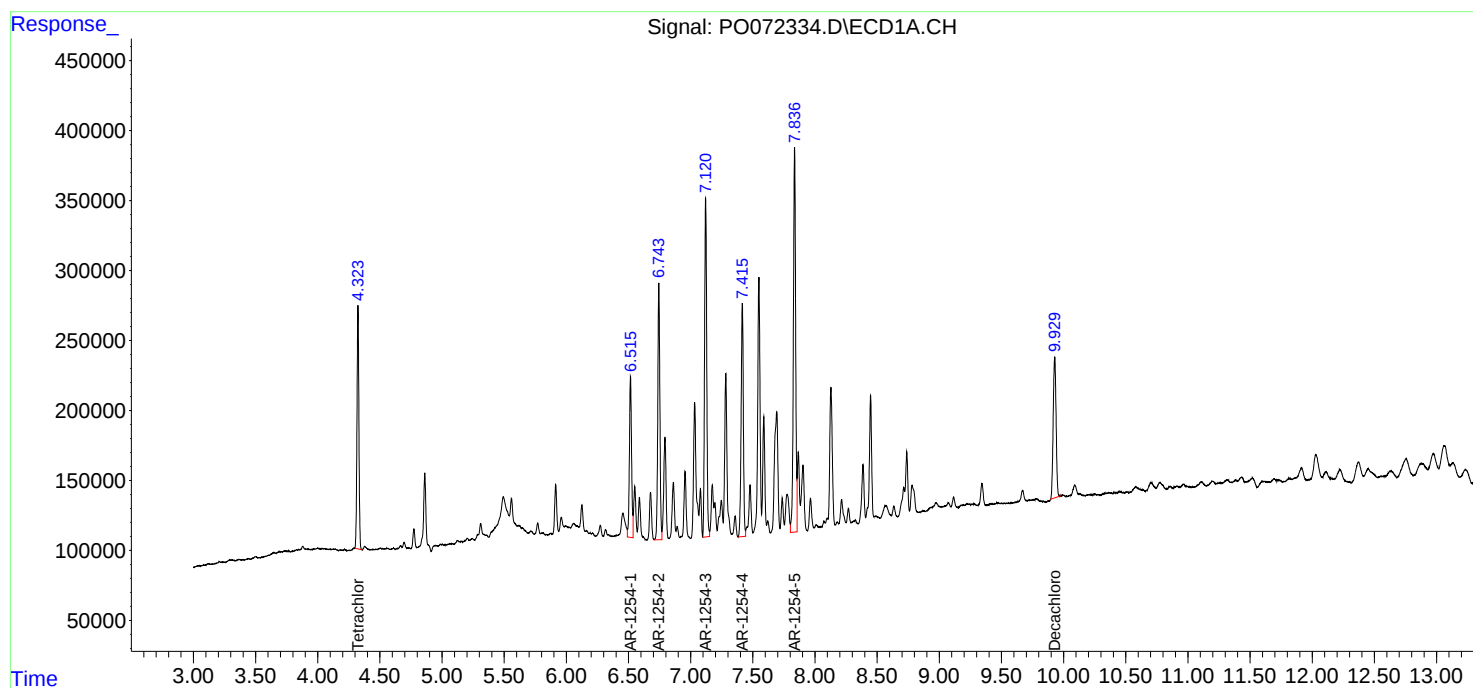

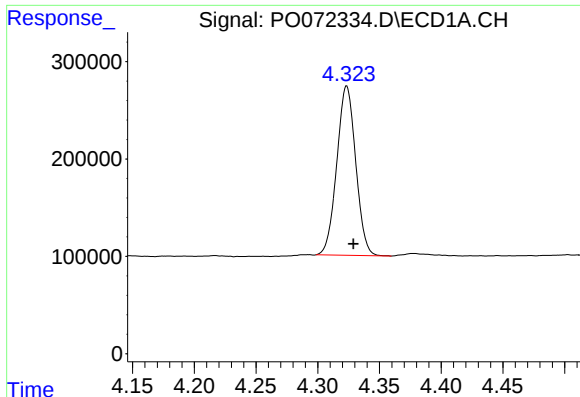


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.006 min
Response: 1855061
Conc: 25.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-3


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:44 PM

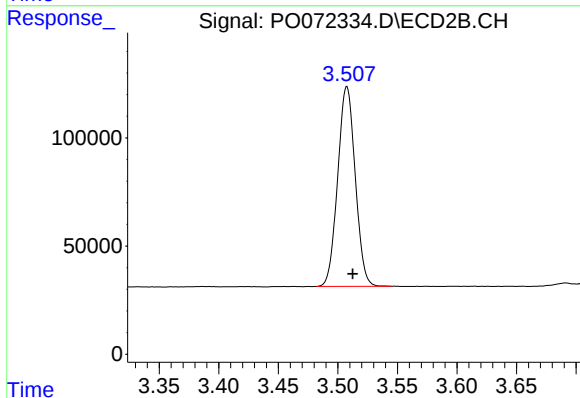


#1 Tetrachloro-m-xylene

R.T.: 3.508 min
Delta R.T.: -0.005 min
Response: 945082
Conc: 25.23 ng/ml

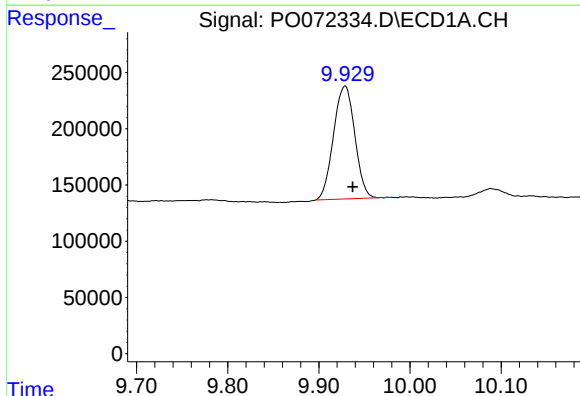


#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.008 min
Response: 1627986
Conc: 14.79 ng/ml

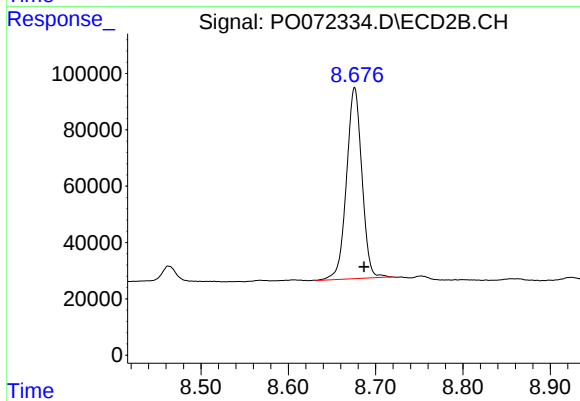

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.011 min
Response: 830483
Conc: 14.60 ng/ml m

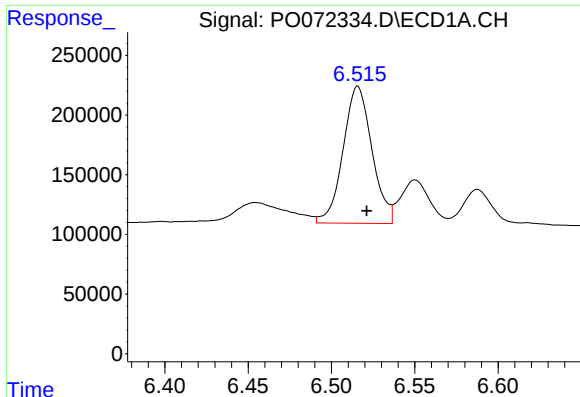


#26 AR-1254-1

R.T.: 6.516 min
Delta R.T.: -0.005 min
Response: 1385854
Conc: 396.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-3


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:44 PM

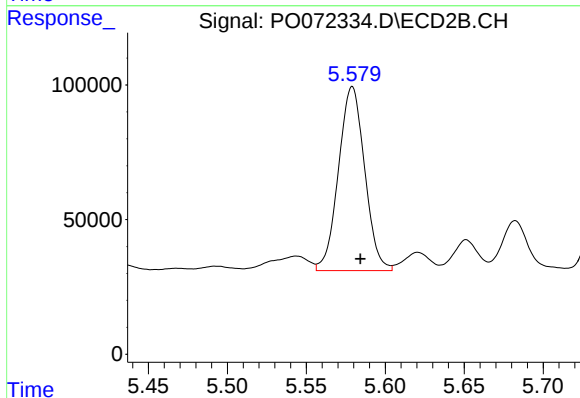


#26 AR-1254-1

R.T.: 5.579 min
Delta R.T.: -0.005 min
Response: 789180
Conc: 330.22 ng/ml

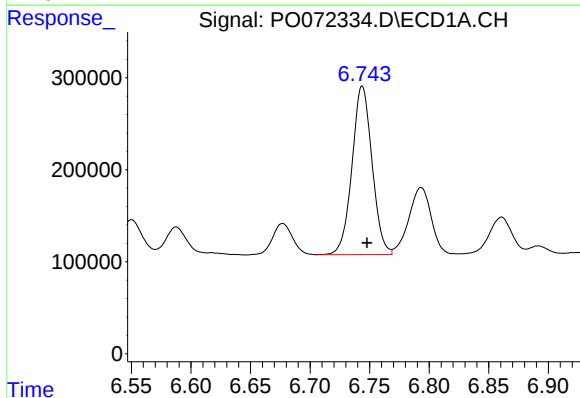


#27 AR-1254-2

R.T.: 6.744 min
Delta R.T.: -0.004 min
Response: 2148448
Conc: 390.23 ng/ml

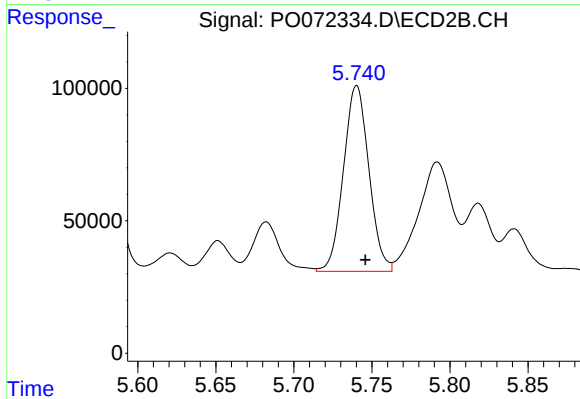

#27 AR-1254-2

R.T.: 5.740 min
Delta R.T.: -0.006 min
Response: 796050
Conc: 372.17 ng/ml

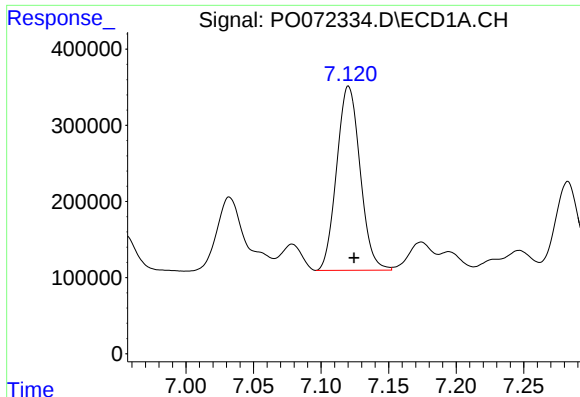


#28 AR-1254-3

R.T.: 7.120 min
Delta R.T.: -0.004 min
Response: 2918126
Conc: 505.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-3


Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:44 PM

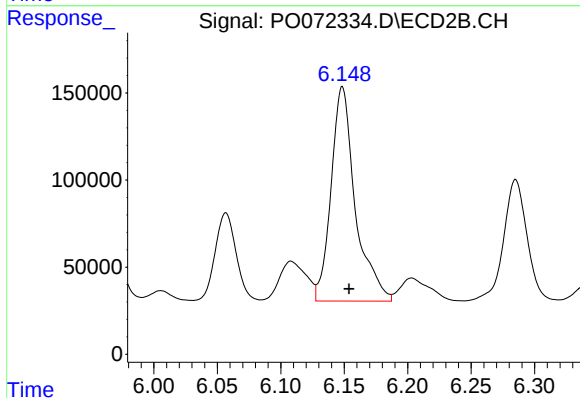


#28 AR-1254-3

R.T.: 6.149 min
Delta R.T.: -0.005 min
Response: 1633888
Conc: 481.24 ng/ml

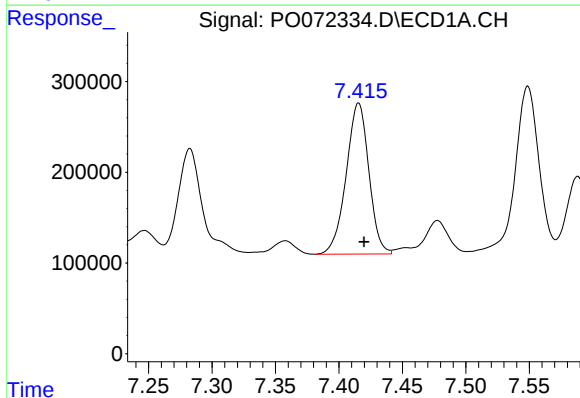


#29 AR-1254-4

R.T.: 7.416 min
Delta R.T.: -0.004 min
Response: 2069876
Conc: 355.29 ng/ml

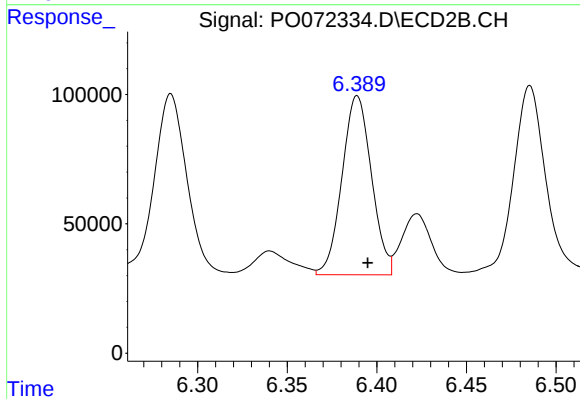

#29 AR-1254-4

R.T.: 6.389 min
Delta R.T.: -0.006 min
Response: 792036
Conc: 326.19 ng/ml

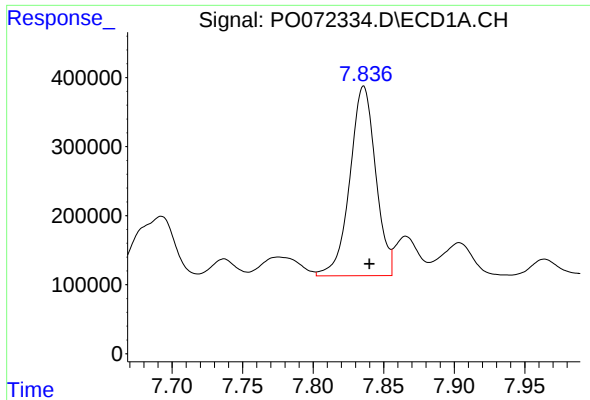


#30 AR-1254-5

R.T.: 7.836 min
Delta R.T.: -0.004 min
Response: 3493587
Conc: 649.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-3

Manual Integrations
APPROVED

Ankita
10/14/2020 12:02:44 PM

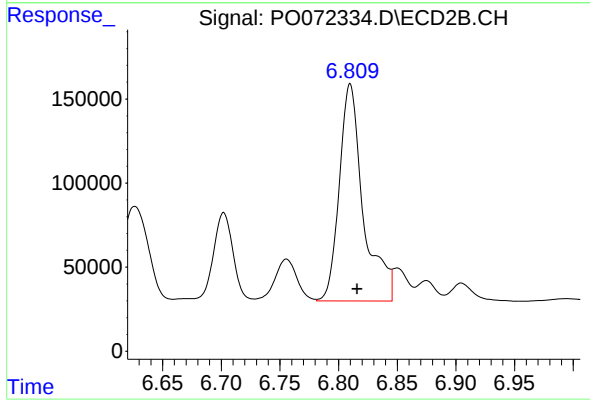

#30 AR-1254-5

R.T.: 6.810 min
Delta R.T.: -0.006 min
Response: 1838647
Conc: 561.91 ng/ml