

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101321\
 Data File : P0082039.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2021 15:40
 Operator : AJ\MA
 Sample : M4175-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31123

Manual Integrations
 APPROVED

mohammad
 10/14/2021 2:18:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:50:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 06:41:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.987	3.974	88045	45210	1.576	1.669
2) SA Decachlor...	11.112	9.305	68384	46008	1.886m	1.924

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101321\
Data File : P0082039.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2021 15:40
Operator : AJ\MA
Sample : M4175-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31123


Manual Integrations
APPROVED

mohammad
10/14/2021 2:18:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:50:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 06:41:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

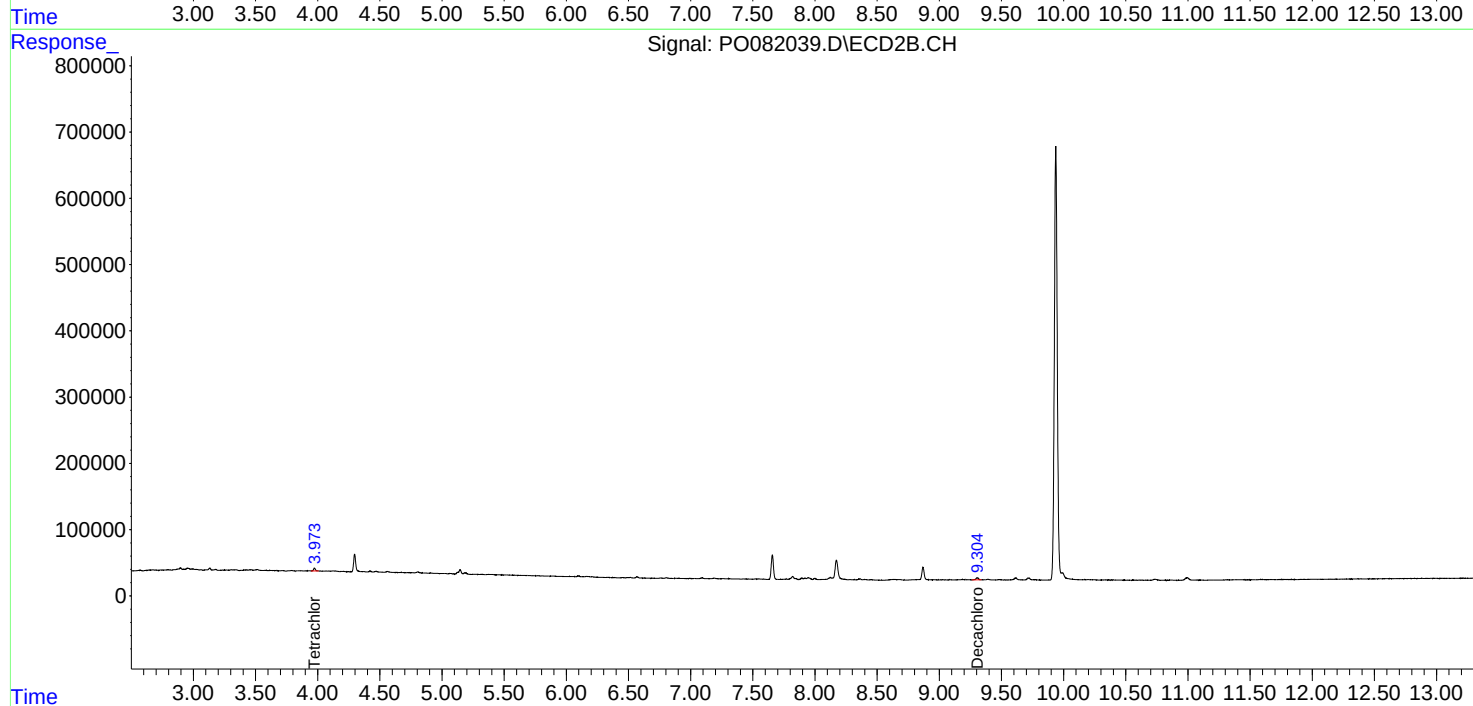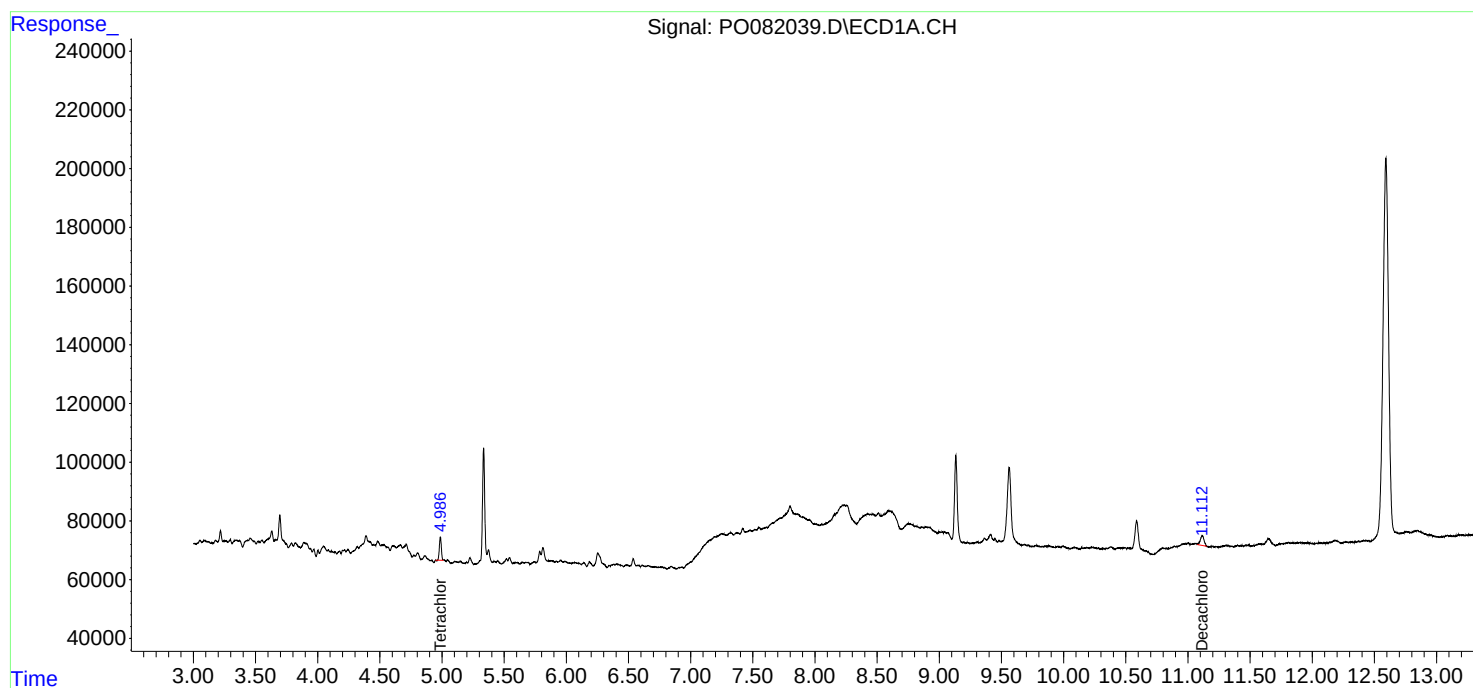

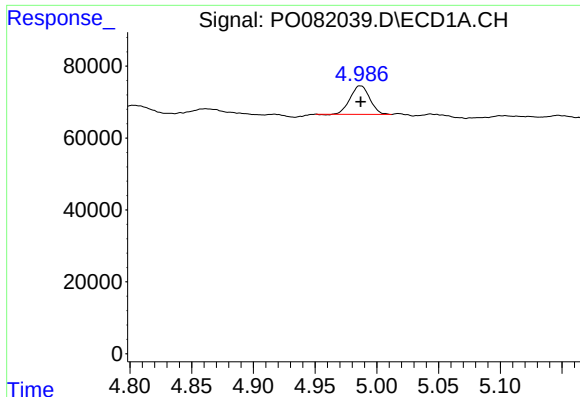


#1 Tetrachloro-m-xylene

R.T.: 4.987 min
Delta R.T.: 0.000 min
Response: 88045
Conc: 1.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
31123


Manual Integrations
APPROVED

mohammad
10/14/2021 2:18:44 PM

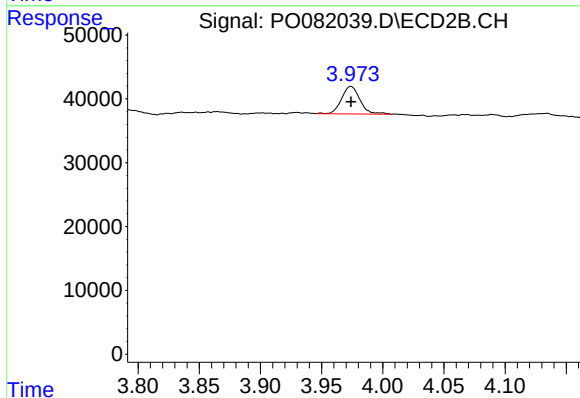


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: 0.000 min
Response: 45210
Conc: 1.67 ng/ml

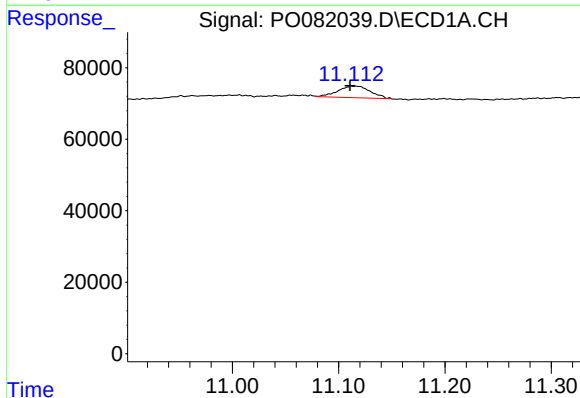

#2 Decachlorobiphenyl

R.T.: 11.112 min
Delta R.T.: 0.001 min
Response: 68384
Conc: 1.89 ng/ml m

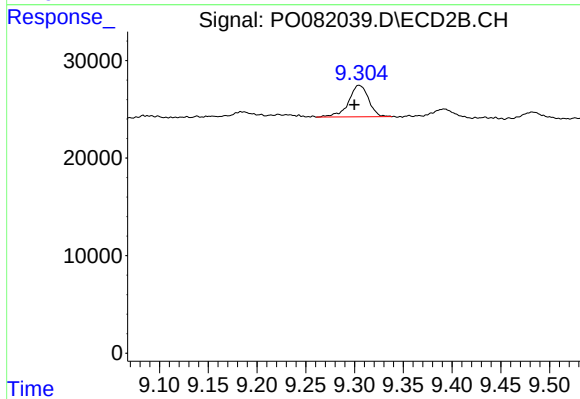

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: 0.005 min
Response: 46008
Conc: 1.92 ng/ml