

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101323\
 Data File : P0098817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 19:21
 Operator : YP/AJ
 Sample : PB156370BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB156370BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/17/2023
 Supervised By :Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:06:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.633	37866983	14855153	19.721	19.073
2) SA Decachlor...	10.286	8.635	26698518	11190302	21.995	20.887m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101323\
Data File : PO098817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 19:21
Operator : YP/AJ
Sample : PB156370BL
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB156370BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:06:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

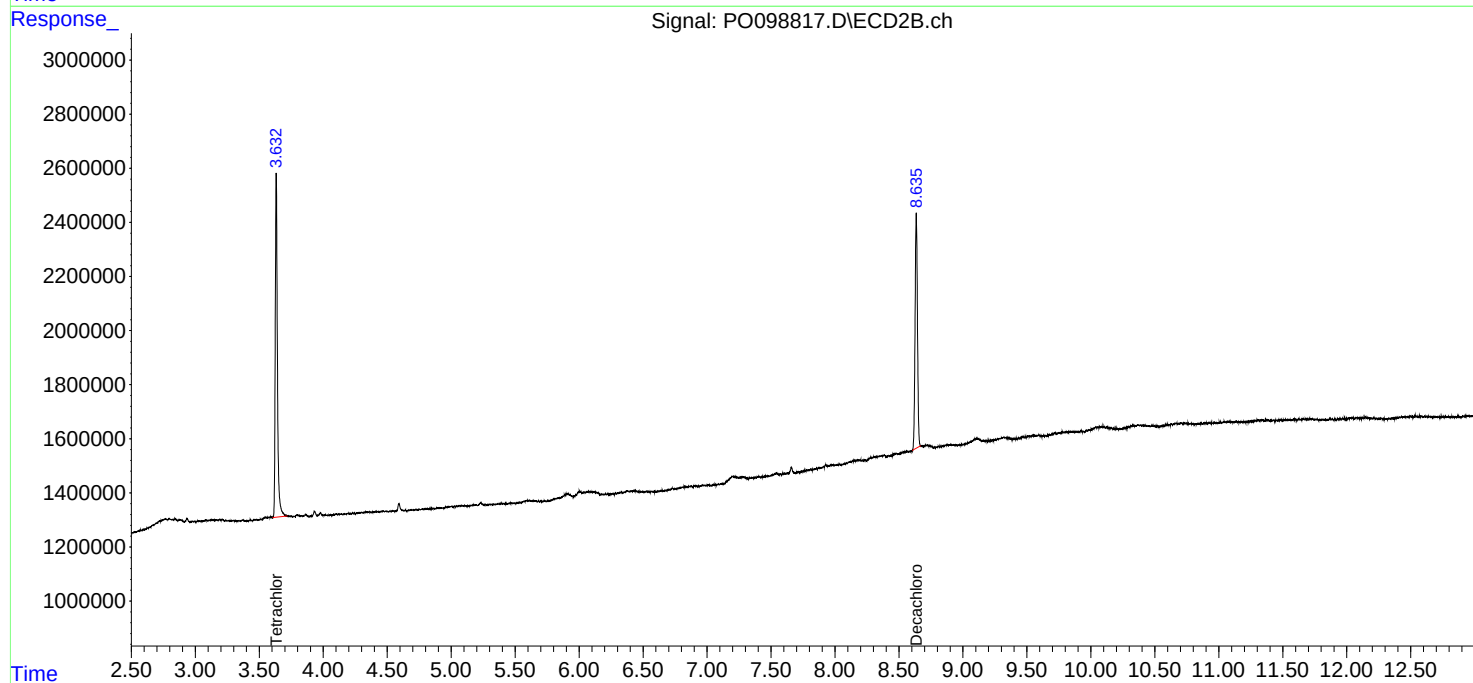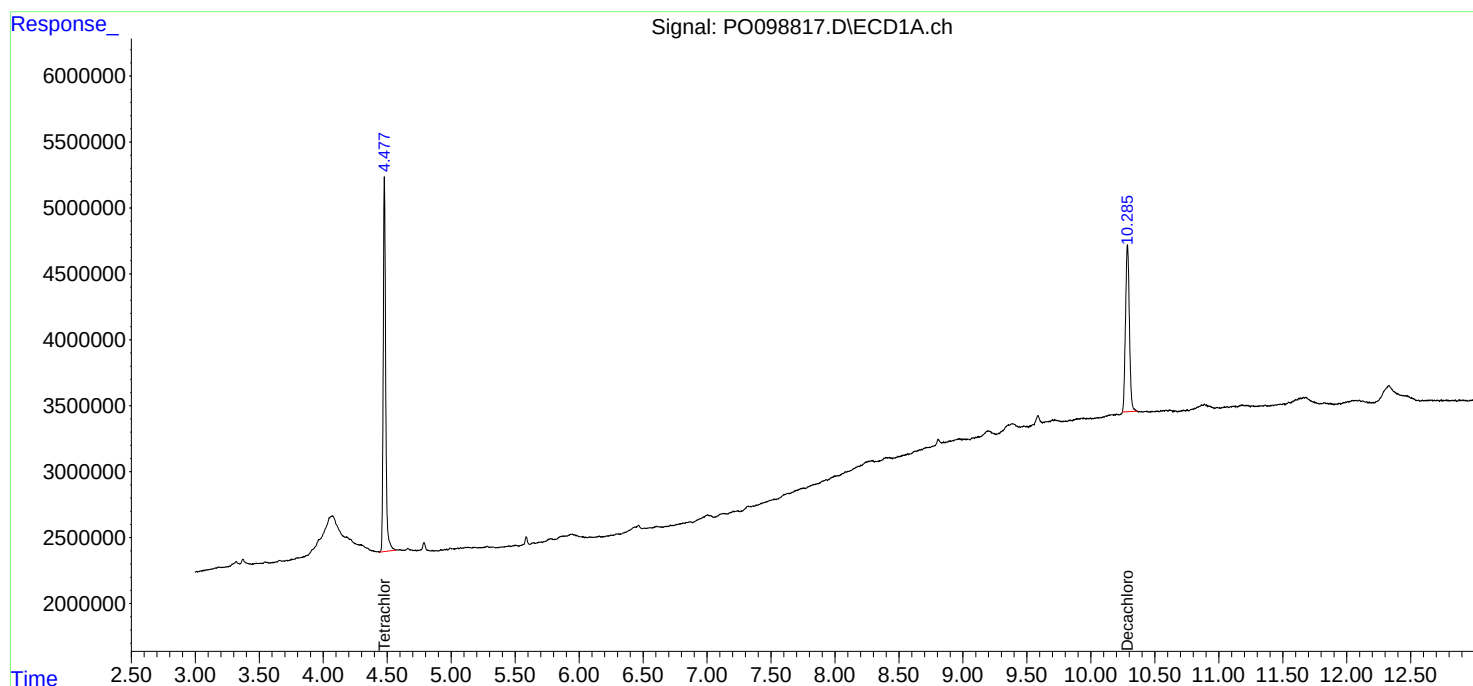

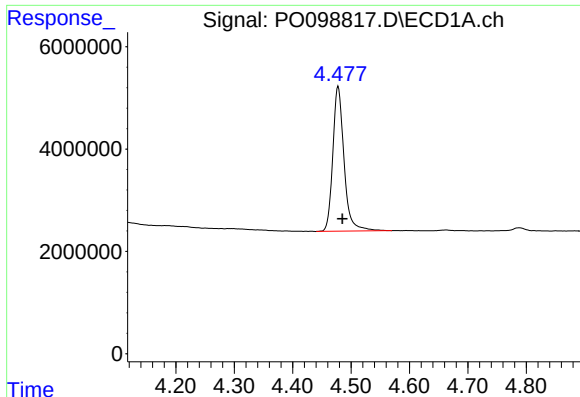


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.007 min
Response: 37866983
Conc: 19.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB156370BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

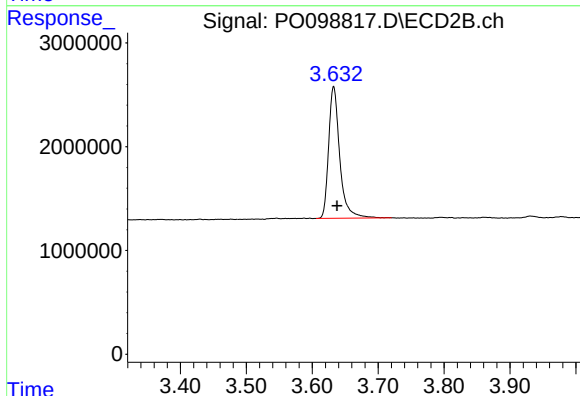


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.005 min
Response: 14855153
Conc: 19.07 ng/ml

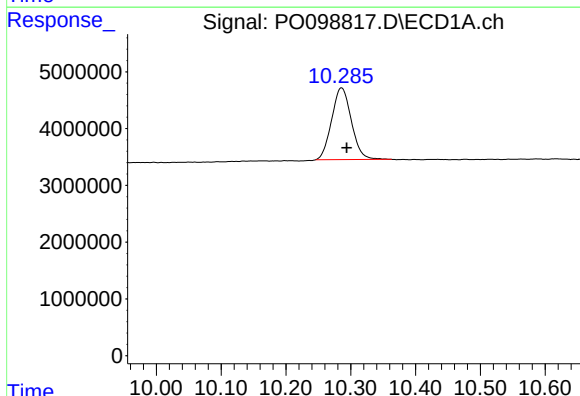

#2 Decachlorobiphenyl

R.T.: 10.286 min
Delta R.T.: -0.008 min
Response: 26698518
Conc: 21.99 ng/ml

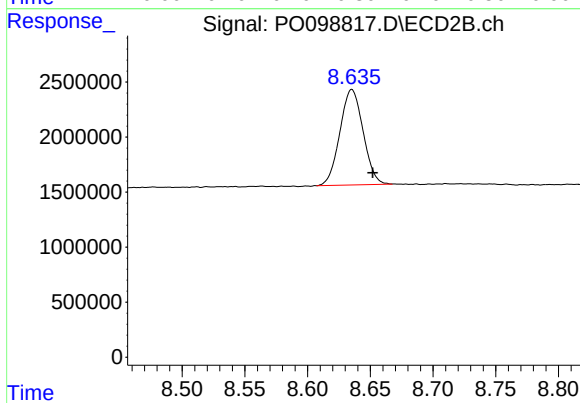

#2 Decachlorobiphenyl

R.T.: 8.635 min
Delta R.T.: -0.017 min
Response: 11190302
Conc: 20.89 ng/ml m