

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101323\
 Data File : PO098820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 20:12
 Operator : YP/AJ
 Sample : 04859-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SVS-GROUNDWATER

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/17/2023
 Supervised By :Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 02:08:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	3.633	40742454	14792212	21.218	18.992
2) SA Decachlor...	10.285	8.634	23308582	9874625	19.202m	18.431m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101323\
Data File : P0098820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 20:12
Operator : YP/AJ
Sample : 04859-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SVS-GROUNDWATER


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 10/17/2023
Supervised By : Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 02:08:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

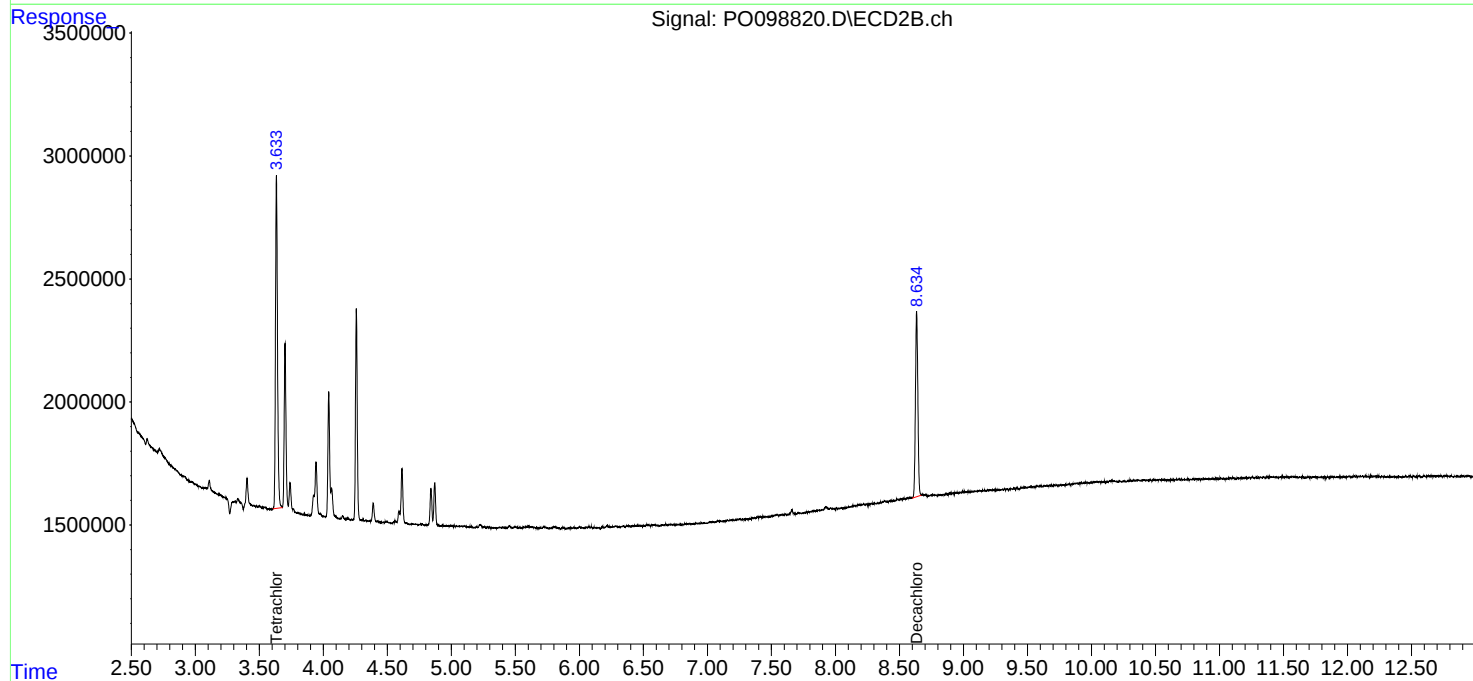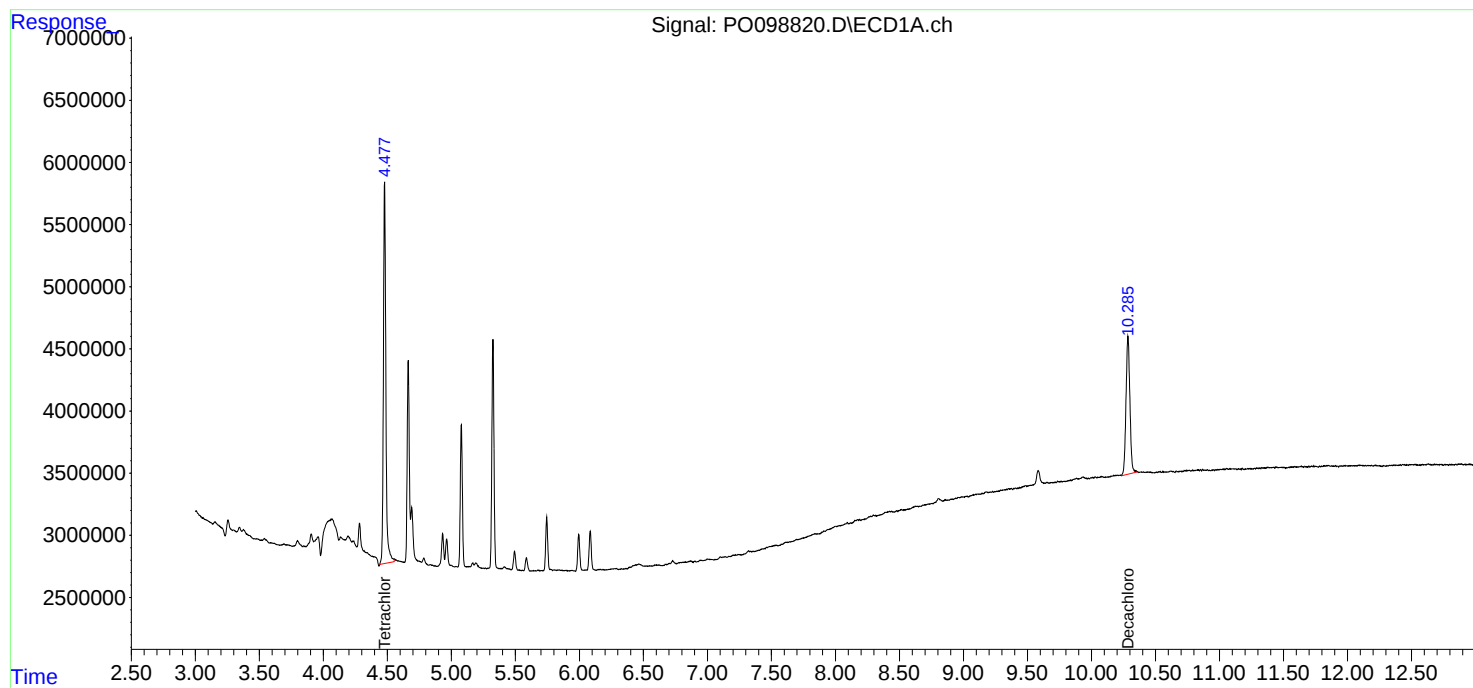

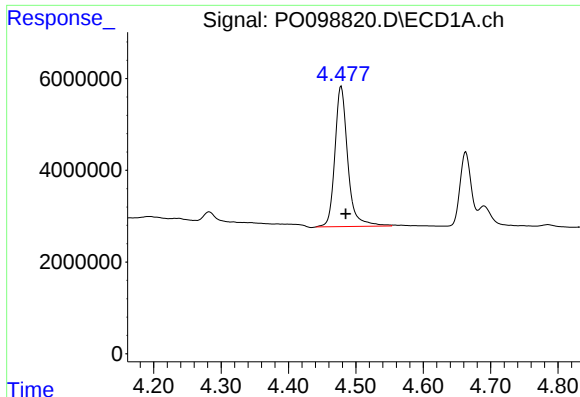

#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.007 min
Response: 40742454
Conc: 21.22 ng/ml

Instrument :

ECD_O


ClientSampleId :

SVS-GROUNDWATER

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

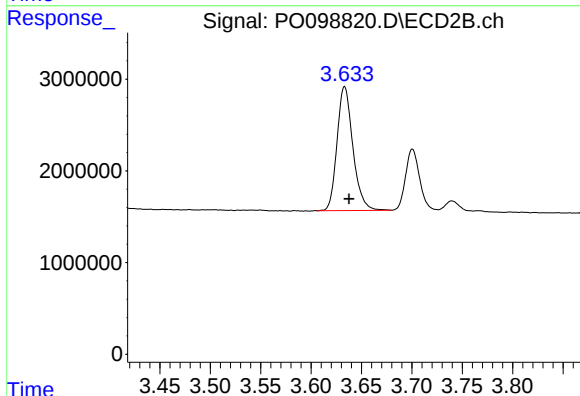


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.004 min
Response: 14792212
Conc: 18.99 ng/ml

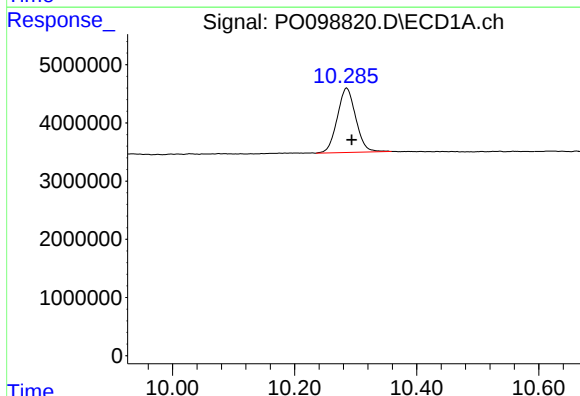

#2 Decachlorobiphenyl

R.T.: 10.285 min
Delta R.T.: -0.009 min
Response: 23308582
Conc: 19.20 ng/ml m

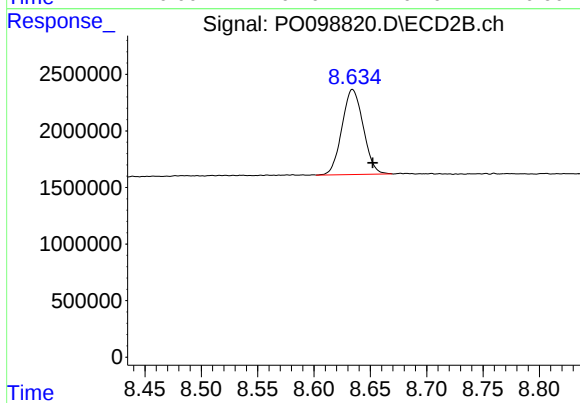

#2 Decachlorobiphenyl

R.T.: 8.634 min
Delta R.T.: -0.018 min
Response: 9874625
Conc: 18.43 ng/ml m