

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101424\
 Data File : P0107128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2024 20:32
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 03:35:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 04:48:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.374	3.645	216.1E6	72402699	18.012	18.152
2) SA Decachlor...	10.058	8.640	59767897	61183512	23.886	21.797

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101424\
Data File : PO107128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 20:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 03:35:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 04:48:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

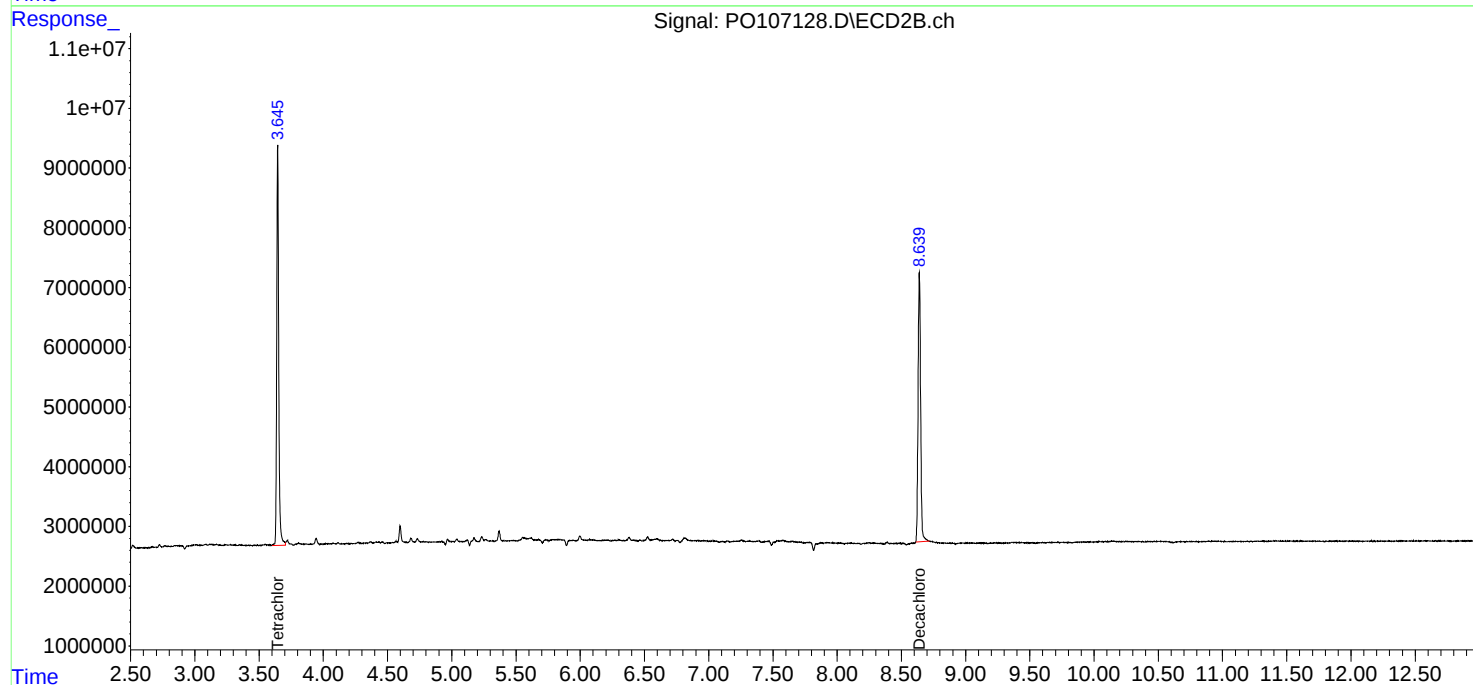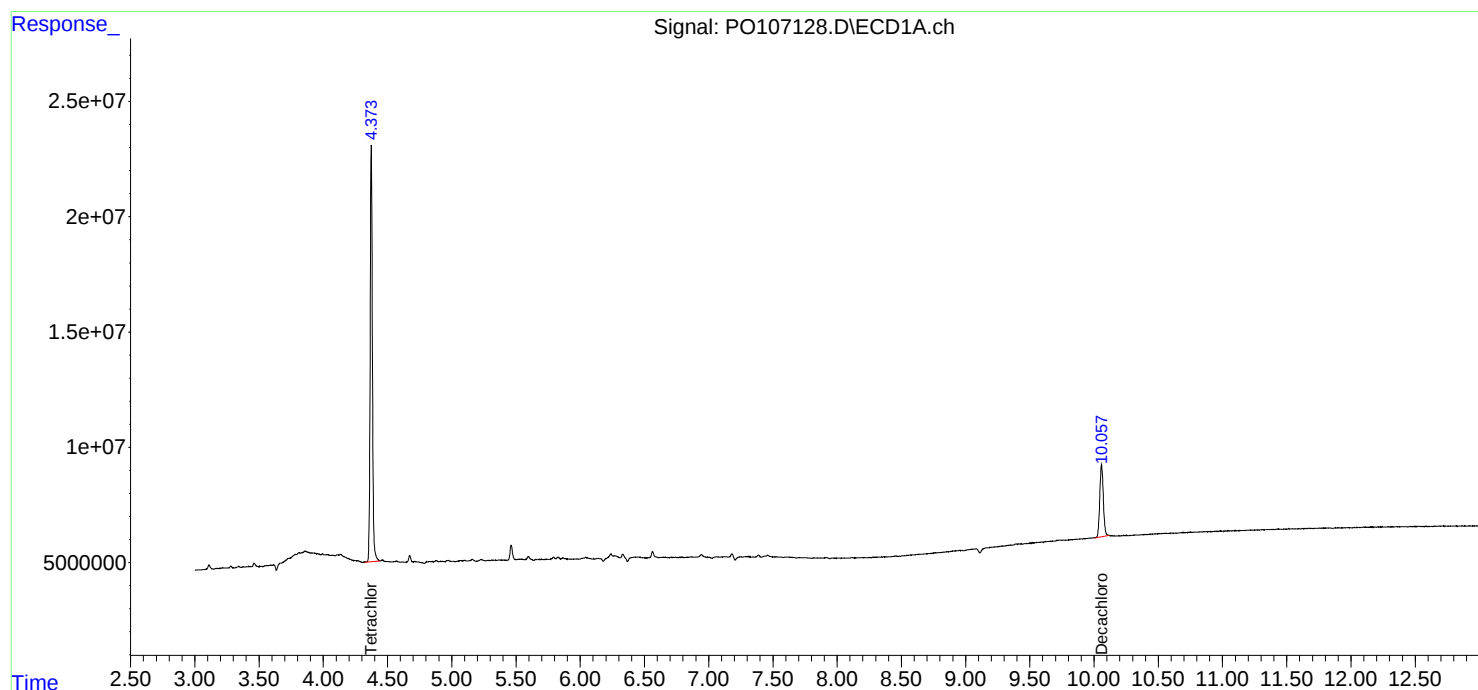


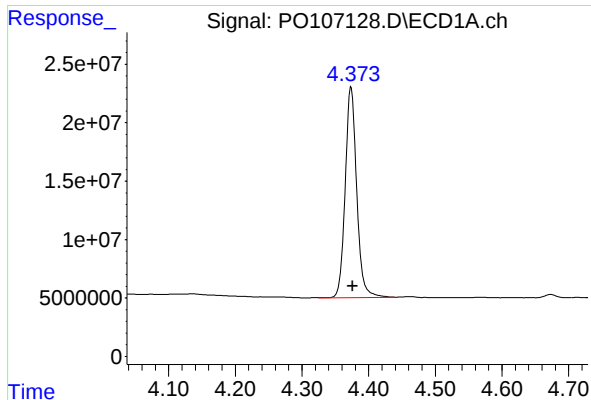

#1 Tetrachloro-m-xylene


R.T.: 4.374 min
Delta R.T.: -0.002 min
Response: 216085024
Conc: 18.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

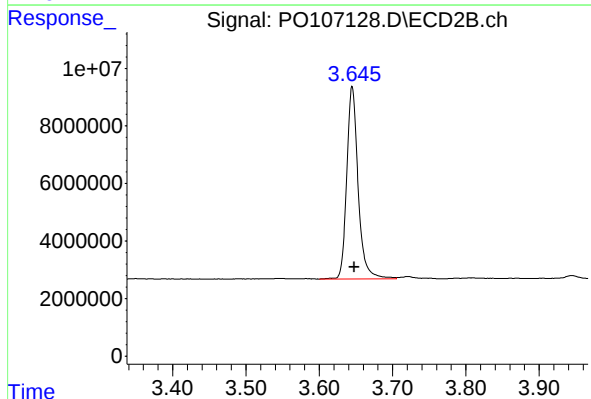


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.003 min
Response: 72402699
Conc: 18.15 ng/ml

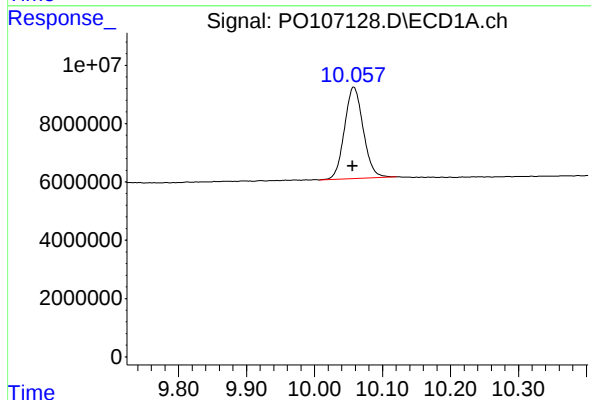

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: 0.002 min
Response: 59767897
Conc: 23.89 ng/ml

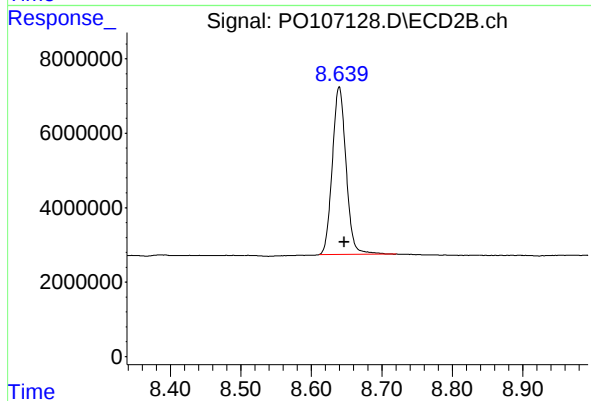

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.007 min
Response: 61183512
Conc: 21.80 ng/ml