

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101520\
 Data File : P0072378.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2020 13:43
 Operator : DD\AJ
 Sample : L4392-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 14:02:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.320	3.503	1835302	958161	21.638	22.747
2)	SA Decachlor...	9.923	8.672	2063687	969760	18.709	18.759
Target Compounds							
9)	L2 AR-1221-2	0.000	3.842	0	14284	N.D.	37.311 #
33)	L7 AR-1260-3	7.921f	0.000	206113	0	32.161	N.D. #
36)	L8 AR-1262-1	7.921f	0.000	206113	0	21.733	N.D. #
39)	L8 AR-1262-4	8.790	0.000	77628	0	19.425	N.D. #
40)	L8 AR-1262-5	0.000	8.194	0	26440	N.D.	10.469 #
42)	L9 AR-1268-2	8.790	0.000	77628	0	4.702	N.D. #
44)	L9 AR-1268-4	0.000	8.194	0	26440	N.D.	9.353 #
45)	L9 AR-1268-5	0.000	8.459	0	10158	N.D.	0.529 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101520\
Data File : PO072378.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2020 13:43
Operator : DD\AJ
Sample : L4392-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 14:02:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

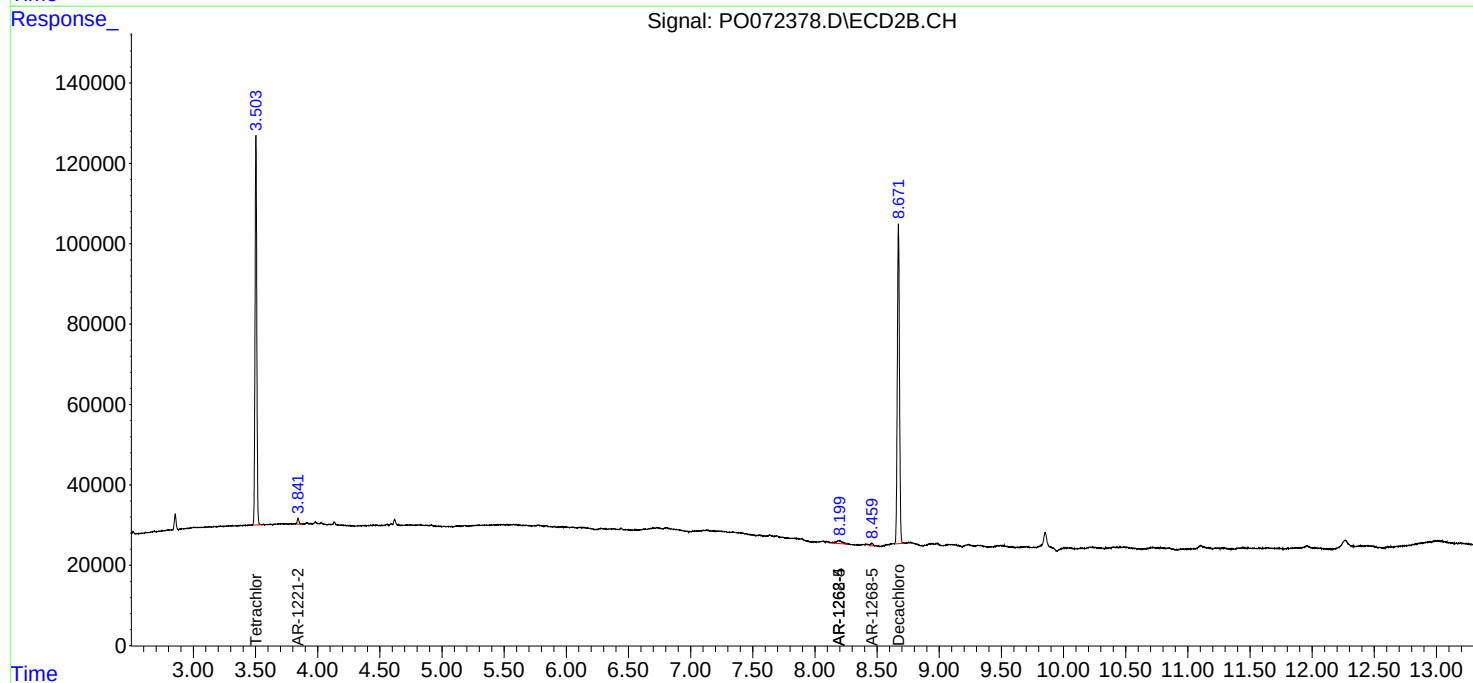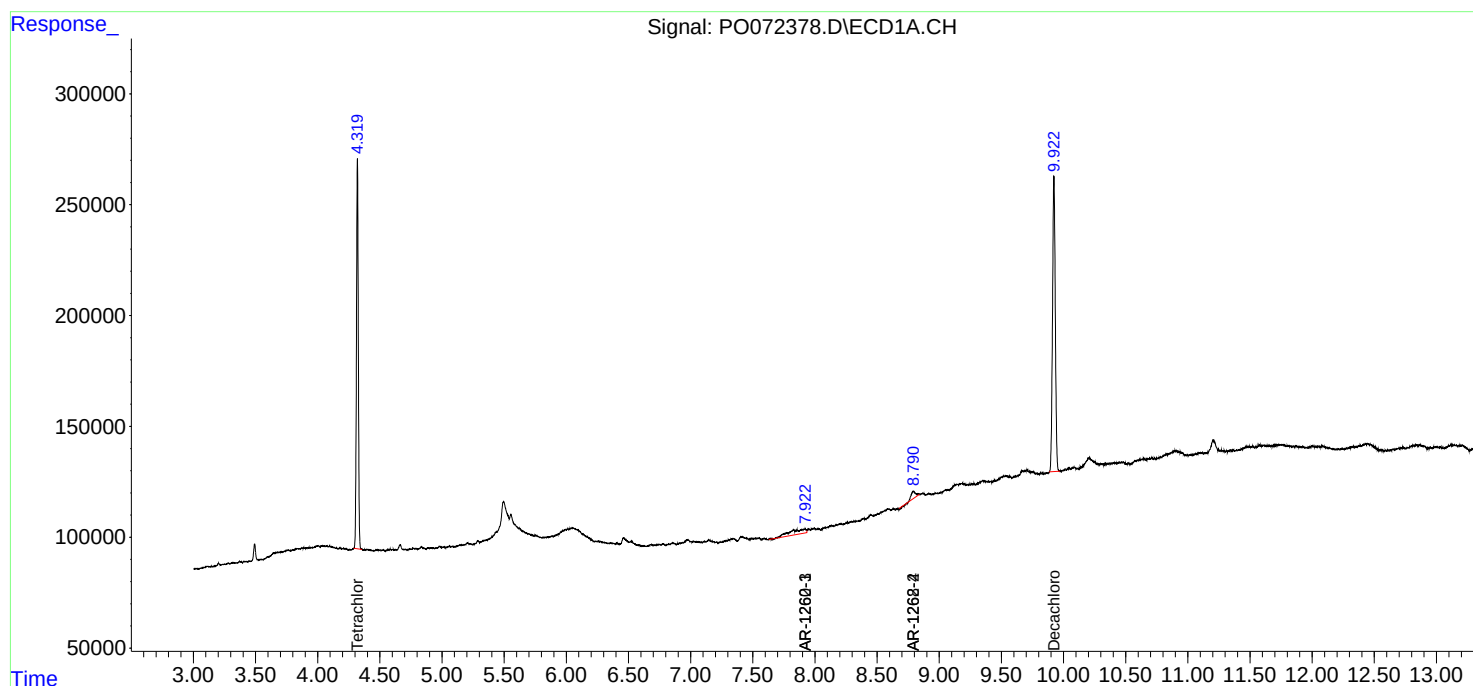


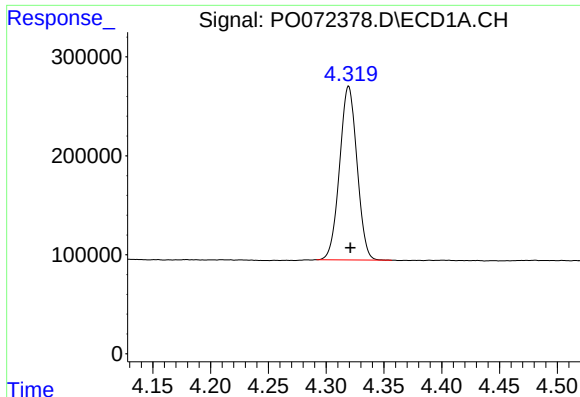

#1 Tetrachloro-m-xylene


R.T.: 4.320 min
Delta R.T.: -0.001 min
Response: 1835302
Conc: 21.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

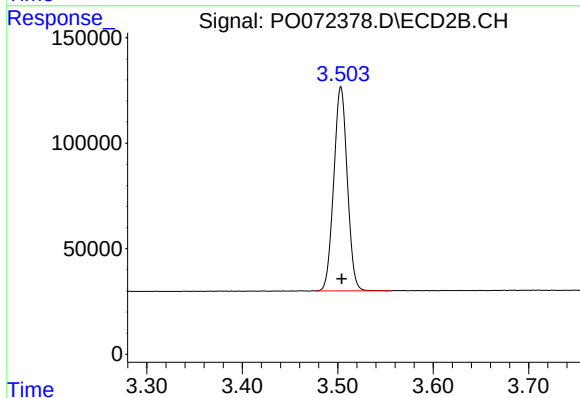


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 958161
Conc: 22.75 ng/ml

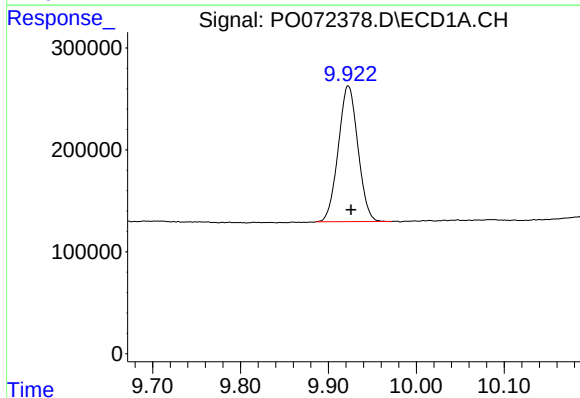


#2 Decachlorobiphenyl

R.T.: 9.923 min
Delta R.T.: -0.003 min
Response: 2063687
Conc: 18.71 ng/ml

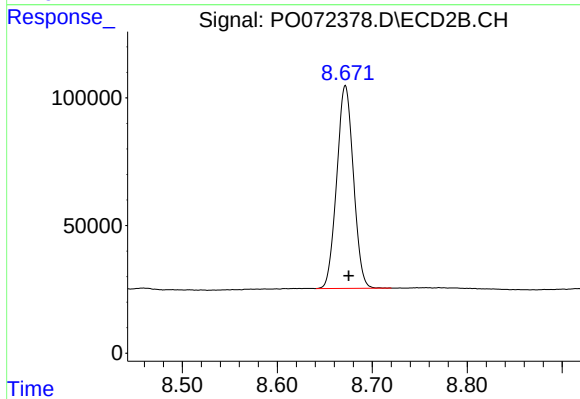

#2 Decachlorobiphenyl


R.T.: 8.672 min
Delta R.T.: -0.003 min
Response: 969760
Conc: 18.76 ng/ml

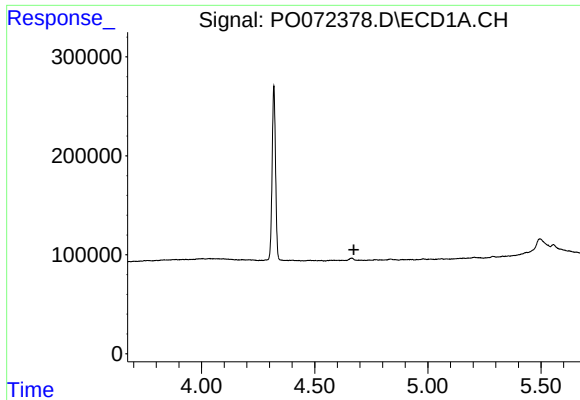

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

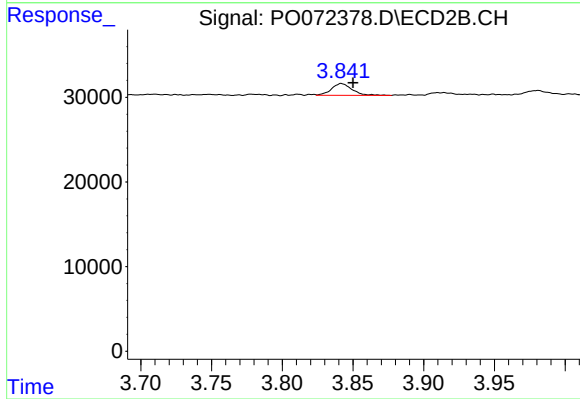


#9 AR-1221-2

R.T.: 3.842 min
Delta R.T.: -0.008 min
Response: 14284
Conc: 37.31 ng/ml

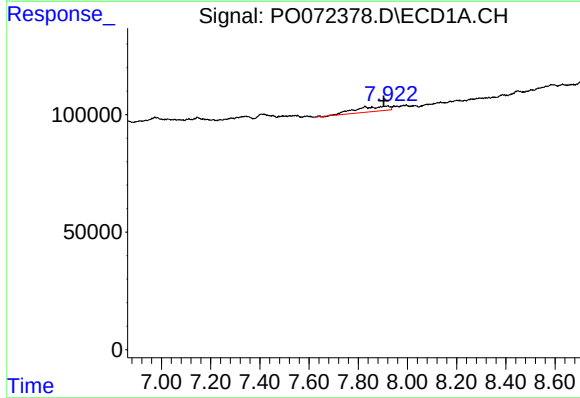


#33 AR-1260-3

R.T.: 7.921 min
Delta R.T.: 0.017 min
Response: 206113
Conc: 32.16 ng/ml

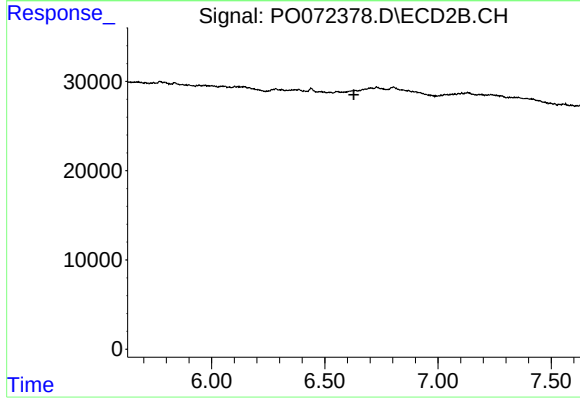

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 6.628 min
Response: 0
Conc: N.D.

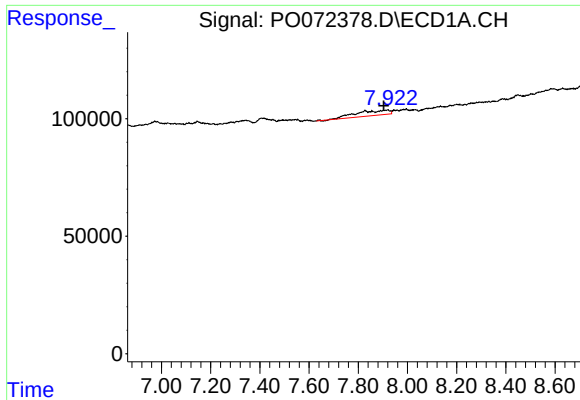

#36 AR-1262-1


R.T.: 7.921 min
Delta R.T.: 0.018 min
Response: 206113
Conc: 21.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

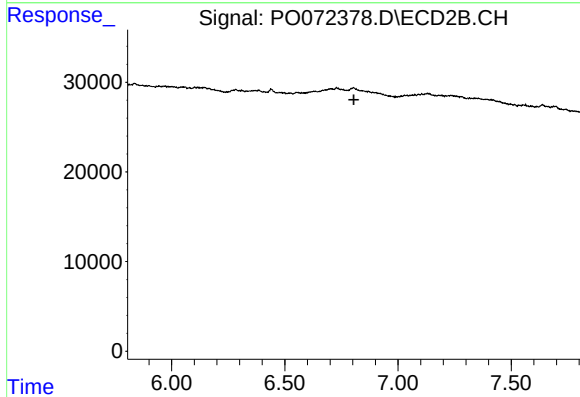


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

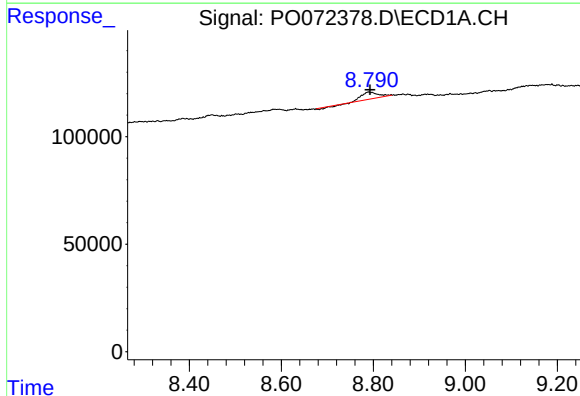


#39 AR-1262-4

R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 77628
Conc: 19.43 ng/ml

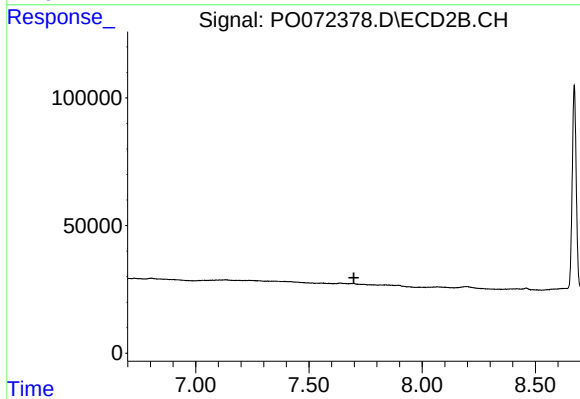

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.698 min
Response: 0
Conc: N.D.

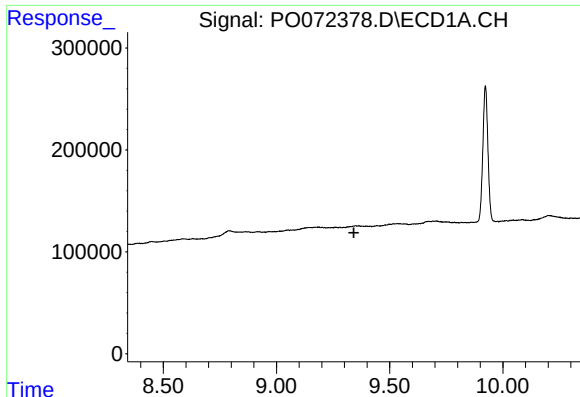

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

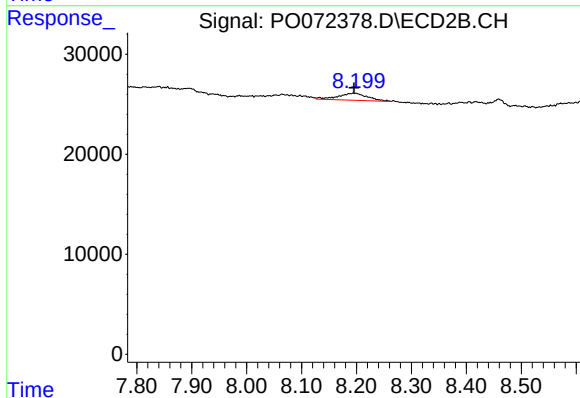


#40 AR-1262-5

R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 26440
Conc: 10.47 ng/ml

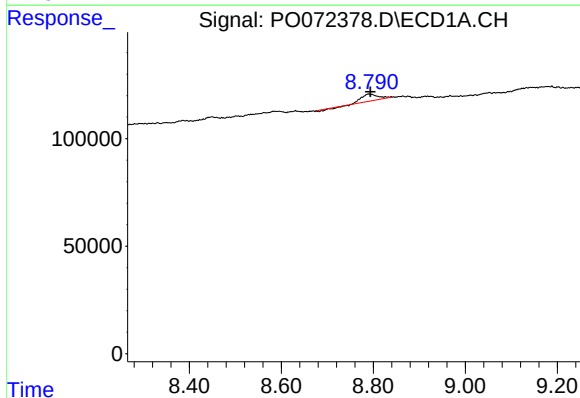


#42 AR-1268-2

R.T.: 8.790 min
Delta R.T.: -0.004 min
Response: 77628
Conc: 4.70 ng/ml

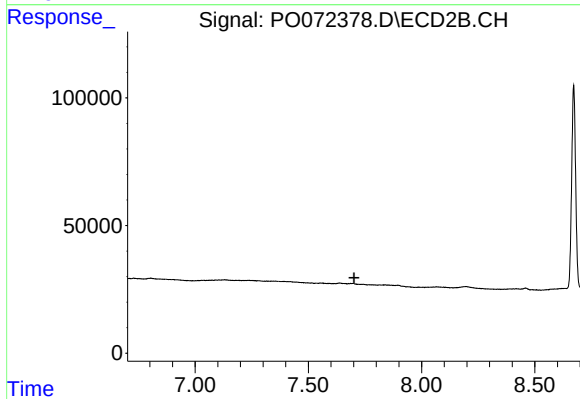

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 7.701 min
Response: 0
Conc: N.D.

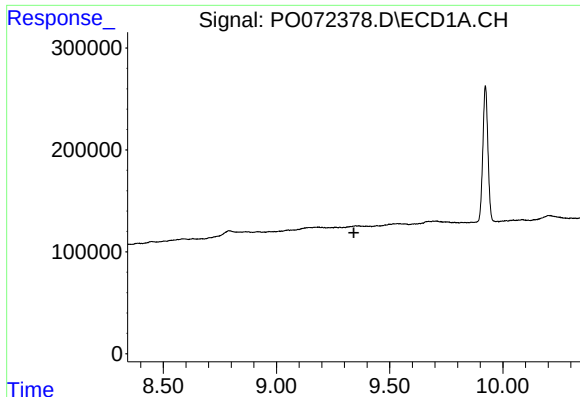

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

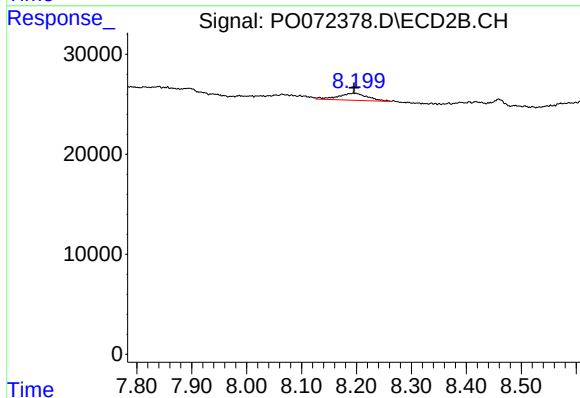


#44 AR-1268-4

R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 26440
Conc: 9.35 ng/ml

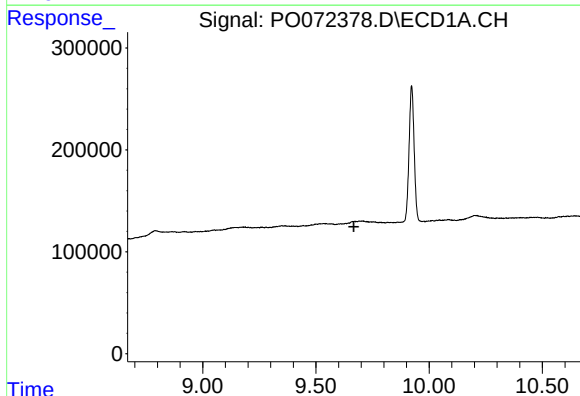

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.668 min
Response: 0
Conc: N.D.

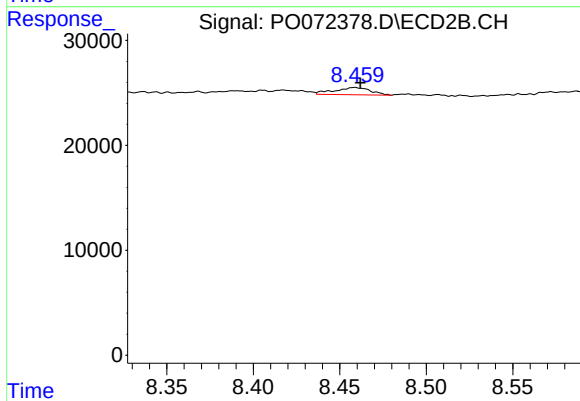

#45 AR-1268-5

R.T.: 8.459 min
Delta R.T.: -0.003 min
Response: 10158
Conc: 0.53 ng/ml