

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101520\
 Data File : PO072395.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2020 18:34
 Operator : DD\AJ
 Sample : L4403-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SHELL-L15-L14-NORTH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 00:58:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.321	3.505	1527522	809088	18.009	19.208
2) SA Decachlor...	9.925	8.673	1514097	655411	13.727	12.678

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101520\
Data File : PO072395.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2020 18:34
Operator : DD\AJ
Sample : L4403-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SHELL-L15-L14-NORTH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 00:58:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

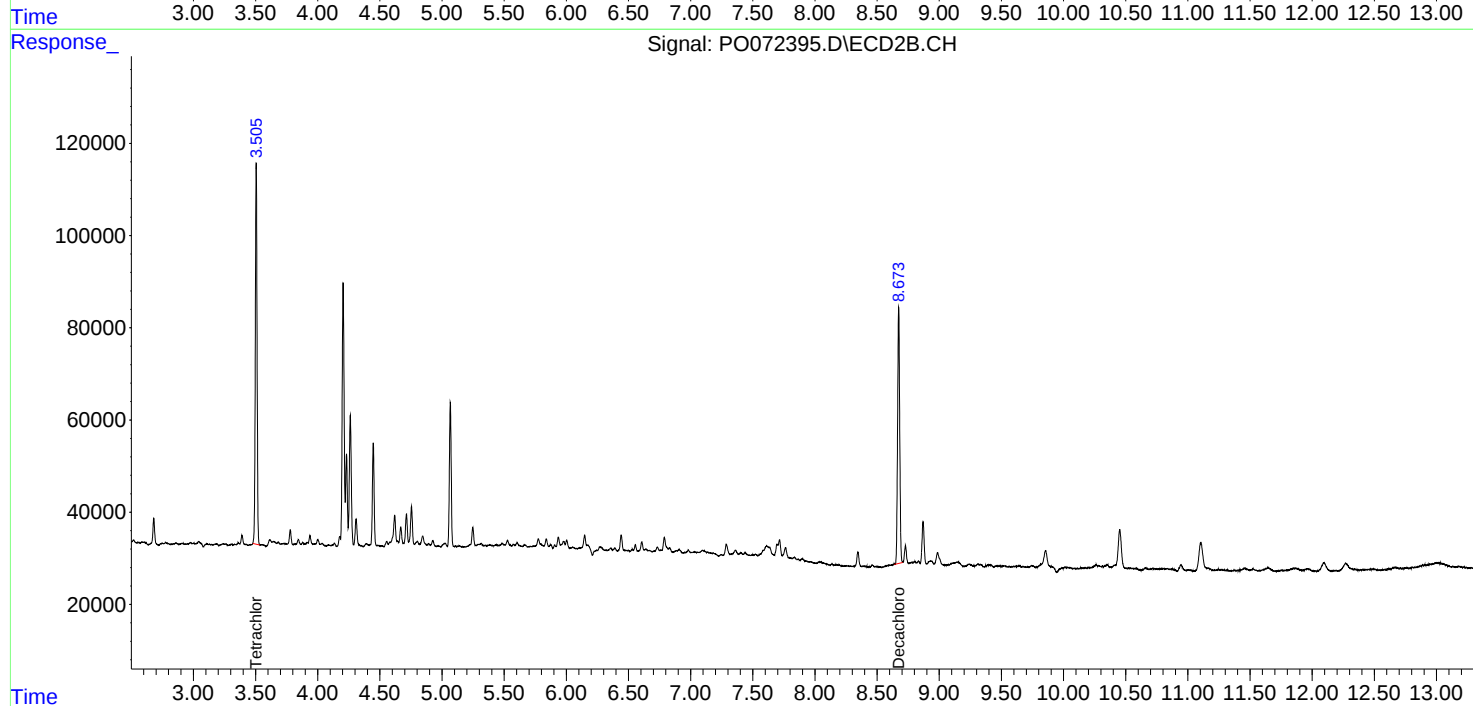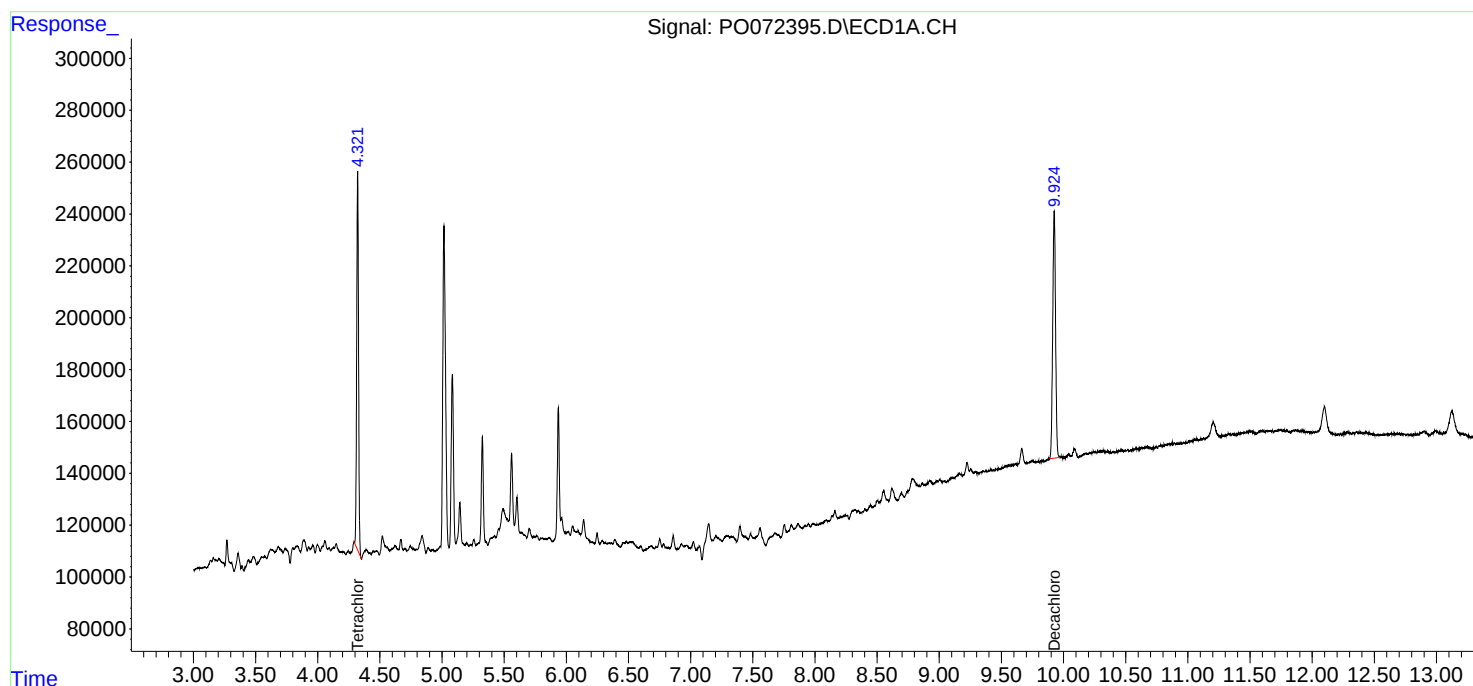


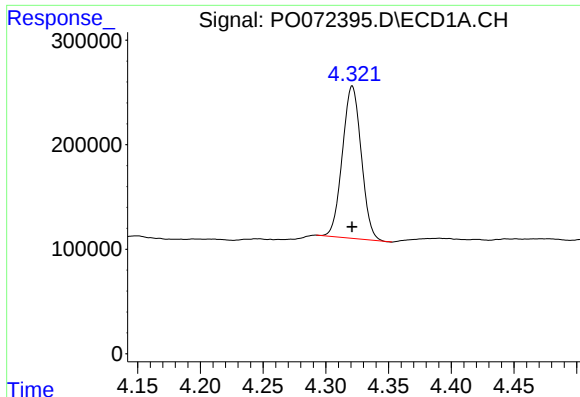

#1 Tetrachloro-m-xylene


R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 1527522
Conc: 18.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
SHELL-L15-L14-NORTH

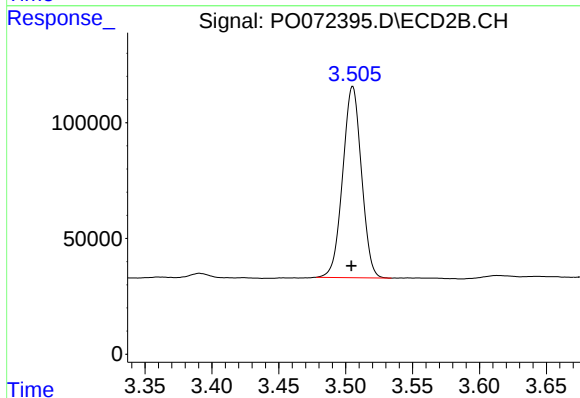


#1 Tetrachloro-m-xylene

R.T.: 3.505 min
Delta R.T.: 0.001 min
Response: 809088
Conc: 19.21 ng/ml

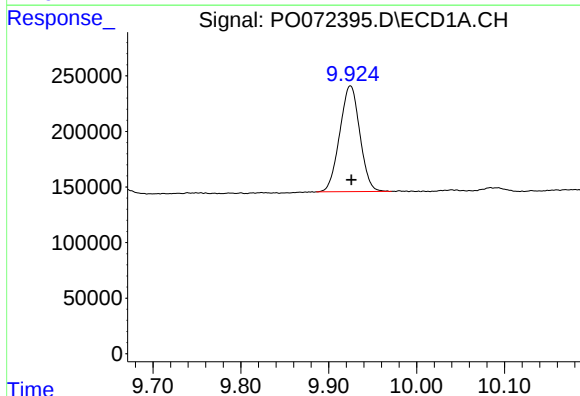

#2 Decachlorobiphenyl

R.T.: 9.925 min
Delta R.T.: -0.001 min
Response: 1514097
Conc: 13.73 ng/ml

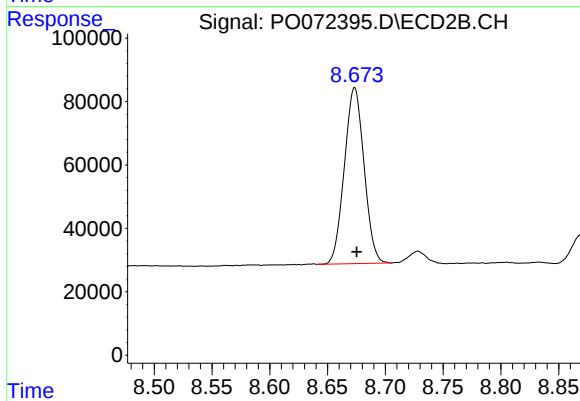

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.002 min
Response: 655411
Conc: 12.68 ng/ml