

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101520\
 Data File : P0072401.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2020 20:17
 Operator : DD\AJ
 Sample : L4404-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SHELL-L15-L14-NORTH

Manual Integrations
 APPROVED

Ankita
 10/16/2020 11:53:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:01:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.504	1783857	904936	21.031m	21.484
2) SA Decachlor...	9.924	8.673	2975861	930960	26.979	18.009 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101520\
Data File : PO072401.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2020 20:17
Operator : DD\AJ
Sample : L4404-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SHELL-L15-L14-NORTH


Manual Integrations
APPROVED

Ankita
10/16/2020 11:53:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:01:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

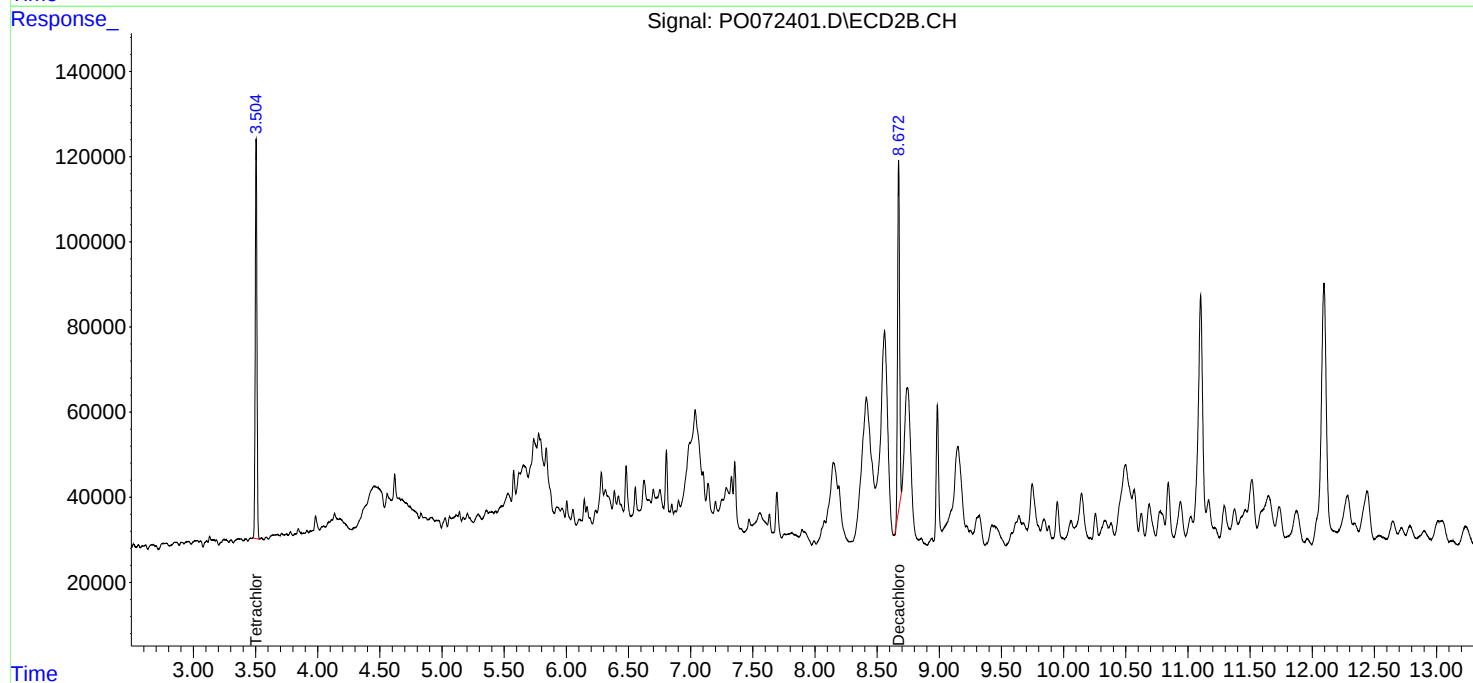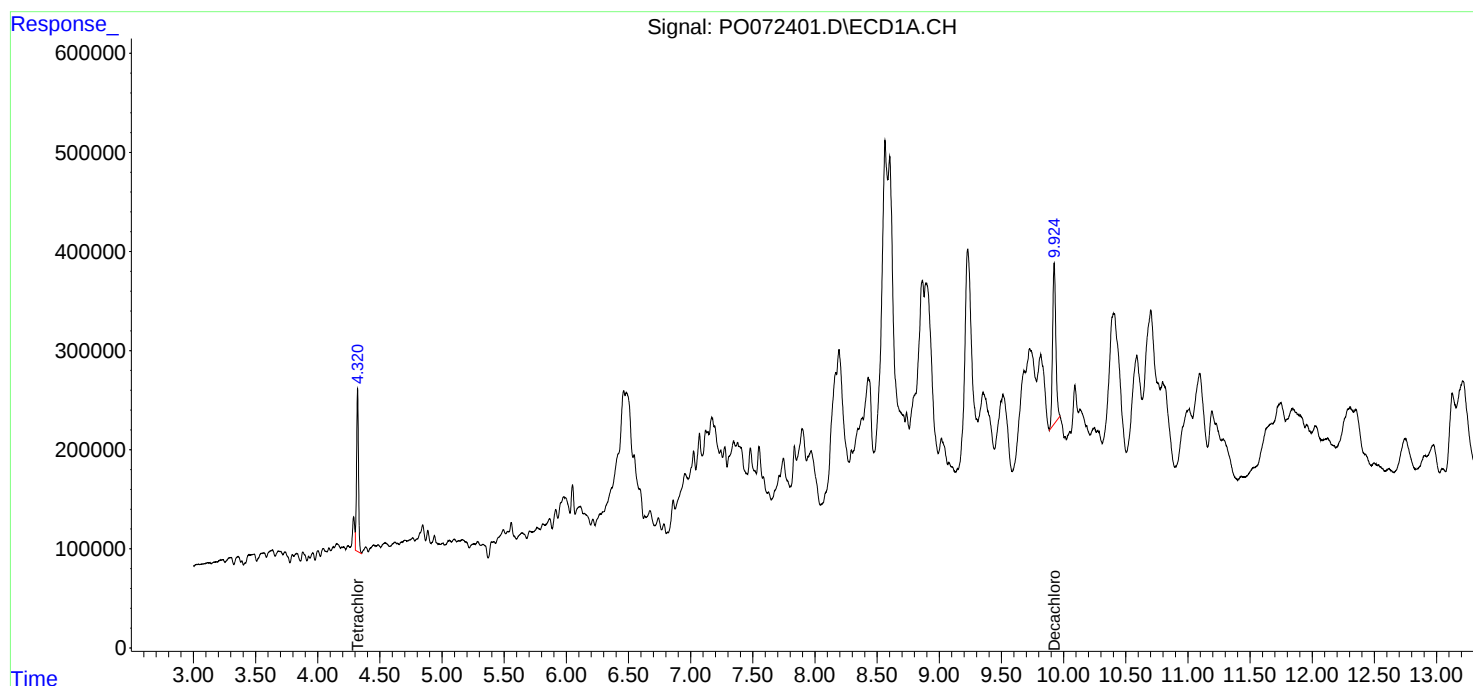

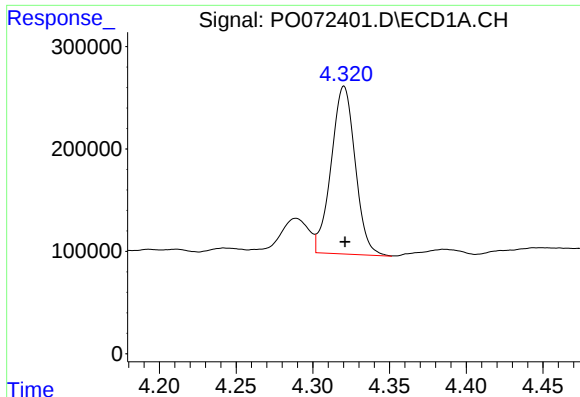


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.001 min
Response: 1783857
Conc: 21.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SHELL-L15-L14-NORTH


Manual Integrations
APPROVED

Ankita
10/16/2020 11:53:48 AM

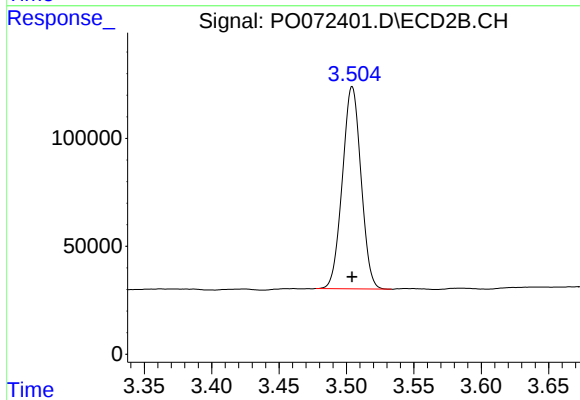


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 904936
Conc: 21.48 ng/ml

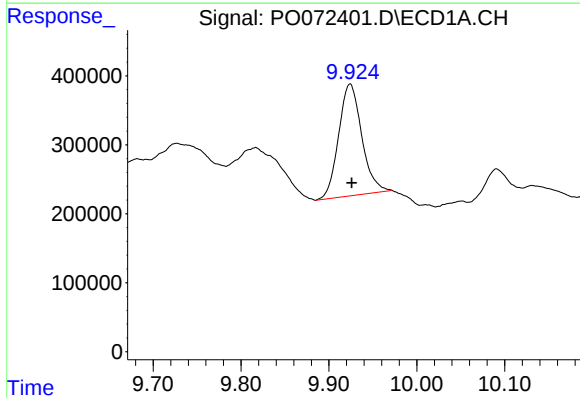

#2 Decachlorobiphenyl

R.T.: 9.924 min
Delta R.T.: -0.002 min
Response: 2975861
Conc: 26.98 ng/ml

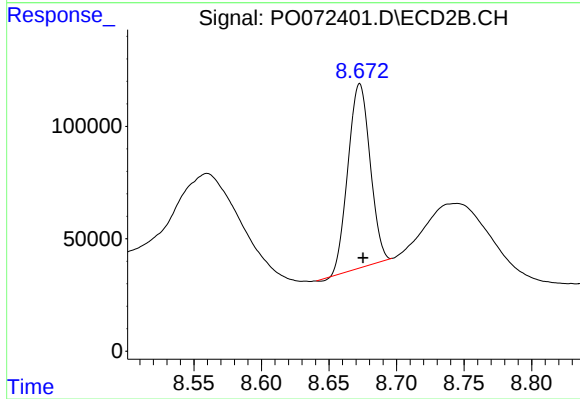

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.002 min
Response: 930960
Conc: 18.01 ng/ml