

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101525\
 Data File : PO114412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2025 14:36
 Operator : YP/AJ
 Sample : Q3342-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONC-ROLLOFF-WC-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/16/2025
 Supervised By :mohammad ahmed 10/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 05:44:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 10 06:46:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.356	3.661	121.4E6	99414291	22.370m	24.840
2) SA Decachlor...	9.941	8.670	84985401	68135108	23.341	20.441

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101525\
Data File : PO114412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2025 14:36
Operator : YP/AJ
Sample : Q3342-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONC-ROLLOFF-WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2025
Supervised By :mohammad ahmed 10/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 05:44:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 10 06:46:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

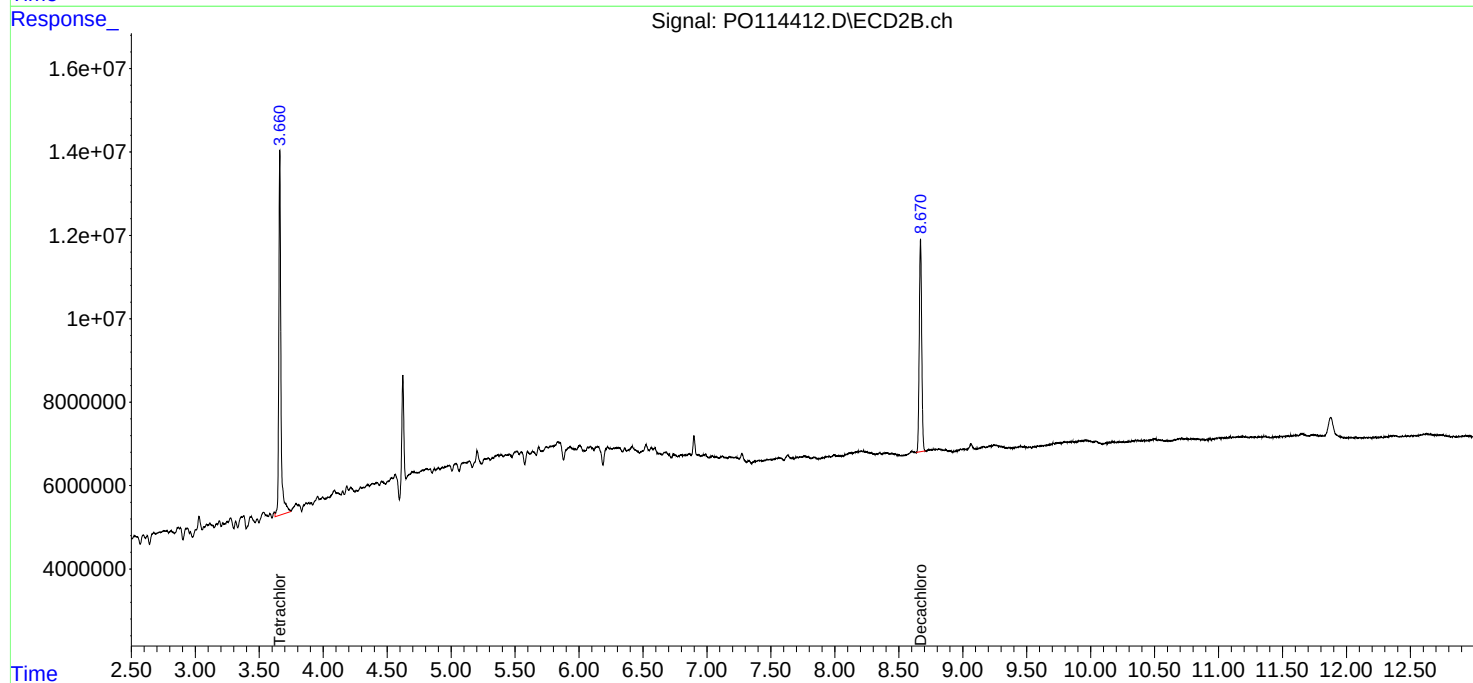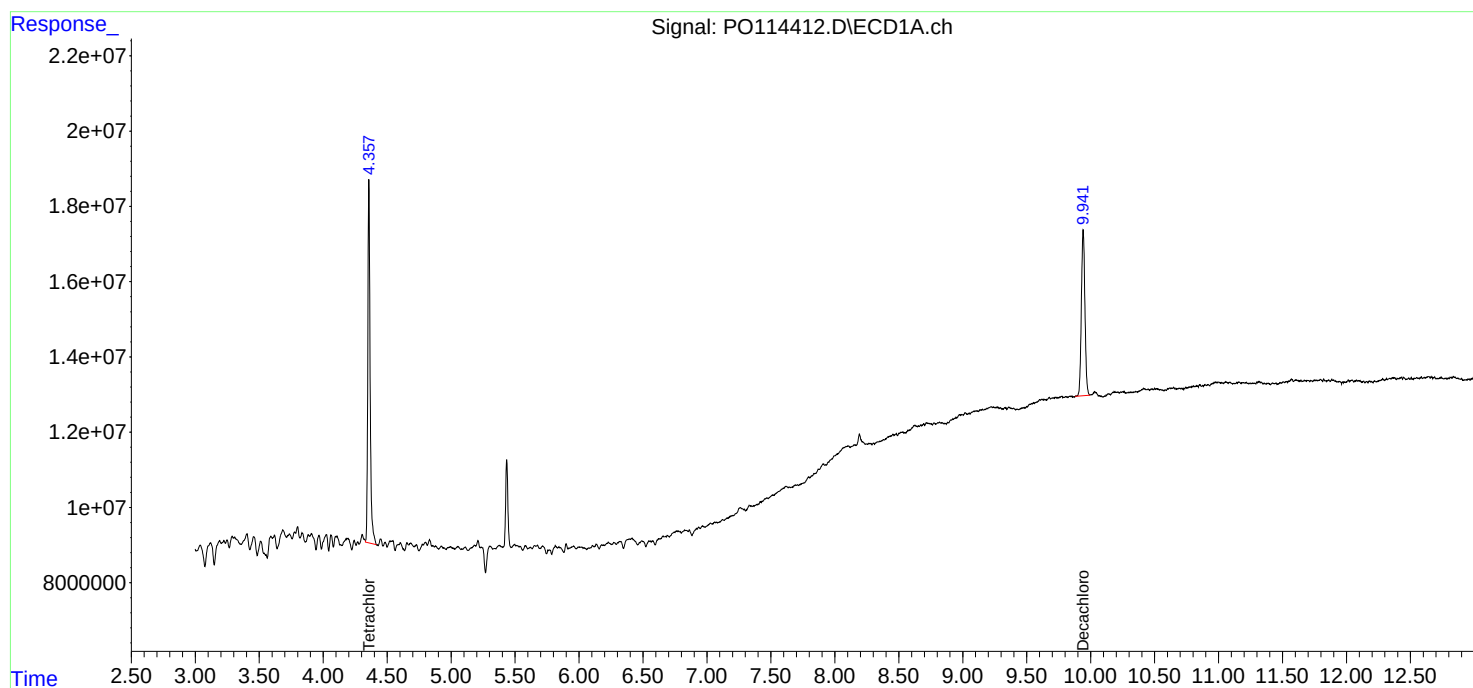

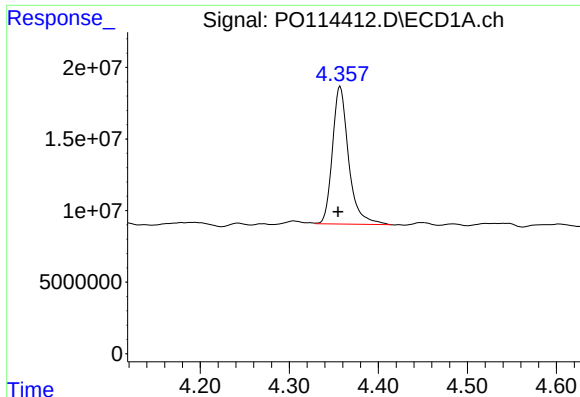


#1 Tetrachloro-m-xylene

R.T.: 4.356 min
Delta R.T.: 0.001 min
Response: 121446842
Conc: 22.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONC-ROLLOFF-WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/16/2025
Supervised By :mohammad ahmed 10/17/2025

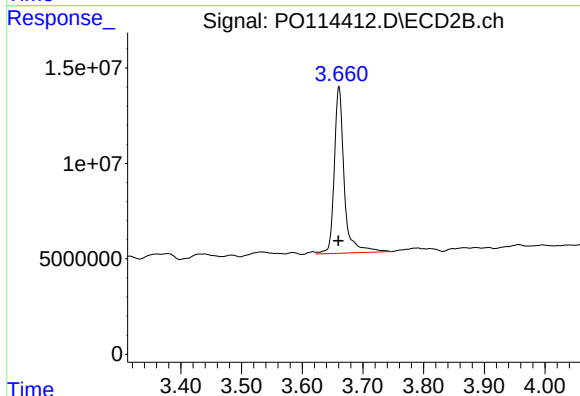


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: 0.000 min
Response: 99414291
Conc: 24.84 ng/ml

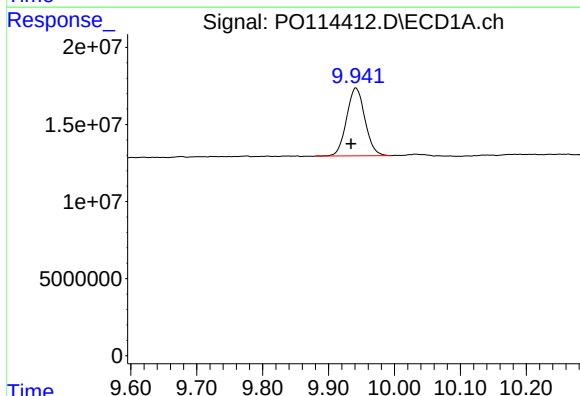

#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: 0.007 min
Response: 84985401
Conc: 23.34 ng/ml

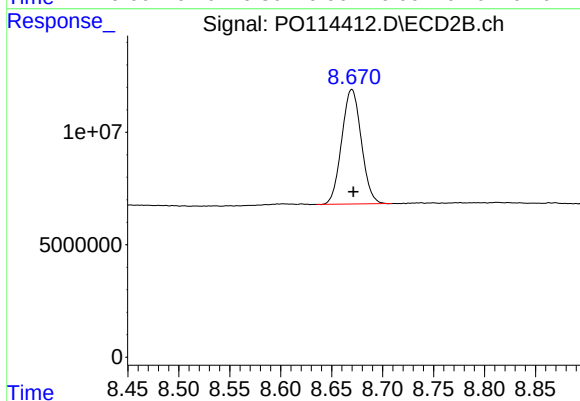

#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 68135108
Conc: 20.44 ng/ml