

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
 Data File : P0050099.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2018 19:41
 Operator : SM/SJ
 Sample : J5511-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 101118-SIDI-F-U-M

Manual Integrations
 APPROVED

sohil
 10/18/2018 5:13:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 06:47:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.362	4017019	3602477	16.306	18.387
2) SA Decachlor...	10.050	8.122	5137089	4200057	27.289m	24.424

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
Data File : PO050099.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2018 19:41
Operator : SM/SJ
Sample : J5511-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
101118-SIDI-F-U-M


Manual Integrations
APPROVED

sohil
10/18/2018 5:13:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 06:47:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

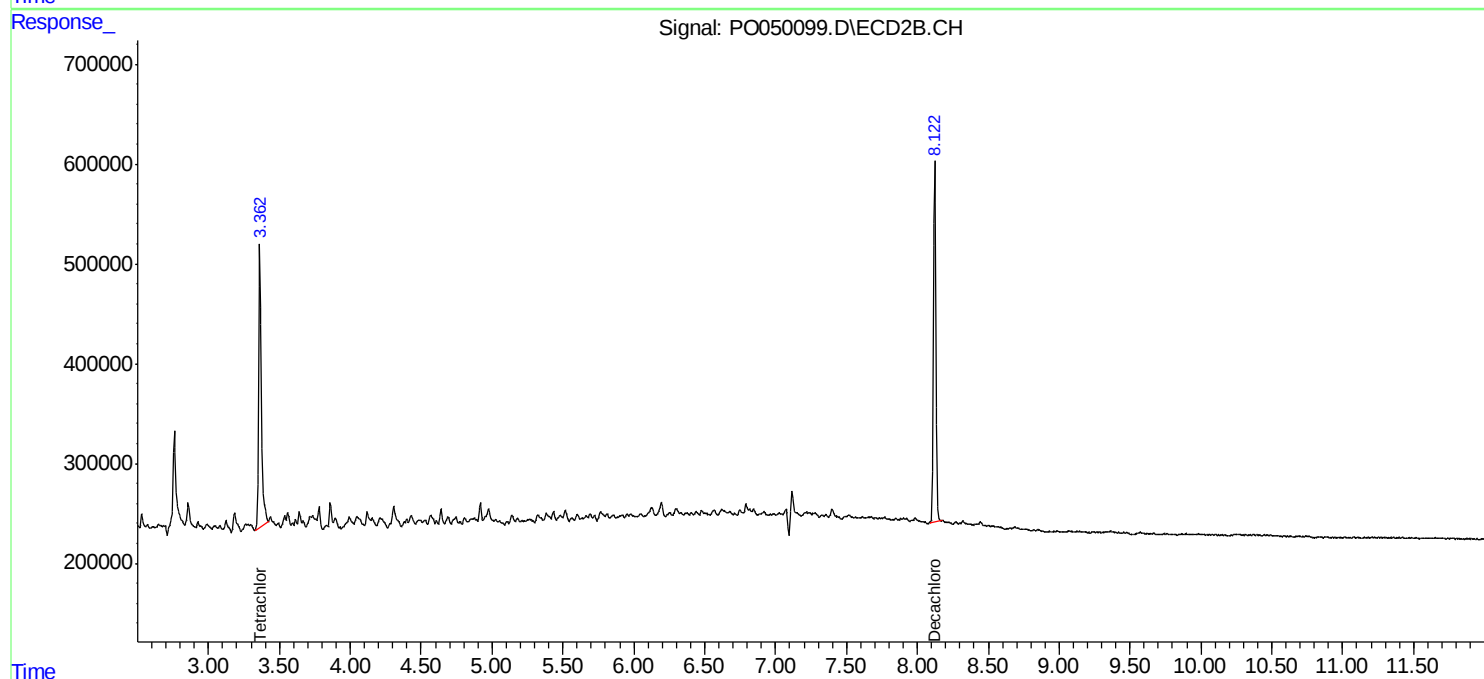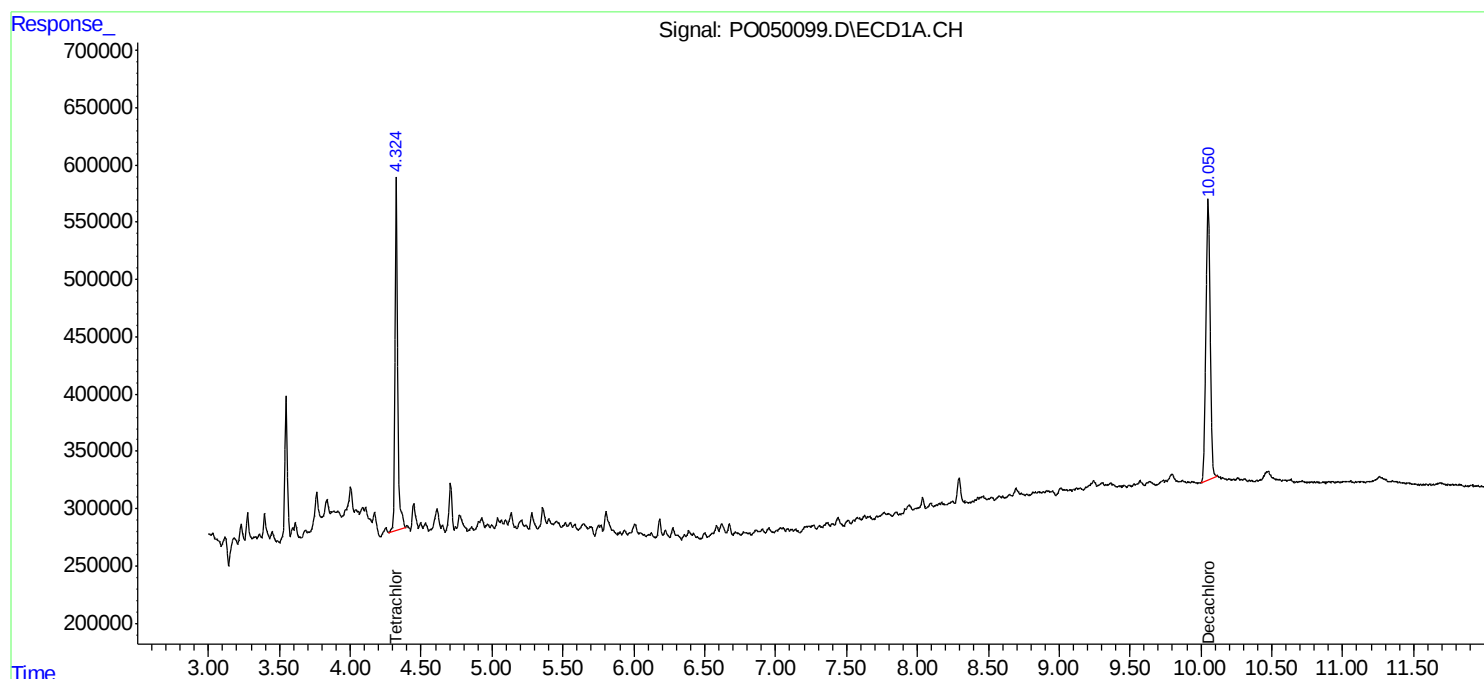

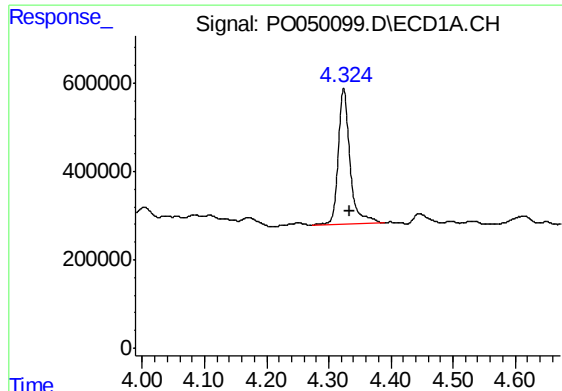


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.010 min
Response: 4017019
Conc: 16.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
101118-SIDI-F-U-M


Manual Integrations
APPROVED

sohil
10/18/2018 5:13:02 PM

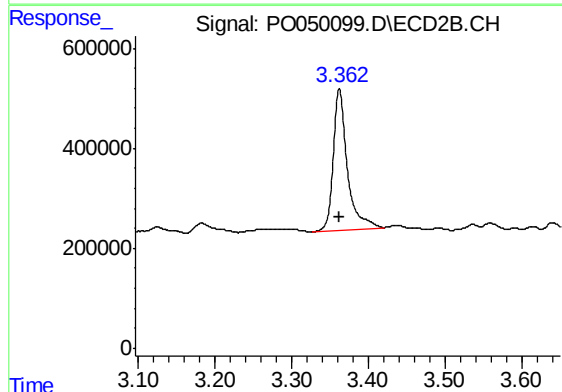


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 3602477
Conc: 18.39 ng/ml

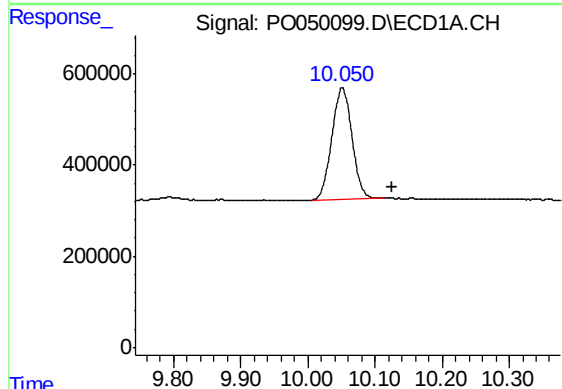

#2 Decachlorobiphenyl

R.T.: 10.050 min
Delta R.T.: -0.074 min
Response: 5137089
Conc: 27.29 ng/ml m

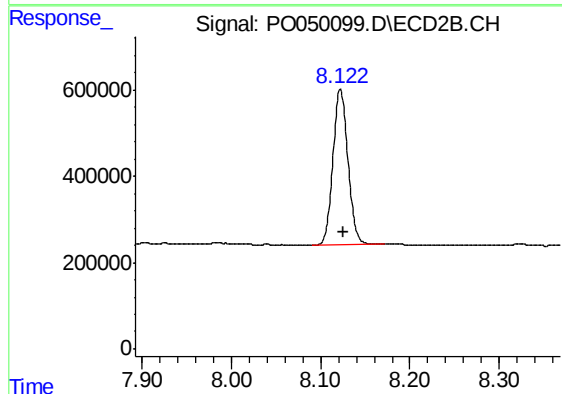

#2 Decachlorobiphenyl

R.T.: 8.122 min
Delta R.T.: -0.003 min
Response: 4200057
Conc: 24.42 ng/ml