

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
 Data File : P0050122.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2018 7:16
 Operator : SM/SJ
 Sample : J5516-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1011-S-DH-30

Manual Integrations
 APPROVED

sohil
 10/18/2018 5:13:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:59:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.361	5229719	4671918	21.229	23.845m
2)	SA Decachlor...	10.066	8.122	5936089	4051201	31.533m	23.559 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
Data File : PO050122.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2018 7:16
Operator : SM/SJ
Sample : J5516-06
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SSSI-1011-S-DH-30


Manual Integrations
APPROVED

sohil
10/18/2018 5:13:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:59:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

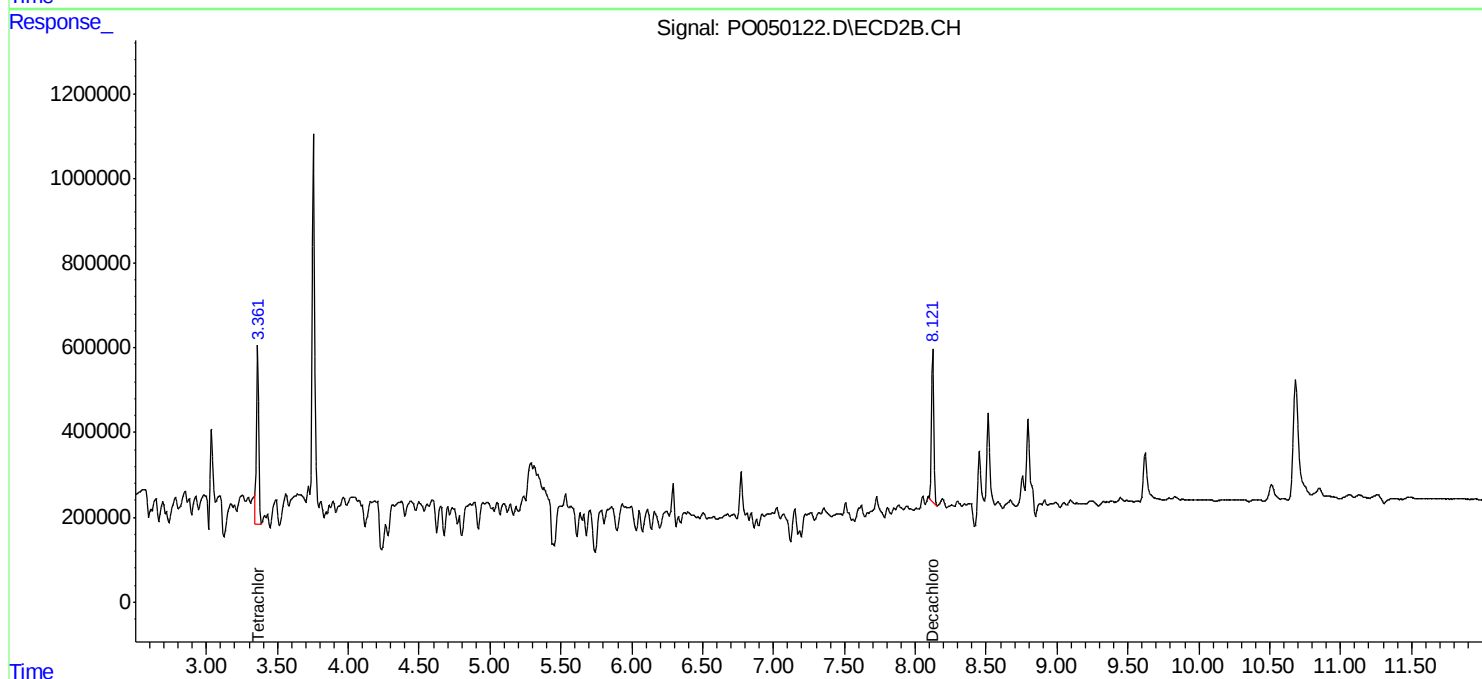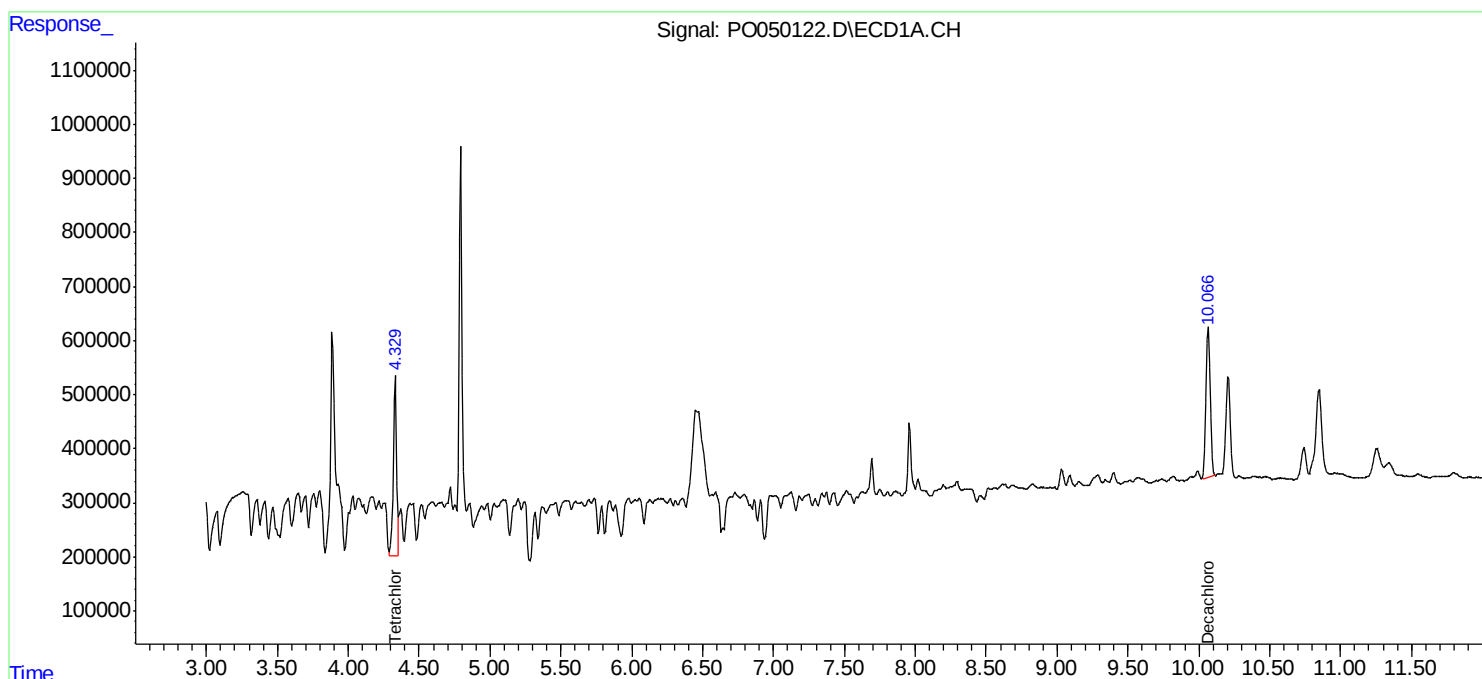

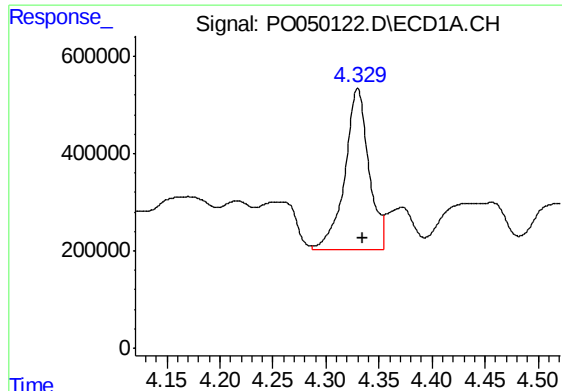


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.004 min
Response: 5229719
Conc: 21.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1011-S-DH-30


Manual Integrations
APPROVED

sohil
10/18/2018 5:13:58 PM

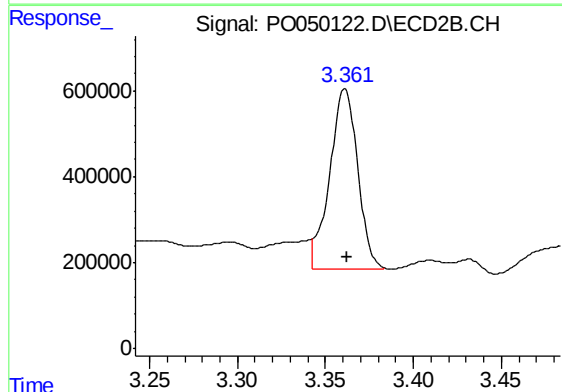


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 4671918
Conc: 23.85 ng/ml m

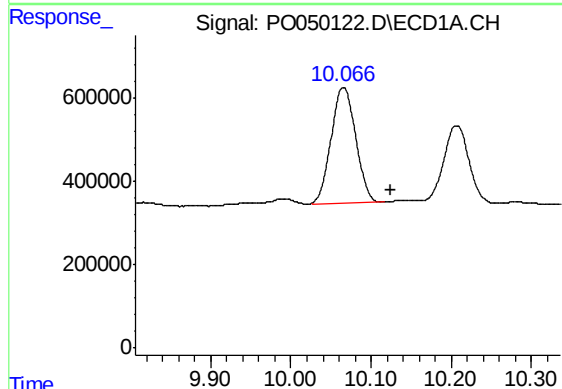

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.059 min
Response: 5936089
Conc: 31.53 ng/ml m

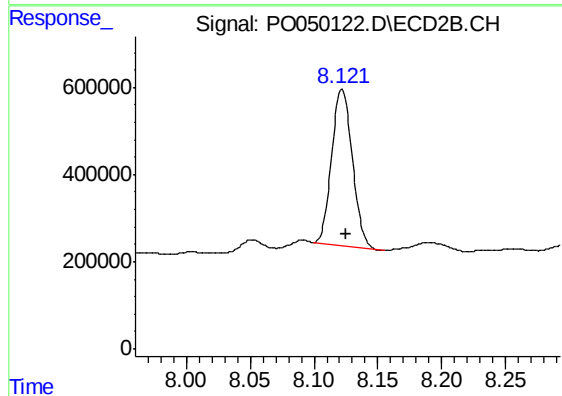

#2 Decachlorobiphenyl

R.T.: 8.122 min
Delta R.T.: -0.003 min
Response: 4051201
Conc: 23.56 ng/ml