

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
 Data File : P0050123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2018 7:34
 Operator : SM/SJ
 Sample : J5516-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1012-S-DH-29

Manual Integrations
 APPROVED

Sohil
 10/25/2018 9:28:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:59:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.330	3.361	4079321	4073110	16.559	20.789 #
2) SA Decachlor...	10.066	8.122	5583620	4147813	29.661m	24.120

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
Data File : PO050123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2018 7:34
Operator : SM/SJ
Sample : J5516-08
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SSSI-1012-S-DH-29


Manual Integrations
APPROVED

Sohil
10/25/2018 9:28:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:59:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

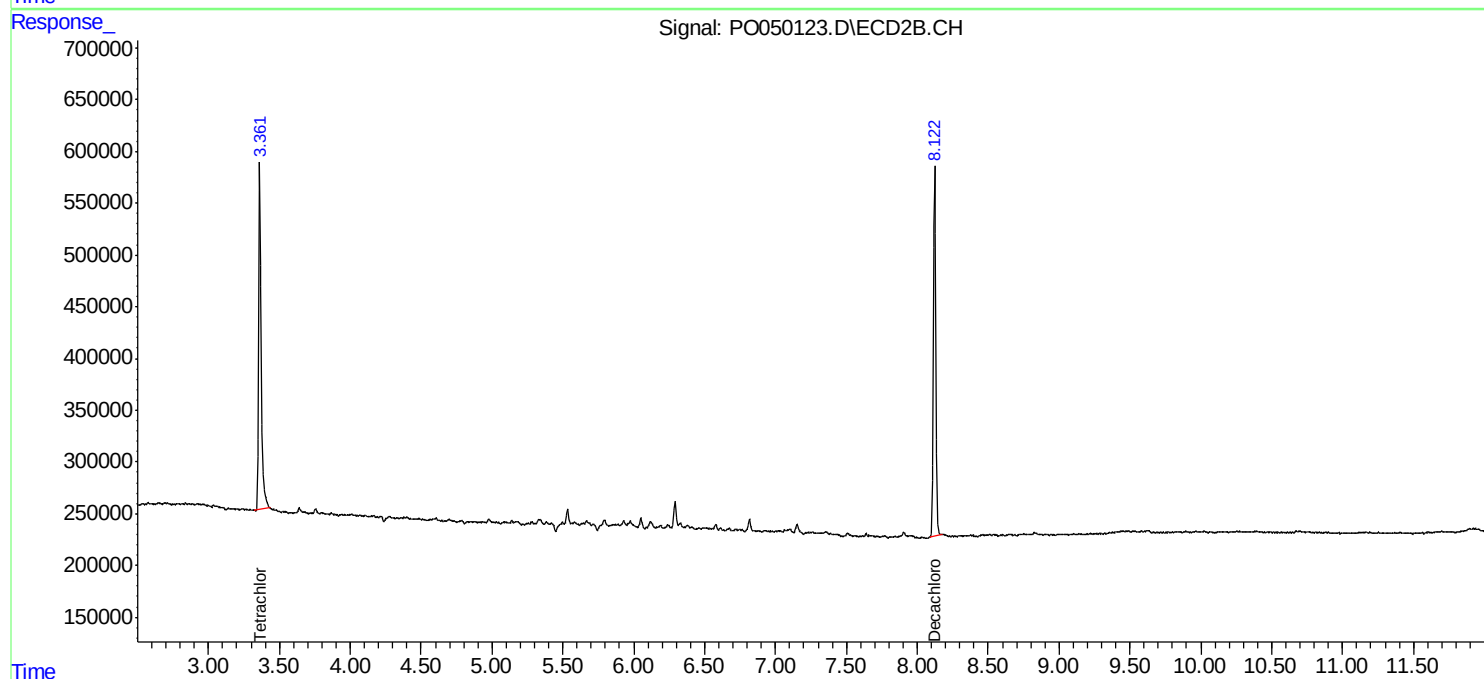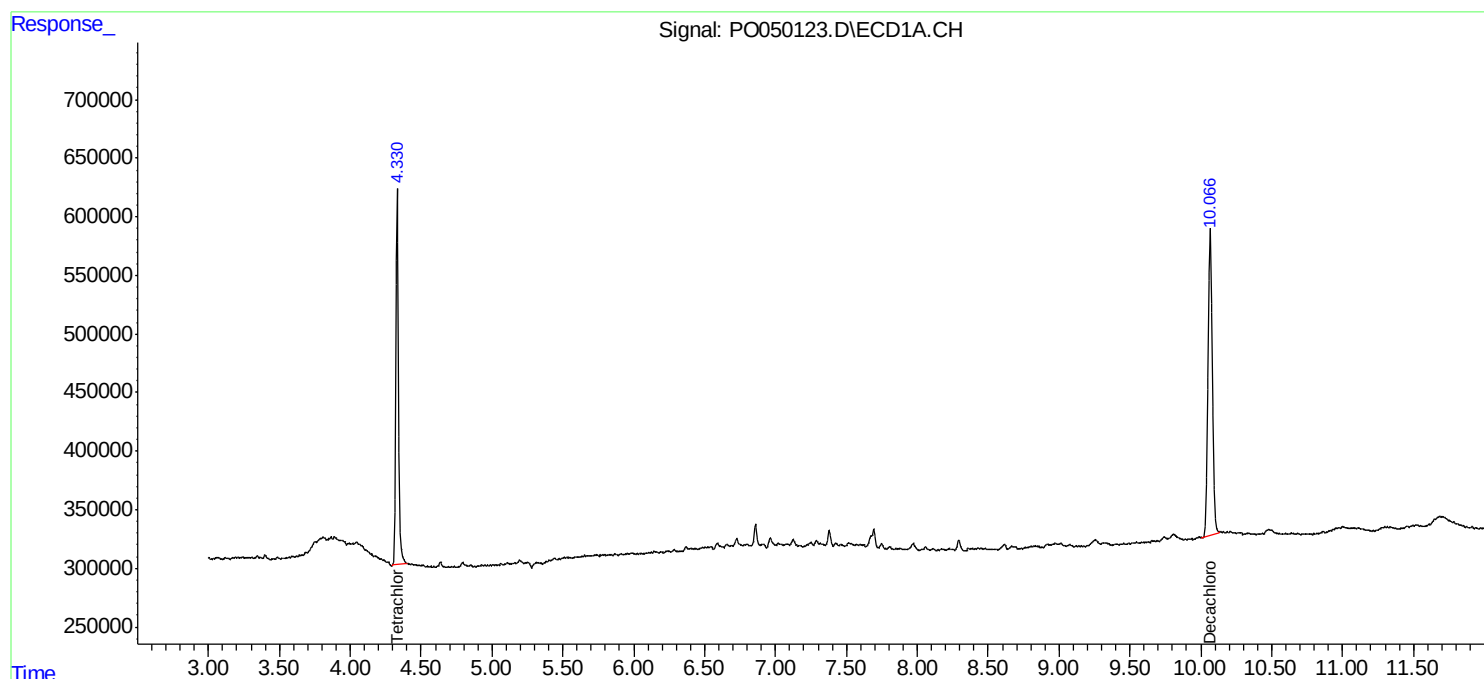

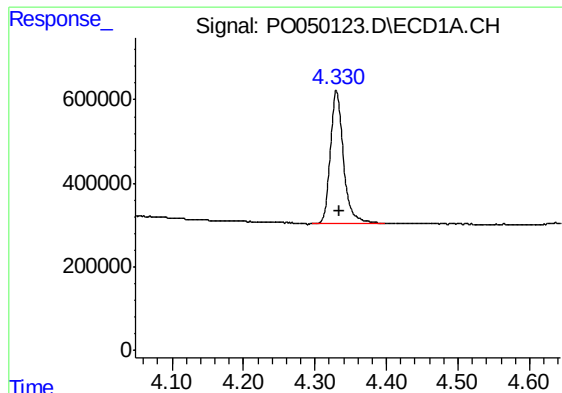


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.004 min
Response: 4079321
Conc: 16.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1012-S-DH-29


Manual Integrations
APPROVED

Sohil
10/25/2018 9:28:14 AM

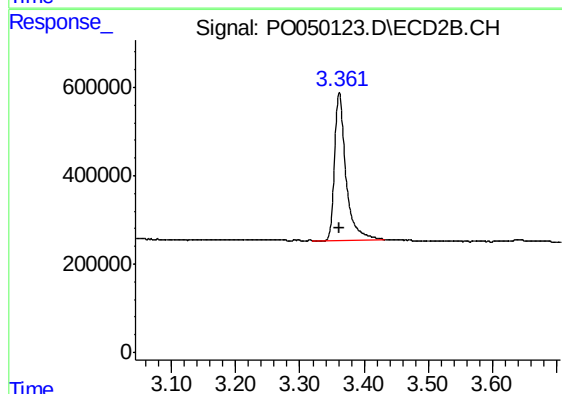


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 4073110
Conc: 20.79 ng/ml

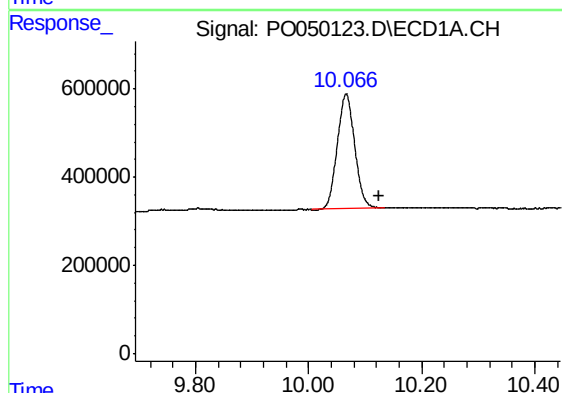

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.058 min
Response: 5583620
Conc: 29.66 ng/ml m

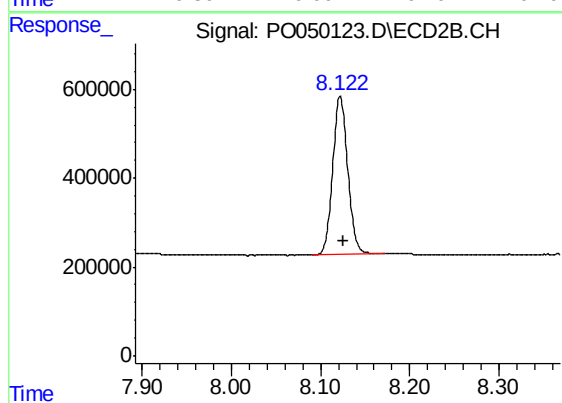

#2 Decachlorobiphenyl

R.T.: 8.122 min
Delta R.T.: -0.003 min
Response: 4147813
Conc: 24.12 ng/ml