

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101618\
 Data File : P0050130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2018 13:03
 Operator : SM/SJ
 Sample : J5383-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 100918-TIPC-F-D-S

Manual Integrations
 APPROVED

sohil
 10/18/2018 5:14:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 13:22:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 15 16:37:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.333	3.361	3011054	2460444	12.223	12.558m
2) SA Decachlor...	10.069	8.122	4048902	2740595	21.508m	15.937 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101618\
Data File : PO050130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2018 13:03
Operator : SM/SJ
Sample : J5383-08
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
100918-TIPC-F-D-S


Manual Integrations
APPROVED

sohil
10/18/2018 5:14:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 13:22:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 15 16:37:53 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

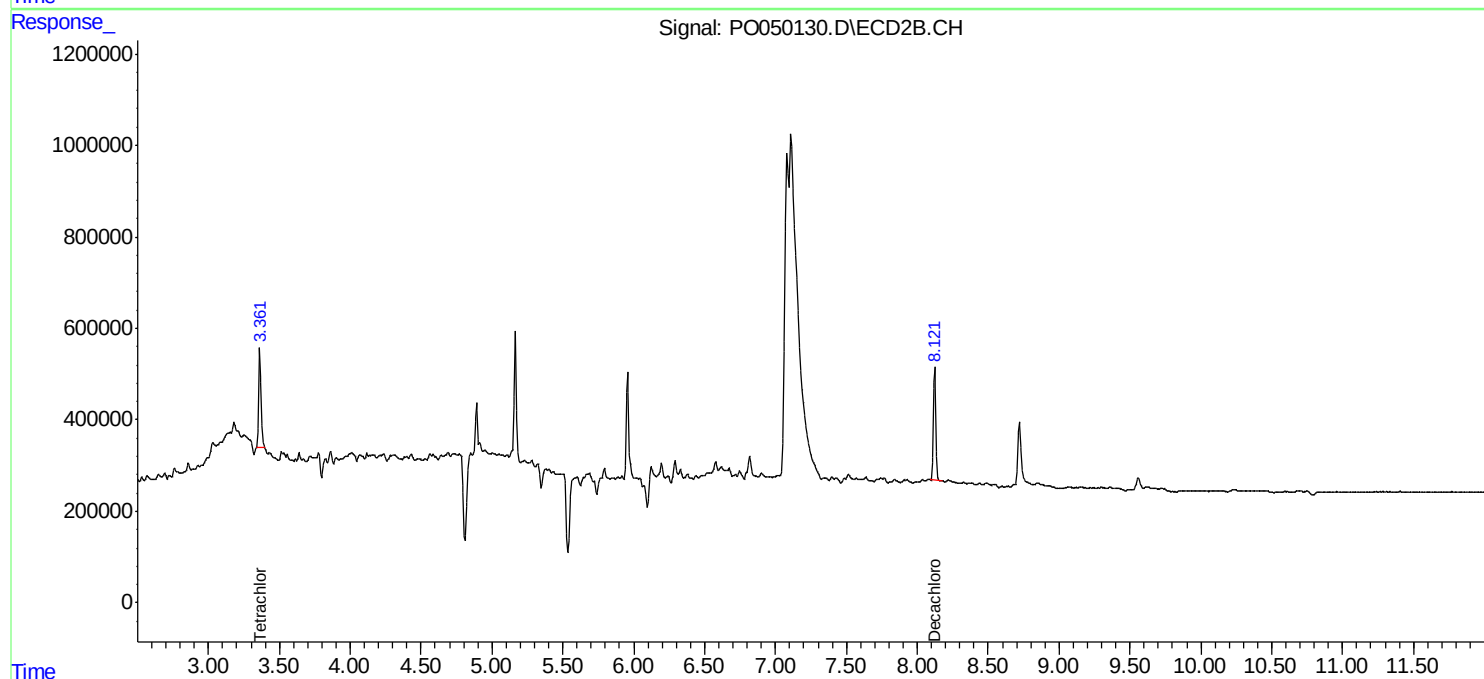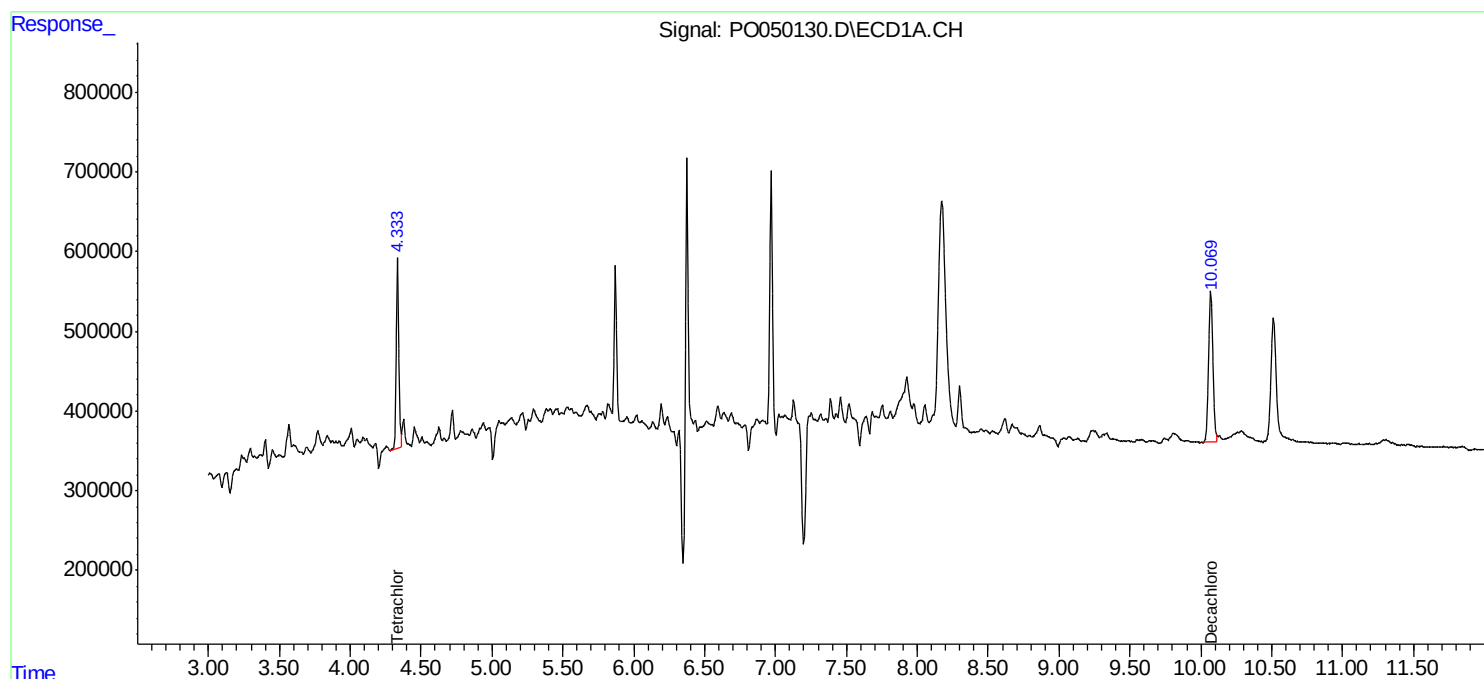

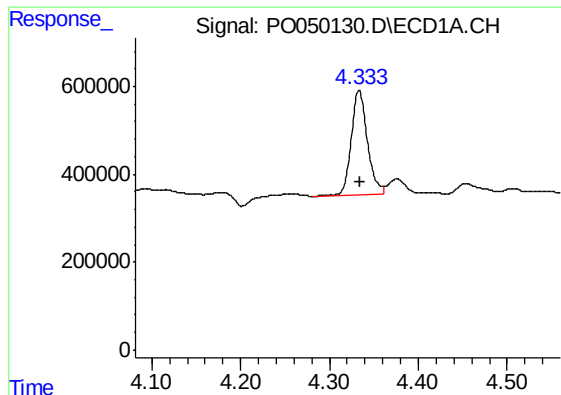


#1 Tetrachloro-m-xylene

R.T.: 4.333 min
Delta R.T.: 0.000 min
Response: 3011054
Conc: 12.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
100918-TIPC-F-D-S


Manual Integrations
APPROVED

sohil
10/18/2018 5:14:11 PM

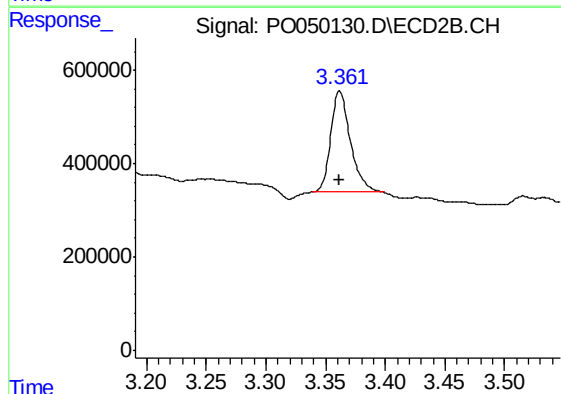


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 2460444
Conc: 12.56 ng/ml m

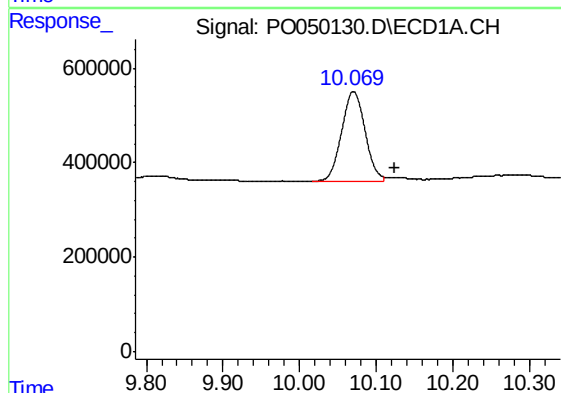

#2 Decachlorobiphenyl

R.T.: 10.069 min
Delta R.T.: -0.055 min
Response: 4048902
Conc: 21.51 ng/ml m

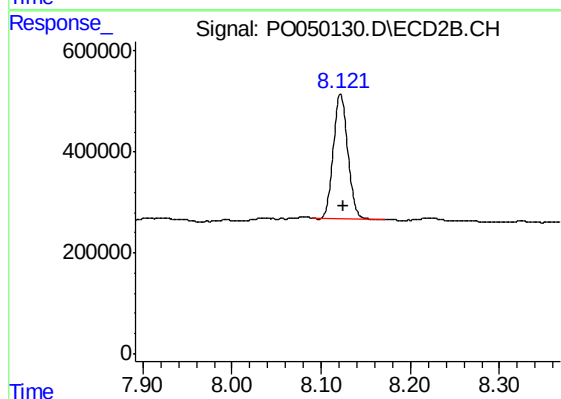

#2 Decachlorobiphenyl

R.T.: 8.122 min
Delta R.T.: -0.004 min
Response: 2740595
Conc: 15.94 ng/ml