

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101619\
 Data File : P0062037.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2019 10:42
 Operator : HP/AJ
 Sample : K5111-07
 Misc : AR1221-LOD-25PPB-WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/17/2019 3:50:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 07:01:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.326	3.484	1389669	957033	22.469	22.318
2)	SA Decachlor...	9.954	8.337	1242302	630289	22.203	21.481
Target Compounds							
8)	L2 AR-1221-1	4.533	3.690	19038	17050	27.358m	33.533m
9)	L2 AR-1221-2	4.624	3.771	30250	23097	58.006m	60.111m
10)	L2 AR-1221-3	4.697	3.844	58516	41705	35.843	35.439m
11)	L3 AR-1232-1	4.697	3.845	58516	43449	26.792	28.040

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101619\
Data File : PO062037.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2019 10:42
Operator : HP/AJ
Sample : K5111-07
Misc : AR1221-LOD-25PPB-WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 3:50:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 07:01:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

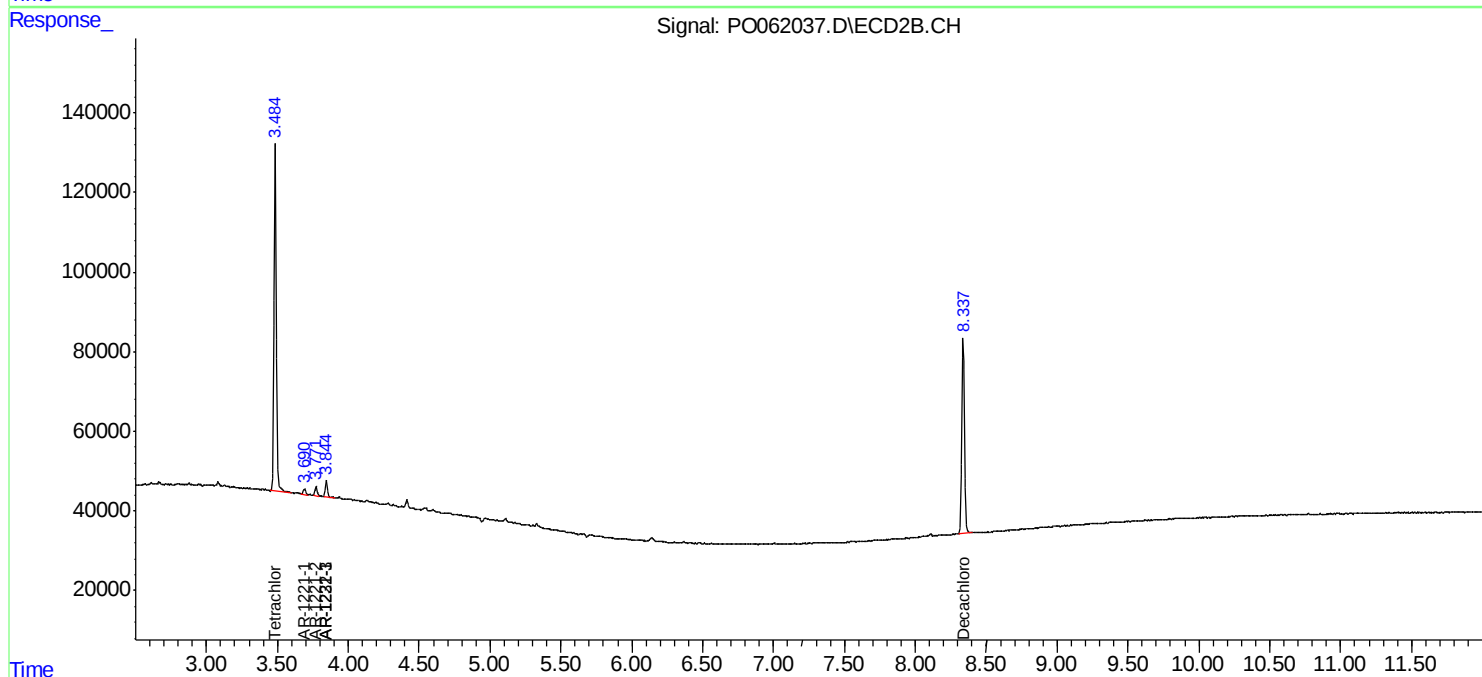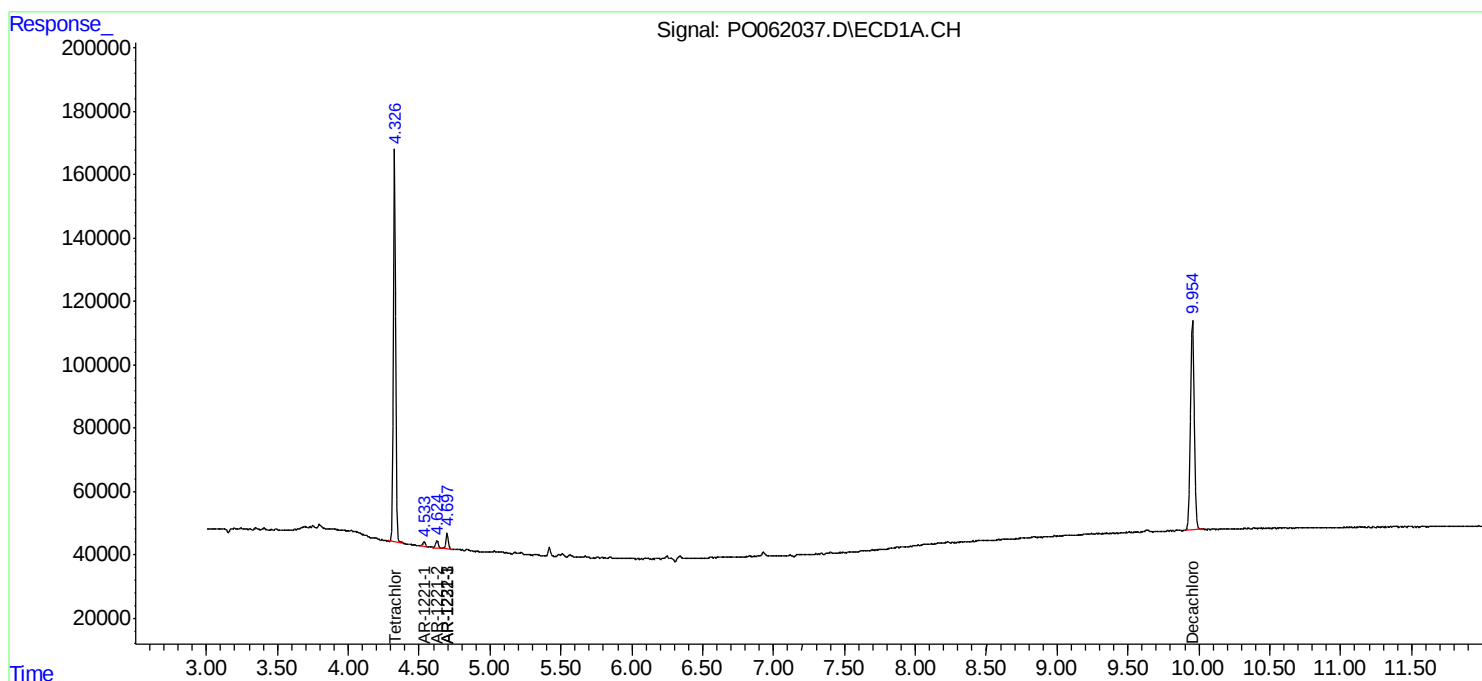

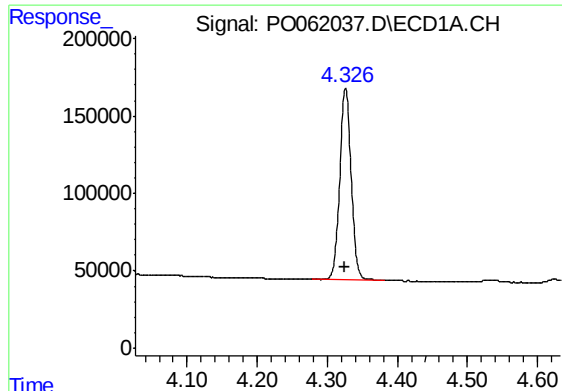


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: 0.001 min
Response: 1389669
Conc: 22.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 3:50:21 PM

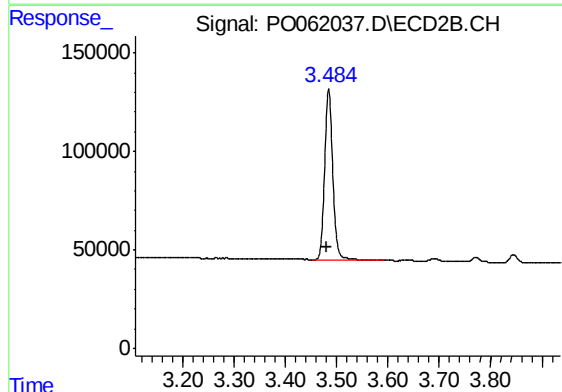


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.003 min
Response: 957033
Conc: 22.32 ng/ml

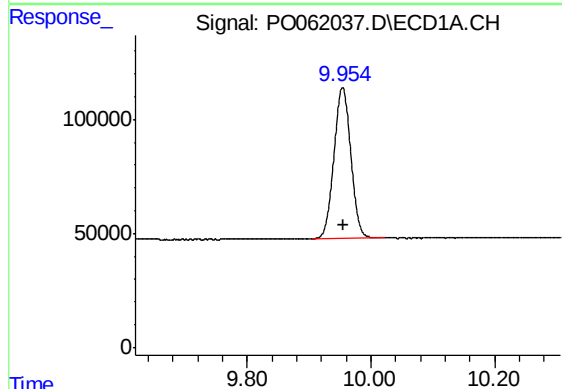


#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.002 min
Response: 1242302
Conc: 22.20 ng/ml

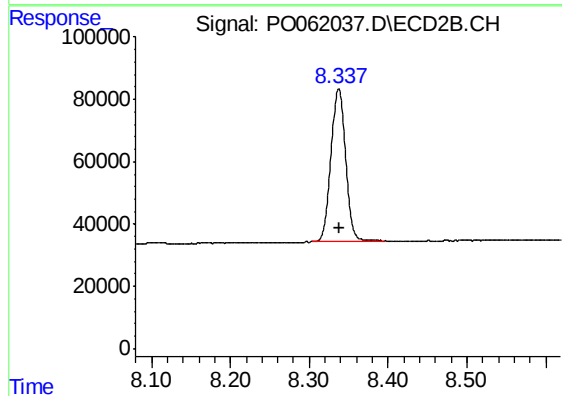

#2 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: 0.000 min
Response: 630289
Conc: 21.48 ng/ml

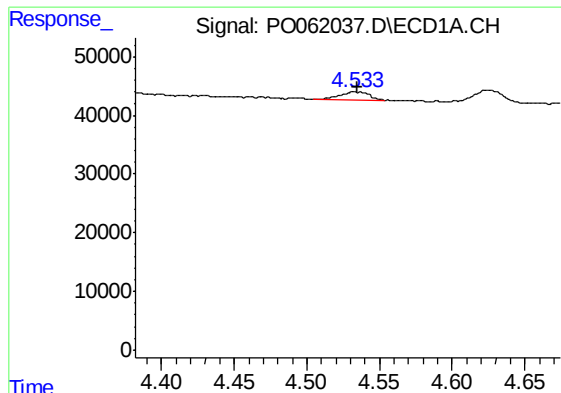


#8 AR-1221-1

R.T.: 4.533 min
Delta R.T.: -0.002 min
Response: 19038
Conc: 27.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 3:50:21 PM

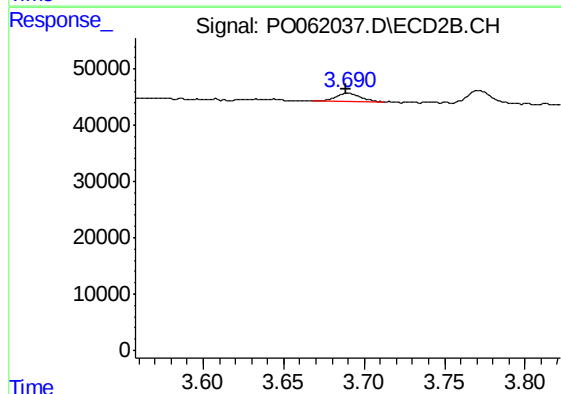


#8 AR-1221-1

R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 17050
Conc: 33.53 ng/ml m

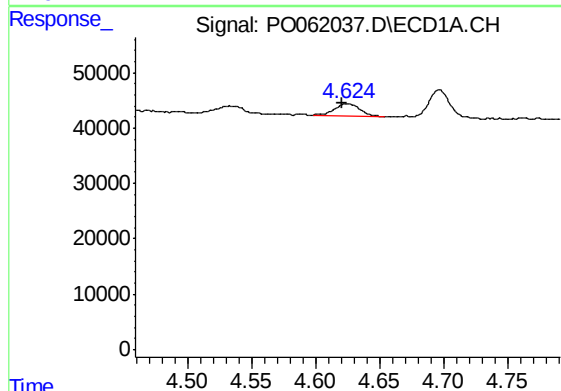


#9 AR-1221-2

R.T.: 4.624 min
Delta R.T.: 0.003 min
Response: 30250
Conc: 58.01 ng/ml m

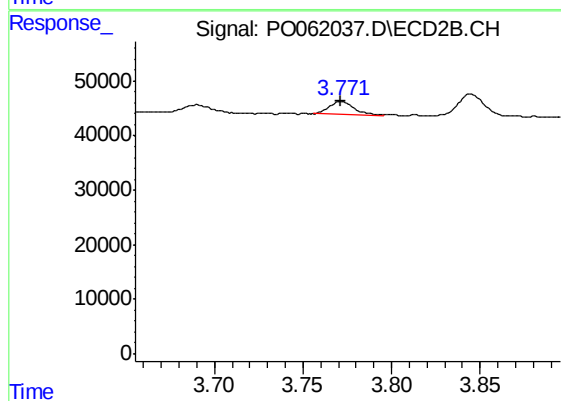

#9 AR-1221-2

R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 23097
Conc: 60.11 ng/ml m

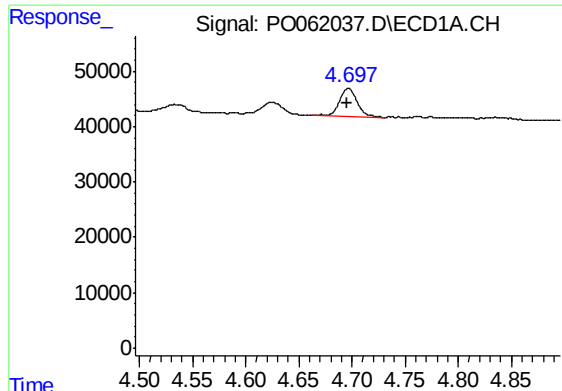


#10 AR-1221-3

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 58516
Conc: 35.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 3:50:21 PM

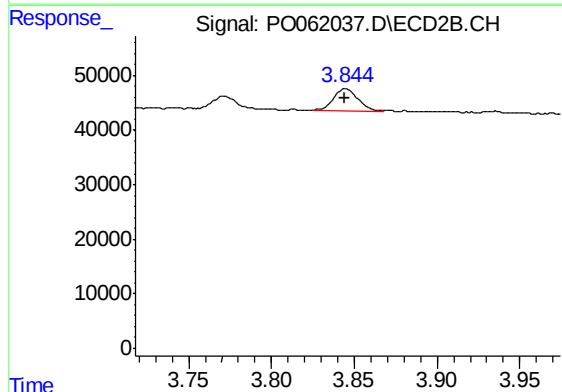


#10 AR-1221-3

R.T.: 3.844 min
Delta R.T.: 0.000 min
Response: 41705
Conc: 35.44 ng/ml m

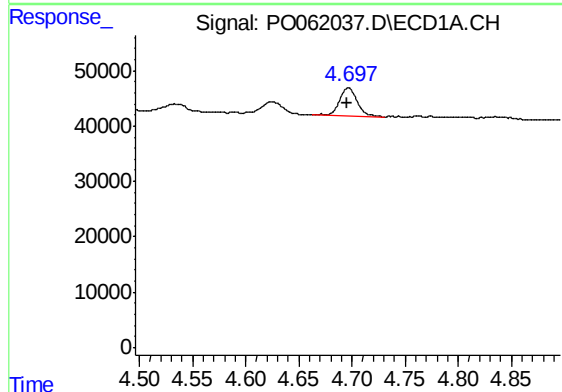

#11 AR-1232-1

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 58516
Conc: 26.79 ng/ml

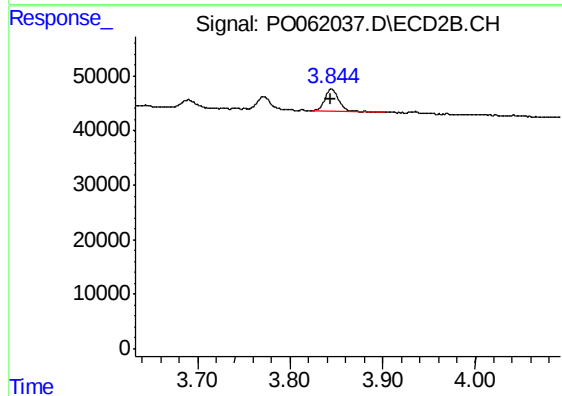

#11 AR-1232-1

R.T.: 3.845 min
Delta R.T.: 0.000 min
Response: 43449
Conc: 28.04 ng/ml