

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101619\
 Data File : P0062041.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2019 11:53
 Operator : HP/AJ
 Sample : K5111-07
 Misc : AR1254-LOD-25PPB-WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2019

Manual Integrations
 APPROVED

Ankita
 10/17/2019 9:14:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 12:08:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.323	3.482	988564	706344	15.984	16.472
2)	SA Decachlor...	9.953	8.336	1001085	518968	17.892	17.687
Target Compounds							
26)	L6 AR-1254-1	6.331	5.303	80150	71401	30.068m	29.193
27)	L6 AR-1254-2	6.550	5.448	111878	61223	27.364	28.908
28)	L6 AR-1254-3	6.915	5.840	114606	89665	27.391	27.520
29)	L6 AR-1254-4	7.199	6.064	79065	47571	26.239	24.630
30)	L6 AR-1254-5	7.616	6.473	77365	71912	24.686m	27.227

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101619\
Data File : PO062041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2019 11:53
Operator : HP/AJ
Sample : K5111-07
Misc : AR1254-LOD-25PPB-WATER
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 9:14:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 12:08:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

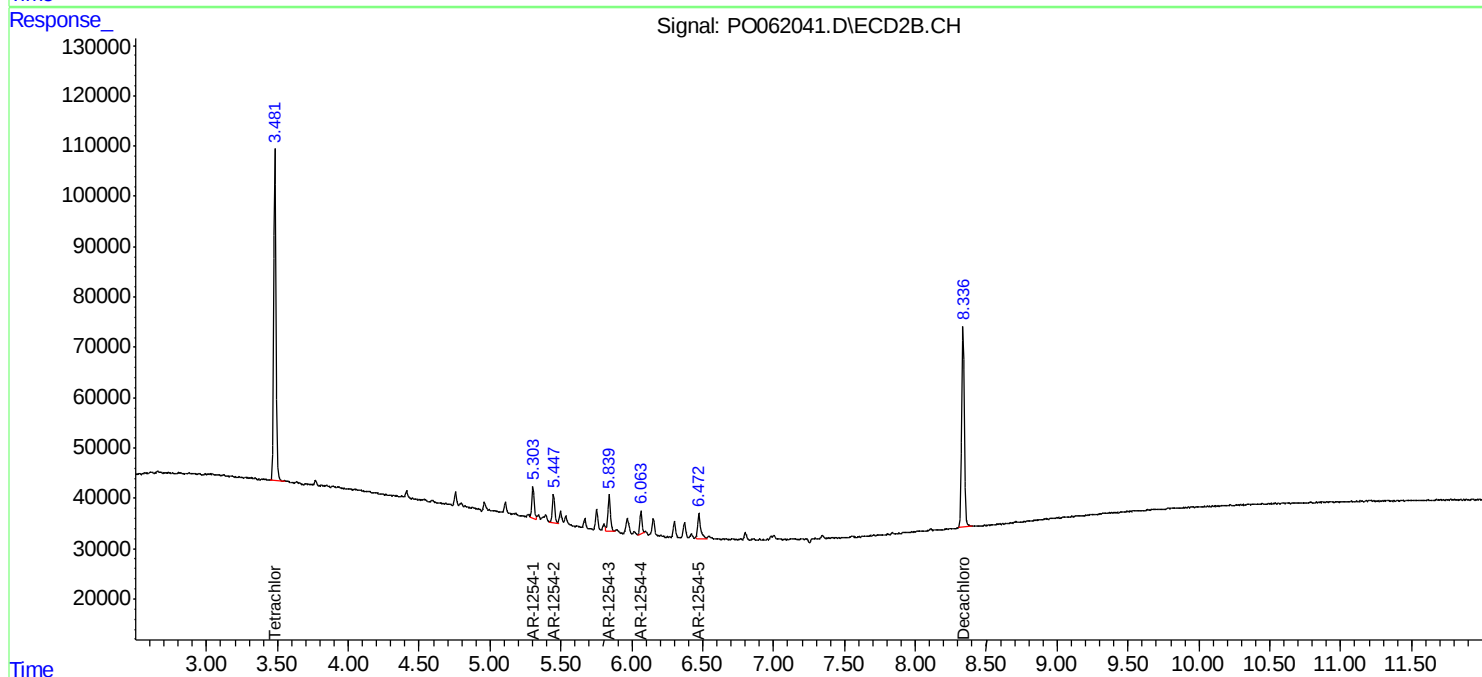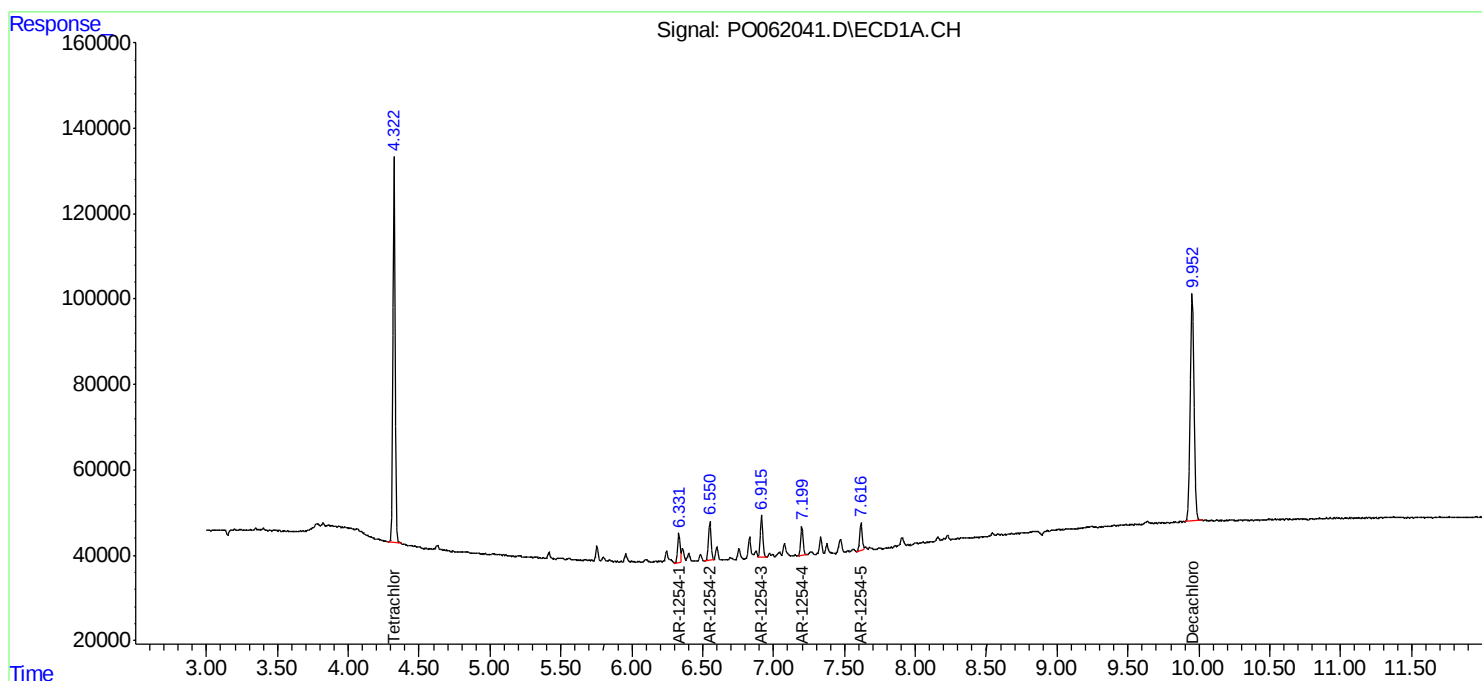

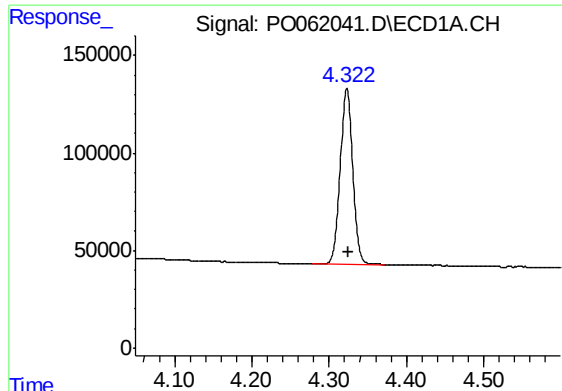


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.002 min
Response: 988564
Conc: 15.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 9:14:35 AM

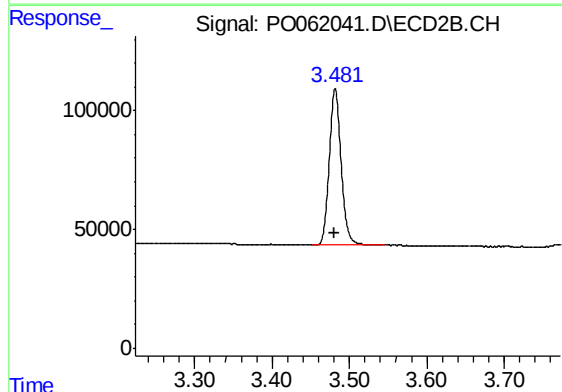


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.000 min
Response: 706344
Conc: 16.47 ng/ml

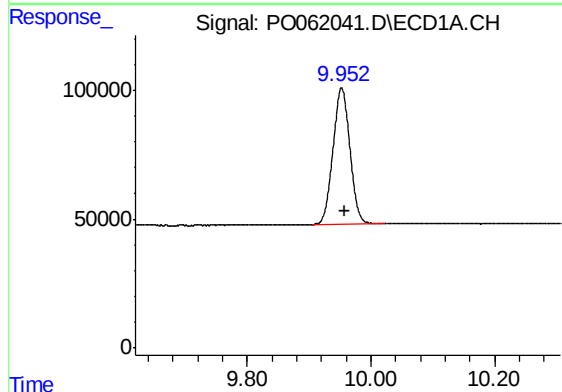


#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.004 min
Response: 1001085
Conc: 17.89 ng/ml

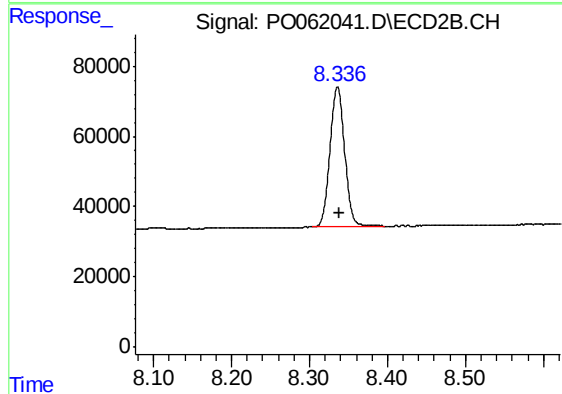

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: -0.002 min
Response: 518968
Conc: 17.69 ng/ml

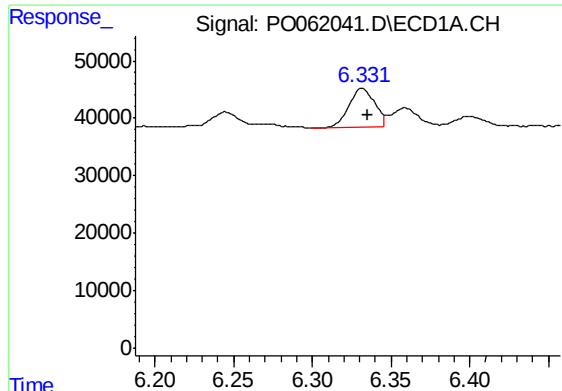


#26 AR-1254-1

R.T.: 6.331 min
Delta R.T.: -0.005 min
Response: 80150
Conc: 30.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 9:14:35 AM

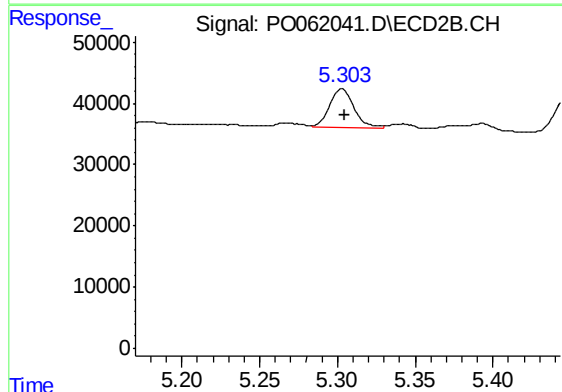


#26 AR-1254-1

R.T.: 5.303 min
Delta R.T.: -0.002 min
Response: 71401
Conc: 29.19 ng/ml

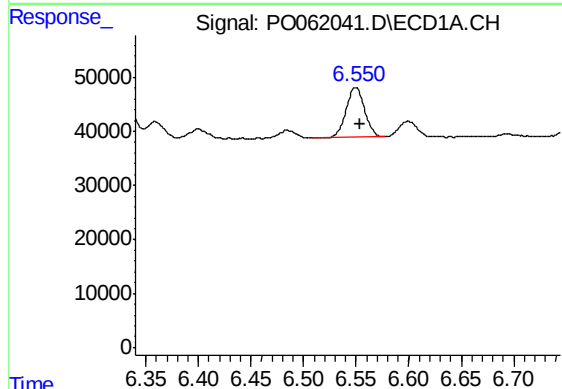


#27 AR-1254-2

R.T.: 6.550 min
Delta R.T.: -0.004 min
Response: 111878
Conc: 27.36 ng/ml

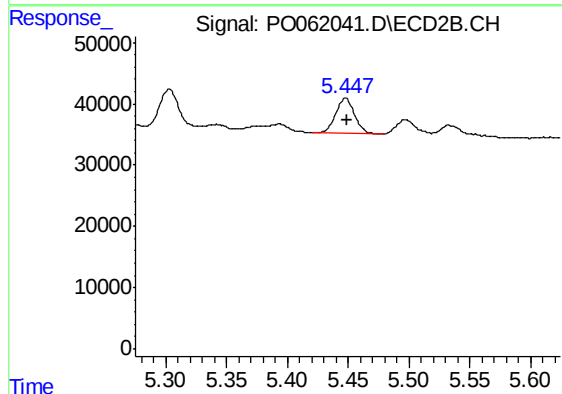

#27 AR-1254-2

R.T.: 5.448 min
Delta R.T.: -0.001 min
Response: 61223
Conc: 28.91 ng/ml

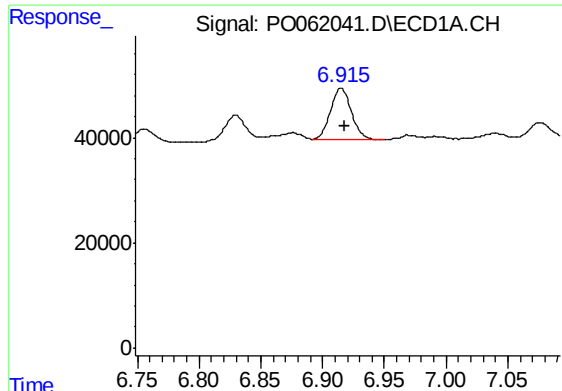


#28 AR-1254-3

R.T.: 6.915 min
Delta R.T.: -0.003 min
Response: 114606
Conc: 27.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019


Manual Integrations
APPROVED

Ankita
10/17/2019 9:14:35 AM

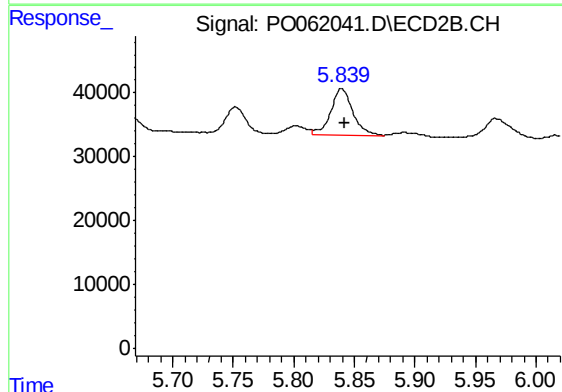


#28 AR-1254-3

R.T.: 5.840 min
Delta R.T.: -0.002 min
Response: 89665
Conc: 27.52 ng/ml

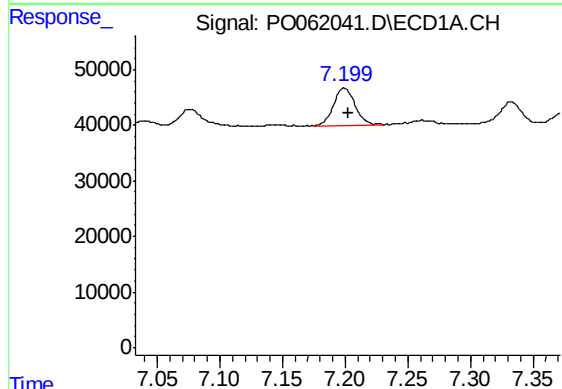


#29 AR-1254-4

R.T.: 7.199 min
Delta R.T.: -0.004 min
Response: 79065
Conc: 26.24 ng/ml

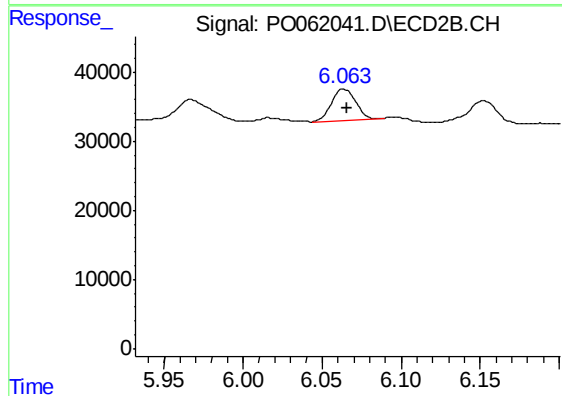

#29 AR-1254-4

R.T.: 6.064 min
Delta R.T.: -0.002 min
Response: 47571
Conc: 24.63 ng/ml

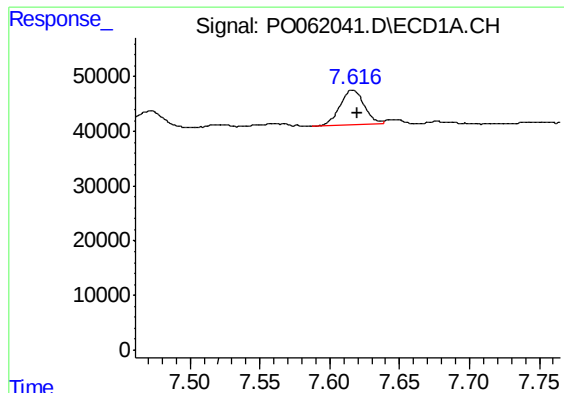


#30 AR-1254-5

R.T.: 7.616 min
Delta R.T.: -0.004 min
Response: 77365
Conc: 24.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2019

Manual Integrations
APPROVED

Ankita
10/17/2019 9:14:35 AM

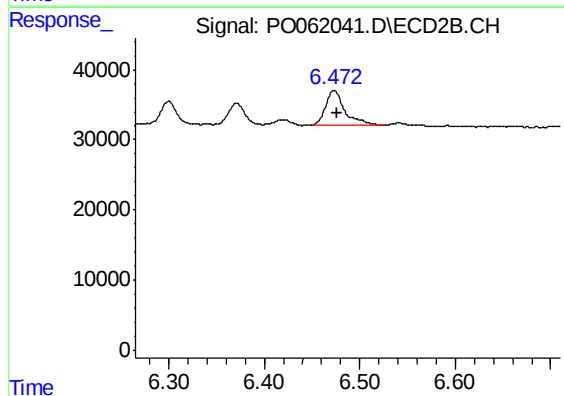

#30 AR-1254-5

R.T.: 6.473 min
Delta R.T.: -0.003 min
Response: 71912
Conc: 27.23 ng/ml