

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101619\
 Data File : P0062074.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2019 21:31
 Operator : HP/AJ
 Sample : K5358-02RE
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20190897-AMENDED-COMP-KM-CA

Manual Integrations
 APPROVED

Ankita
 10/17/2019 9:16:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 01:08:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 12 06:25:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.483	1044820	672442	16.894	15.681m
2)	SA Decachlor...	9.961	8.340	498689	276085	8.913	9.409m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101619\
Data File : PO062074.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2019 21:31
Operator : HP/AJ
Sample : K5358-02RE
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20190897-AMENDED-COMP-KM-CA


Manual Integrations
APPROVED

Ankita
10/17/2019 9:16:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 01:08:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101119.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 12 06:25:38 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

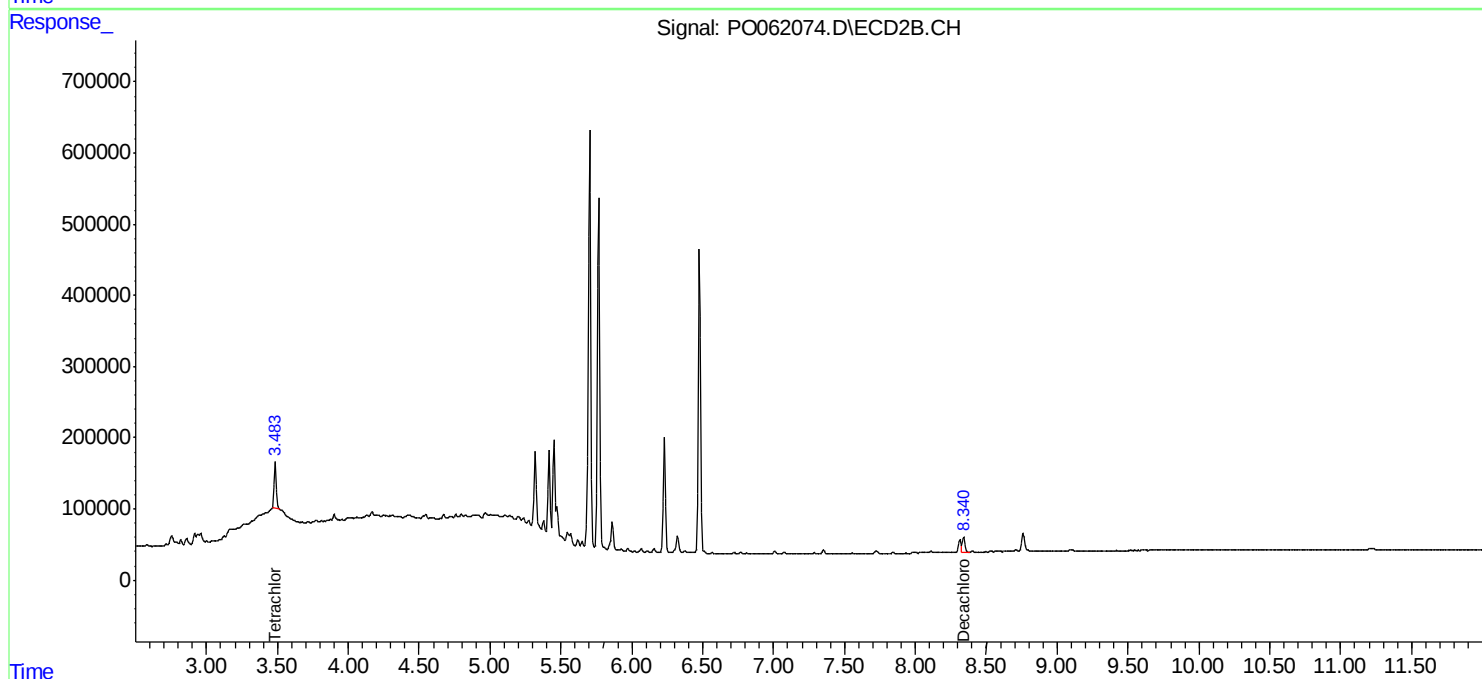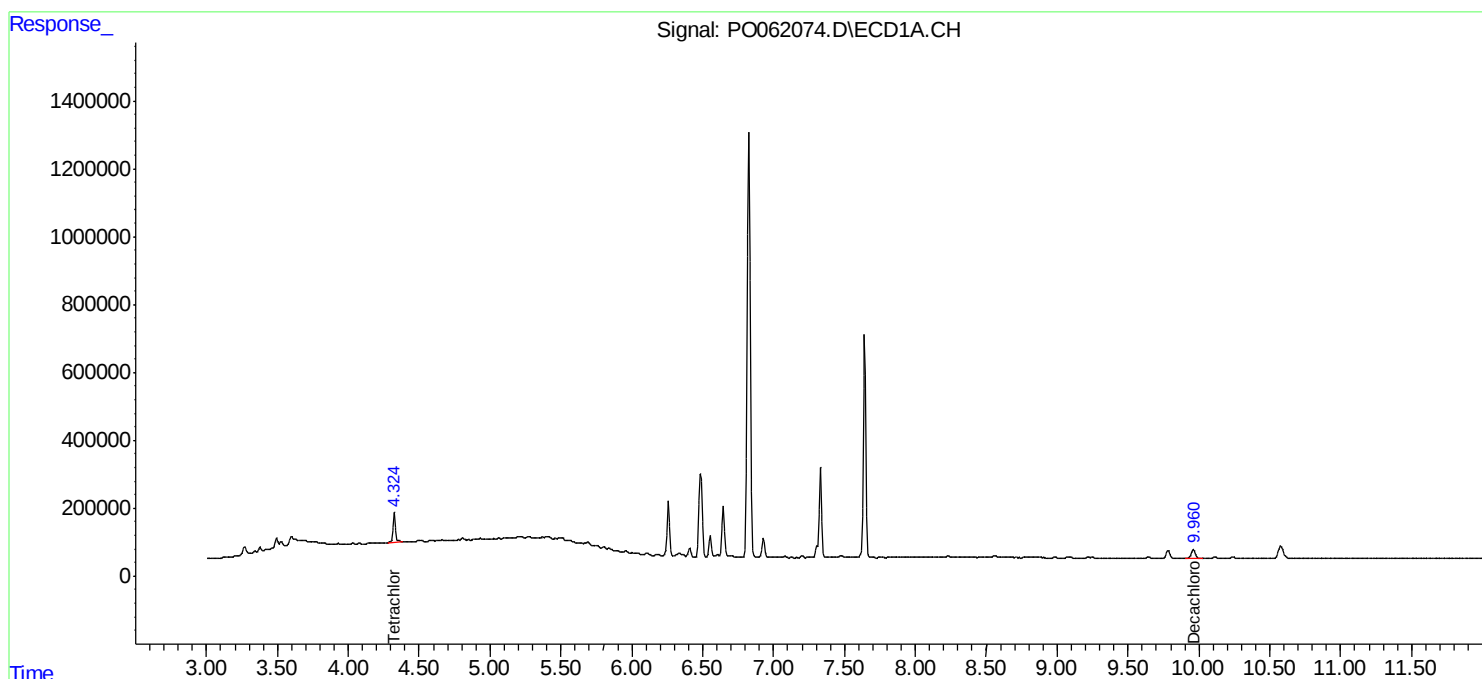

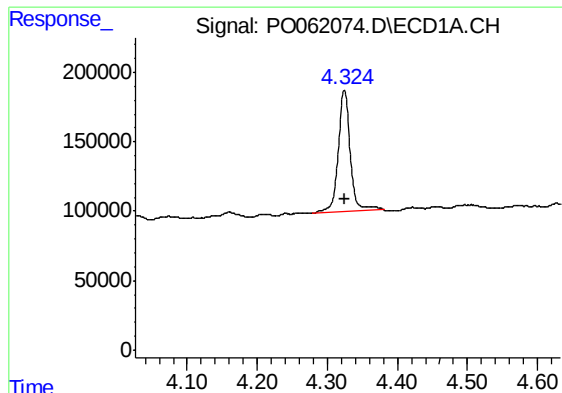


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: 0.000 min
Response: 1044820
Conc: 16.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190897-AMENDED-COMP-KM-CA


Manual Integrations
APPROVED

Ankita
10/17/2019 9:16:06 AM

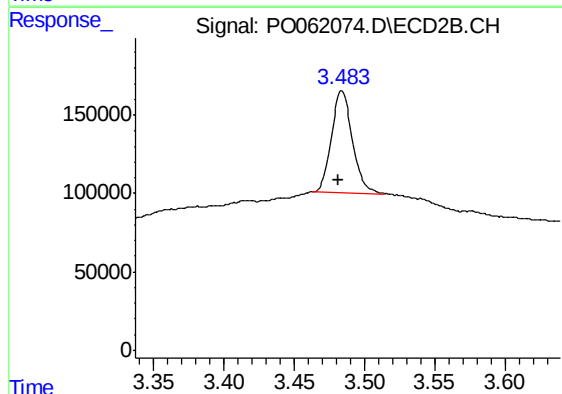


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.002 min
Response: 672442
Conc: 15.68 ng/ml m

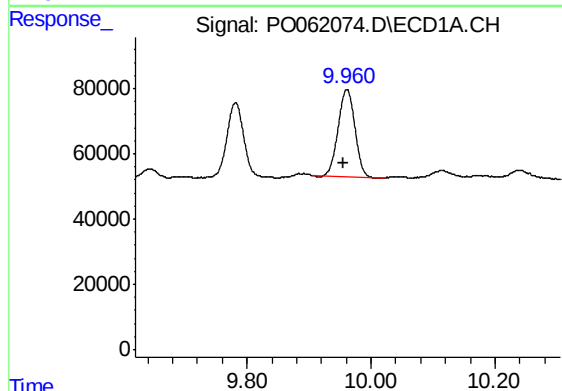

#2 Decachlorobiphenyl

R.T.: 9.961 min
Delta R.T.: 0.005 min
Response: 498689
Conc: 8.91 ng/ml

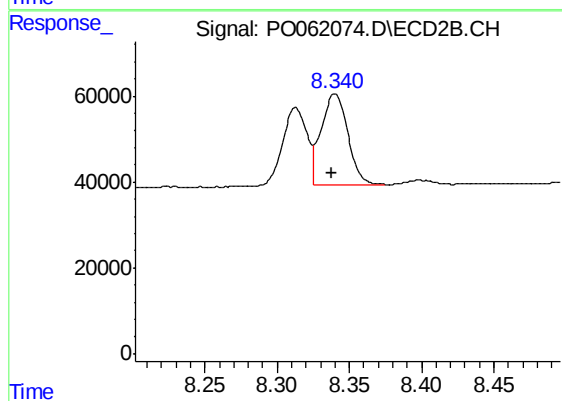

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.002 min
Response: 276085
Conc: 9.41 ng/ml m