

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101620\
 Data File : P0072415.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2020 8:28
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:41:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
2)	SA Decachlor...	0.000	8.695f	0	29397	N.D.	0.569 #
Target Compounds							
12)	L3 AR-1232-2	5.318	0.000	8992	0	9.443	N.D. #
24)	L5 AR-1248-4	6.537	0.000	117297	0	26.525	N.D. #
26)	L6 AR-1254-1	6.537f	0.000	117297	0	27.766	N.D. #
29)	L6 AR-1254-4	7.423	0.000	90661	0	13.678	N.D. #
30)	L6 AR-1254-5	7.837	0.000	34720	0	5.420	N.D. #
35)	L7 AR-1260-5	8.460	0.000	36866	0	2.538	N.D. #
37)	L8 AR-1262-2	8.460	0.000	36866	0	2.307	N.D. #
40)	L8 AR-1262-5	9.364f	0.000	63034	0	11.849	N.D. #
44)	L9 AR-1268-4	9.364f	0.000	63034	0	10.564	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
Data File : PO072415.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2020 8:28
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:41:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

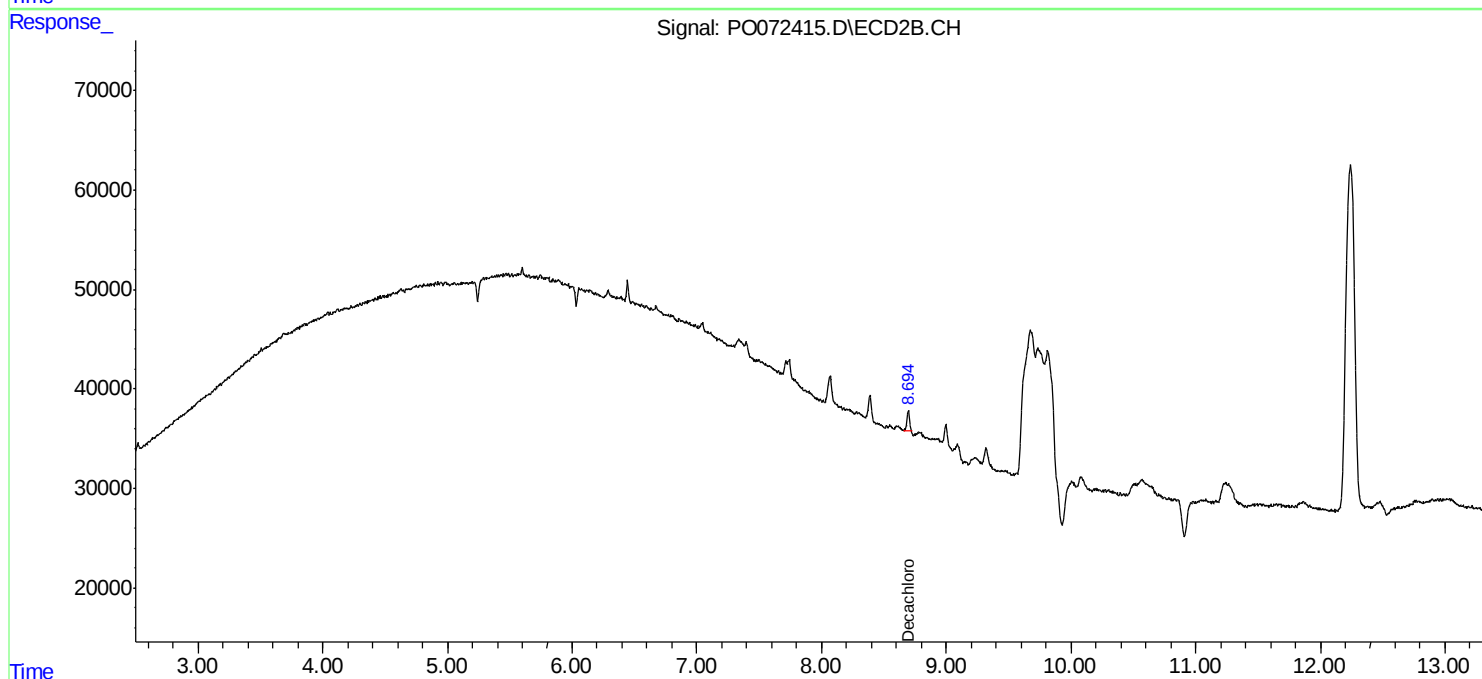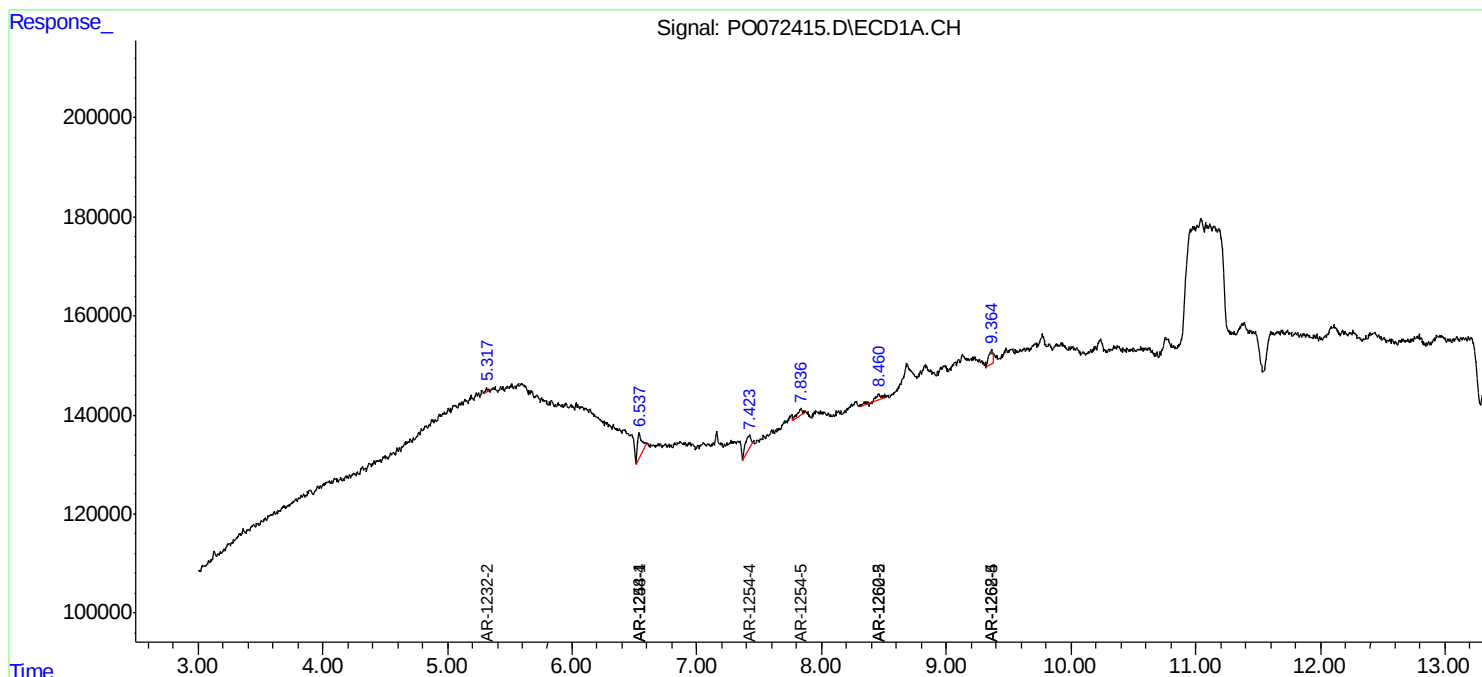


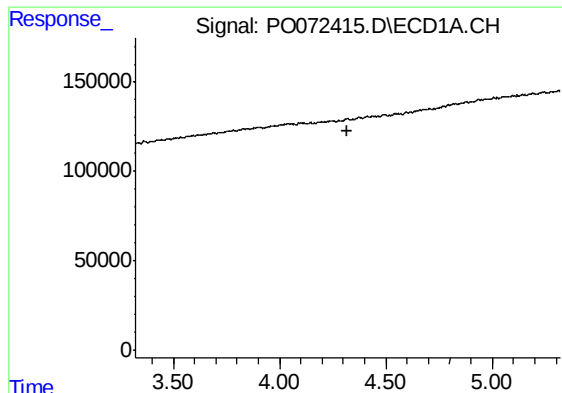

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.321 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

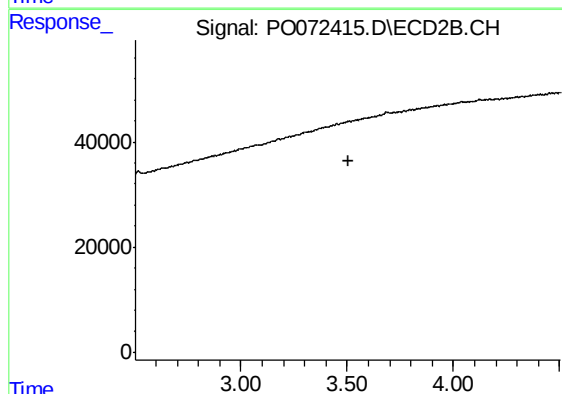


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.504 min
Response: 0
Conc: N.D.

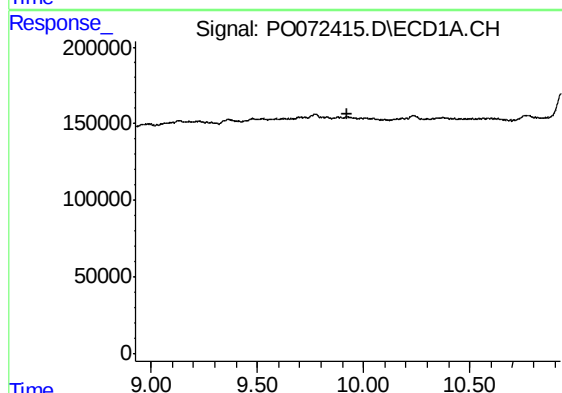


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.926 min
Response: 0
Conc: N.D.

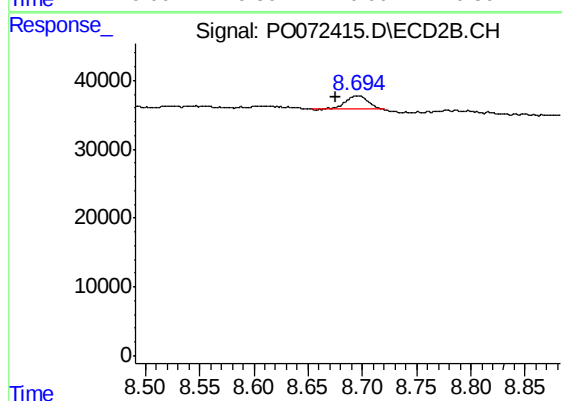

#2 Decachlorobiphenyl


R.T.: 8.695 min
Delta R.T.: 0.020 min
Response: 29397
Conc: 0.57 ng/ml

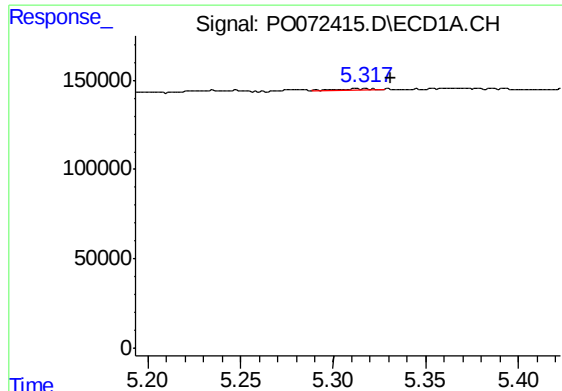

#12 AR-1232-2


R.T.: 5.318 min
Delta R.T.: -0.013 min
Response: 8992
Conc: 9.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

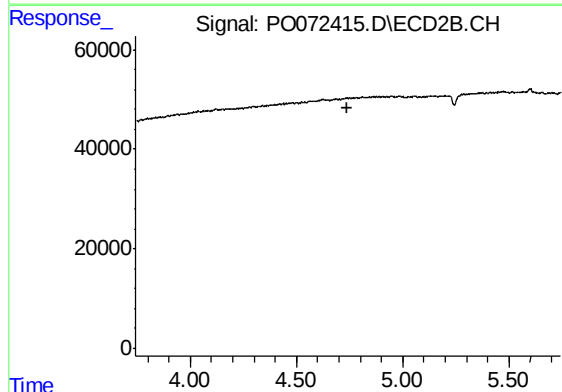


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.742 min
Response: 0
Conc: N.D.

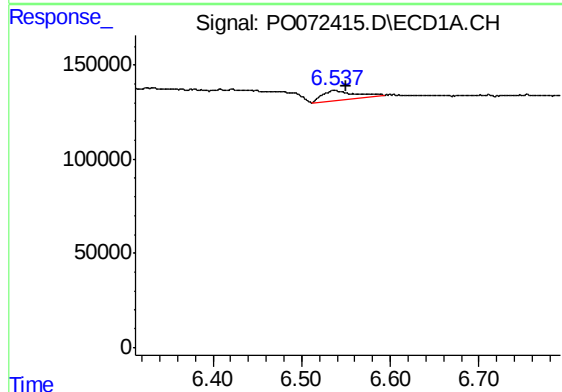


#24 AR-1248-4

R.T.: 6.537 min
Delta R.T.: -0.013 min
Response: 117297
Conc: 26.52 ng/ml

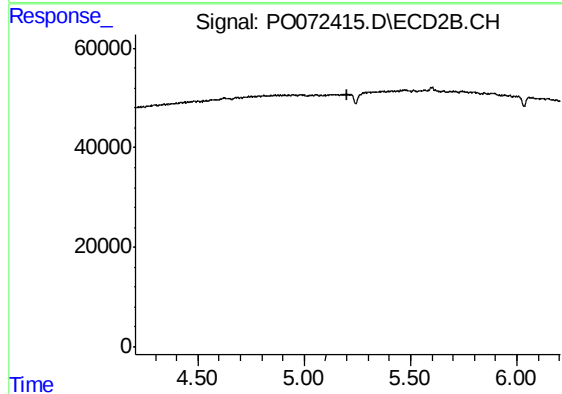

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.205 min
Response: 0
Conc: N.D.

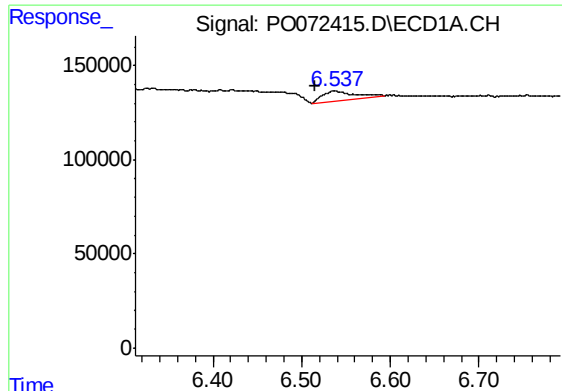

#26 AR-1254-1


R.T.: 6.537 min
Delta R.T.: 0.022 min
Response: 117297
Conc: 27.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

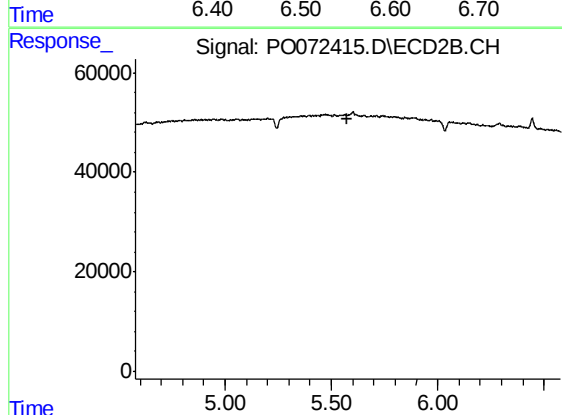


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.578 min
Response: 0
Conc: N.D.

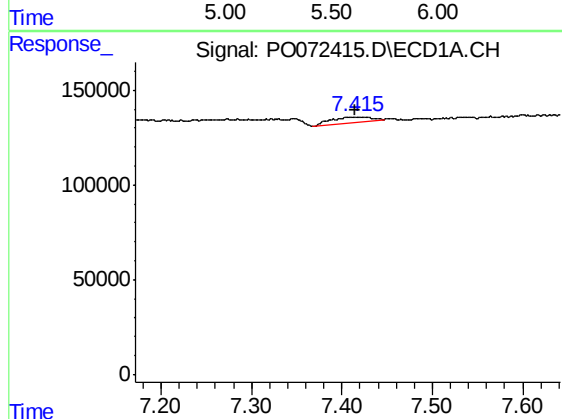


#29 AR-1254-4

R.T.: 7.423 min
Delta R.T.: 0.009 min
Response: 90661
Conc: 13.68 ng/ml

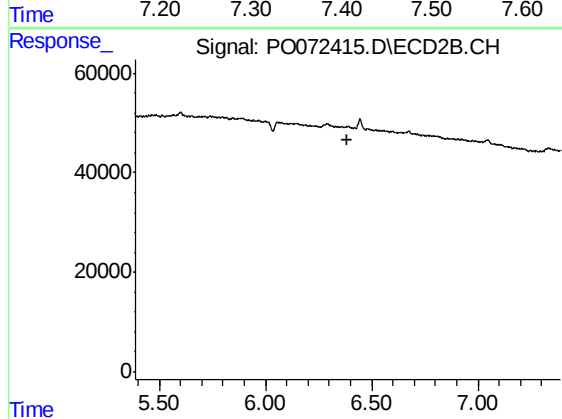

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.388 min
Response: 0
Conc: N.D.

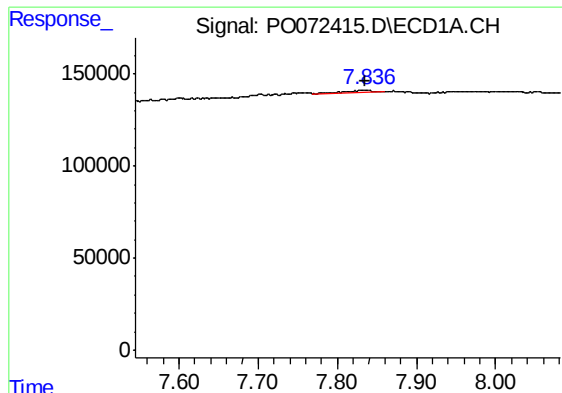

#30 AR-1254-5


R.T.: 7.837 min
Delta R.T.: 0.002 min
Response: 34720
Conc: 5.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

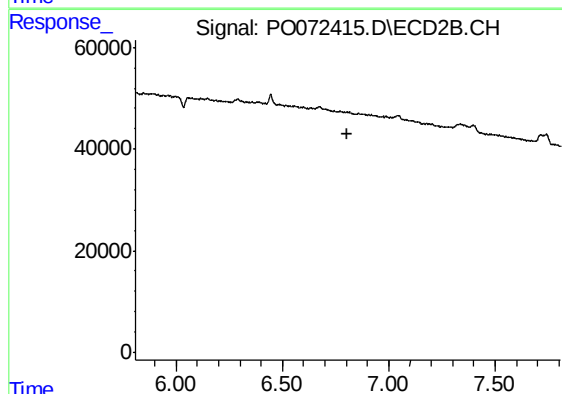


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

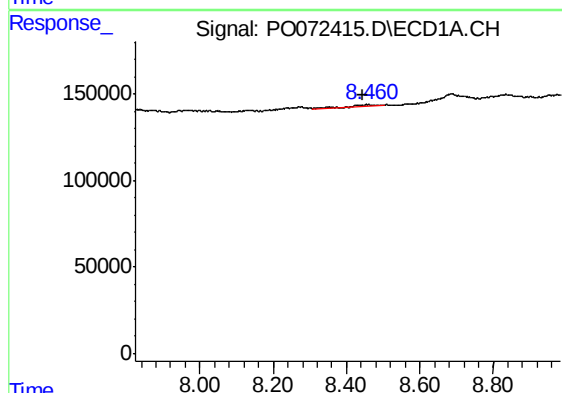


#35 AR-1260-5

R.T.: 8.460 min
Delta R.T.: 0.015 min
Response: 36866
Conc: 2.54 ng/ml

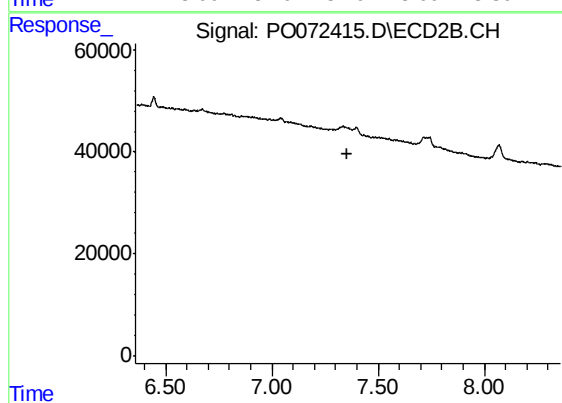

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

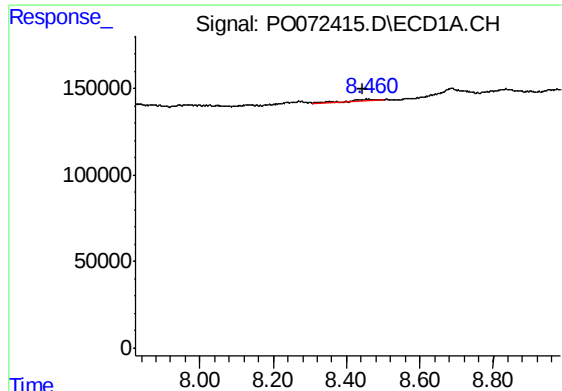

#37 AR-1262-2


R.T.: 8.460 min
Delta R.T.: 0.015 min
Response: 36866
Conc: 2.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

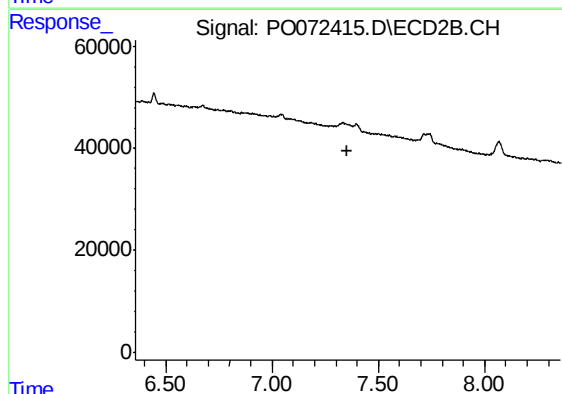


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.

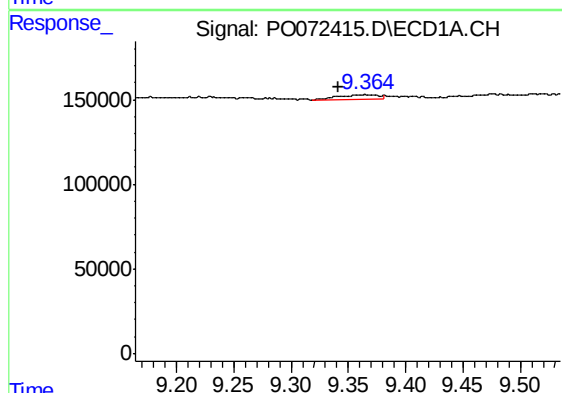


#40 AR-1262-5

R.T.: 9.364 min
Delta R.T.: 0.023 min
Response: 63034
Conc: 11.85 ng/ml

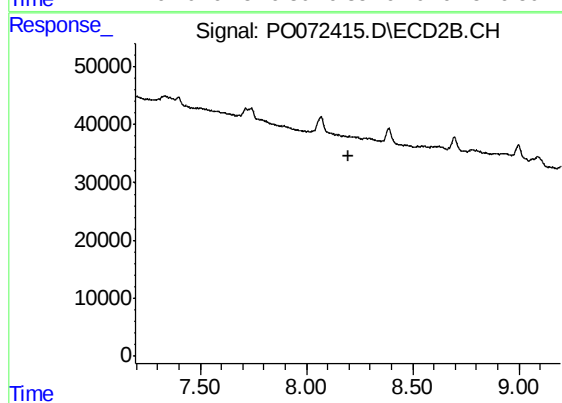

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.195 min
Response: 0
Conc: N.D.

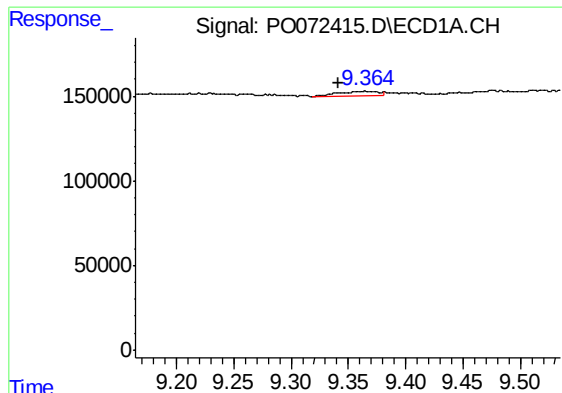

#44 AR-1268-4

R.T.: 9.364 min
Delta R.T.: 0.023 min
Response: 63034
Conc: 10.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

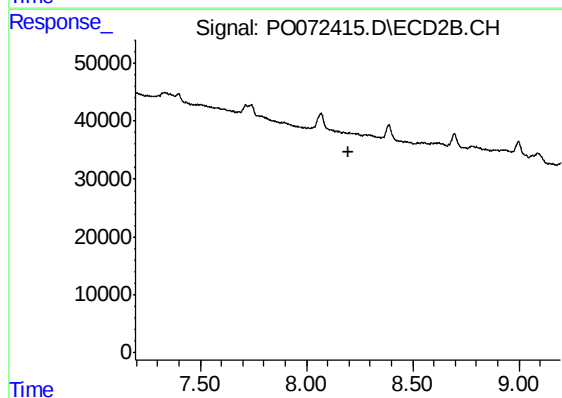

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.195 min
Response: 0
Conc: N.D.