

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101620\
 Data File : P0072429.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2020 14:01
 Operator : DD\AJ
 Sample : L4224-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-101520

Manual Integrations
 APPROVED

Ankita
 10/19/2020 3:07:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:50:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.504	1982601	984107	23.375m	23.363
2) SA Decachlor...	9.921	8.673	1948151	877968	17.662	16.984

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
Data File : PO072429.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2020 14:01
Operator : DD\AJ
Sample : L4224-06
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-101520


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:50:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

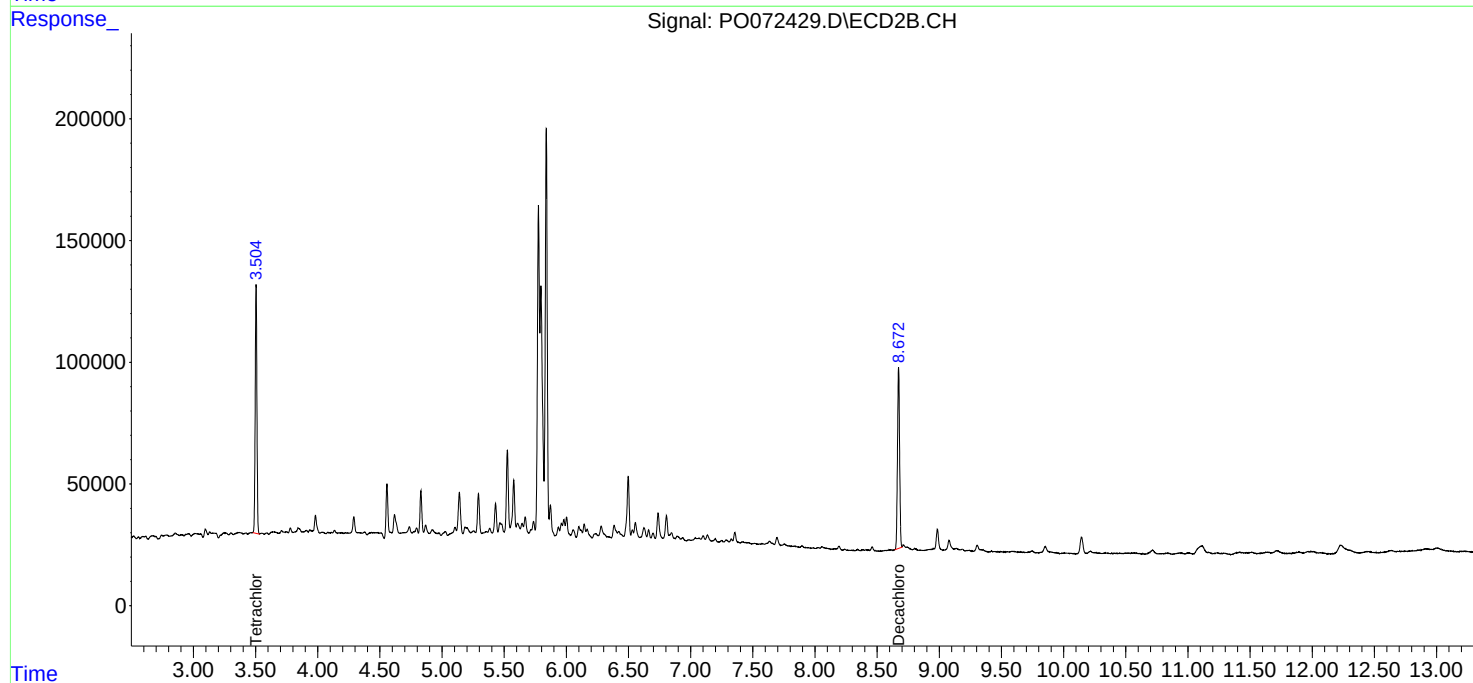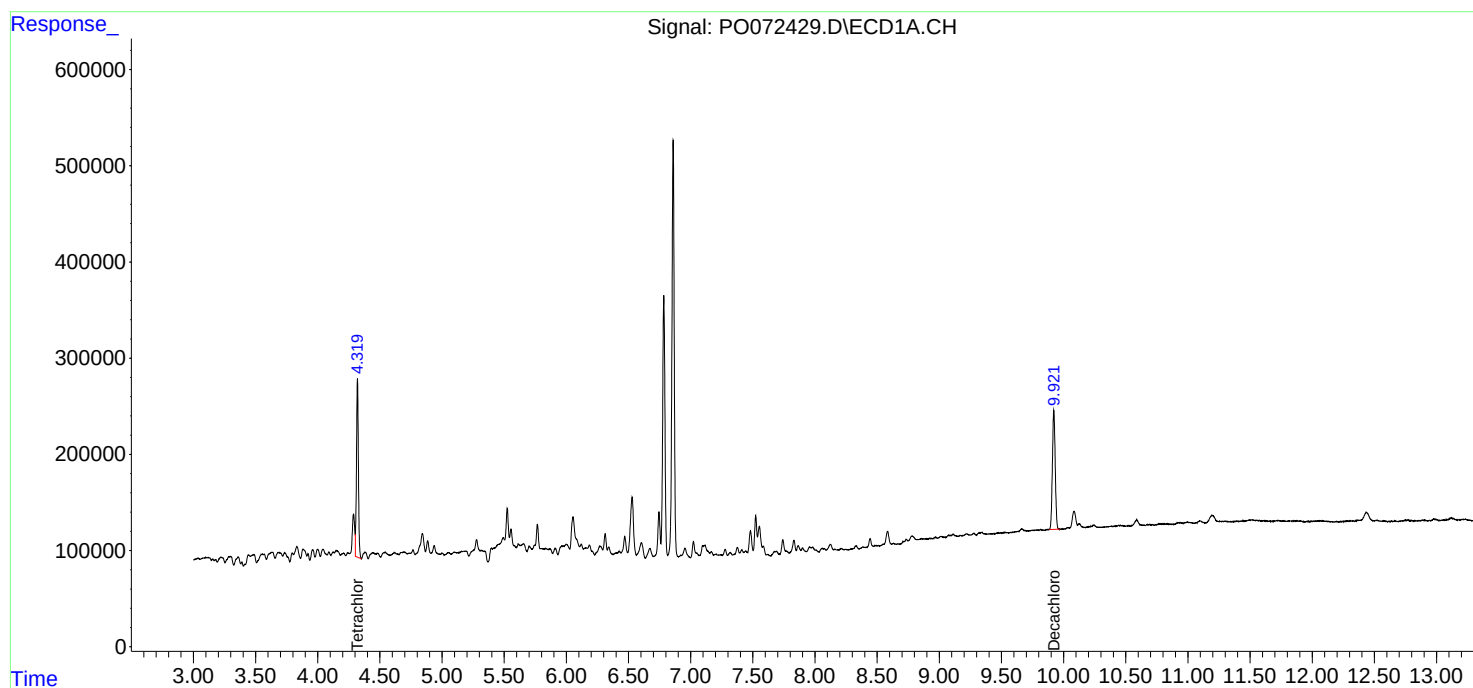

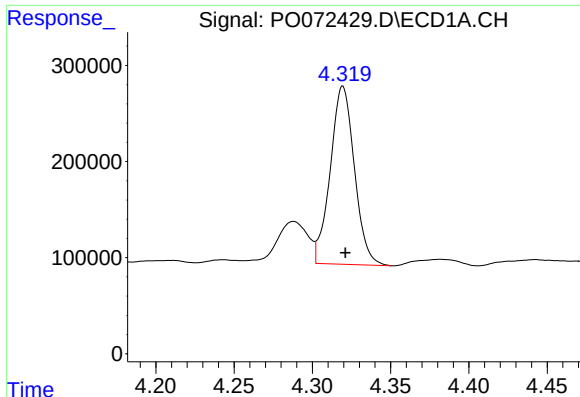


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 1982601
Conc: 23.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-03-101520


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:06 PM

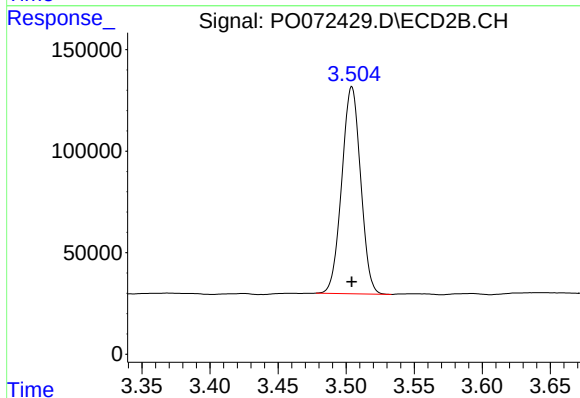


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 984107
Conc: 23.36 ng/ml

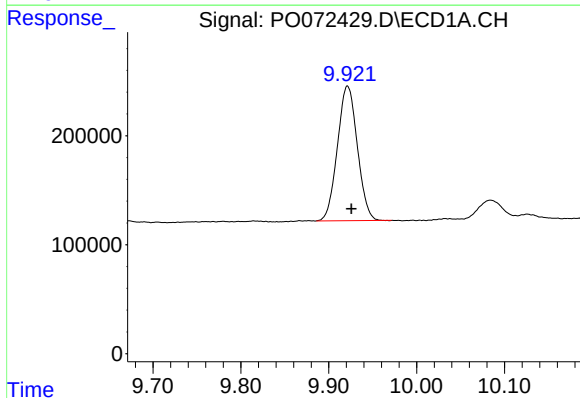

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.005 min
Response: 1948151
Conc: 17.66 ng/ml

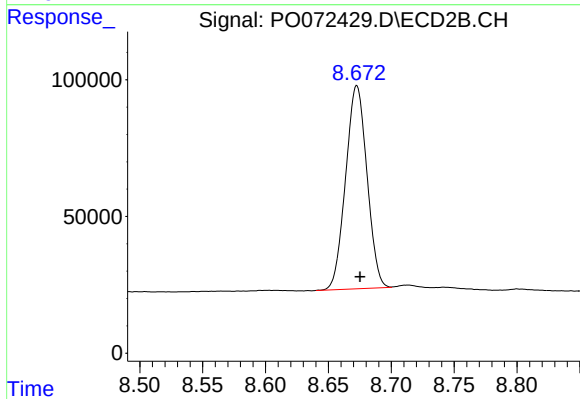

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.003 min
Response: 877968
Conc: 16.98 ng/ml