

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
 Data File : PO072437.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2020 16:36
 Operator : DD\AJ
 Sample : L4415-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CALTANK1-20201014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:55:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.320	3.504	1811934	894540	21.362	21.237
2)	SA Decachlor...	9.922	8.671	1735898	841562	15.737	16.279

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
Data File : PO072437.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2020 16:36
Operator : DD\AJ
Sample : L4415-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CALTANK1-20201014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:55:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

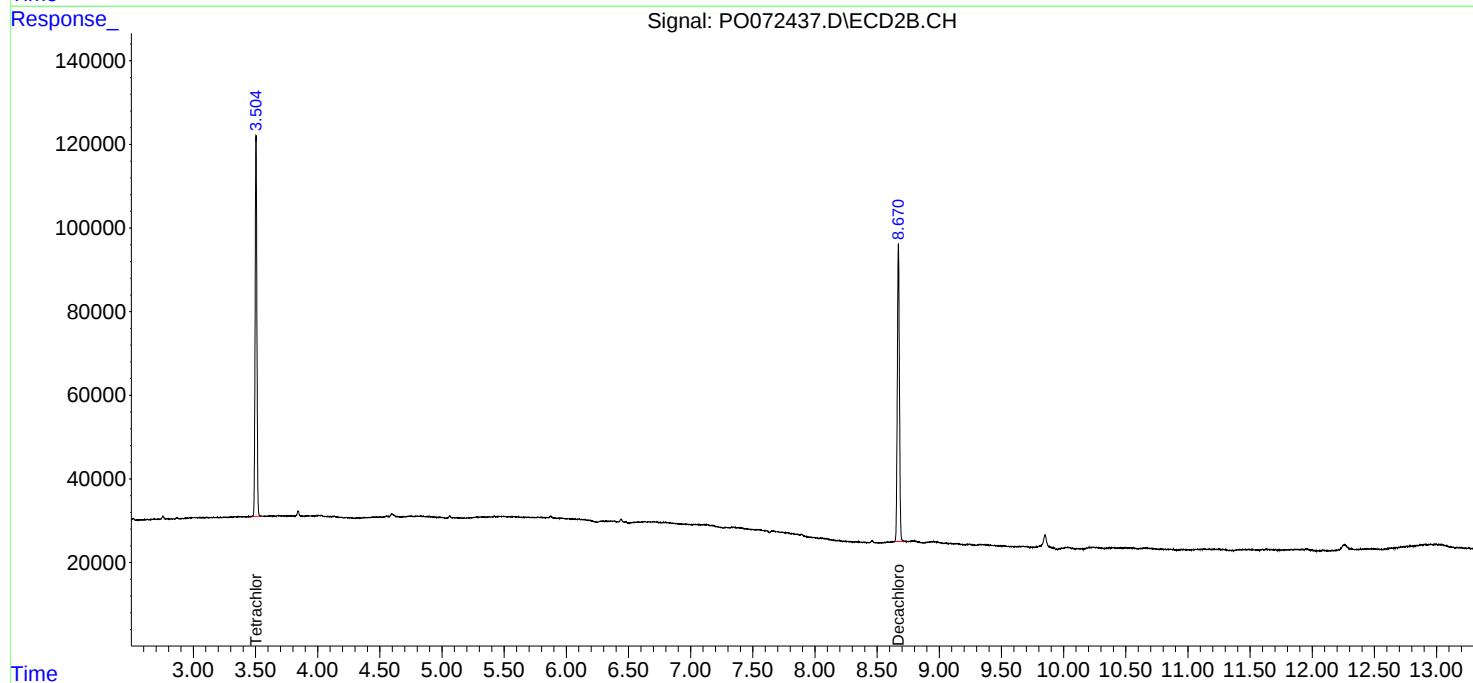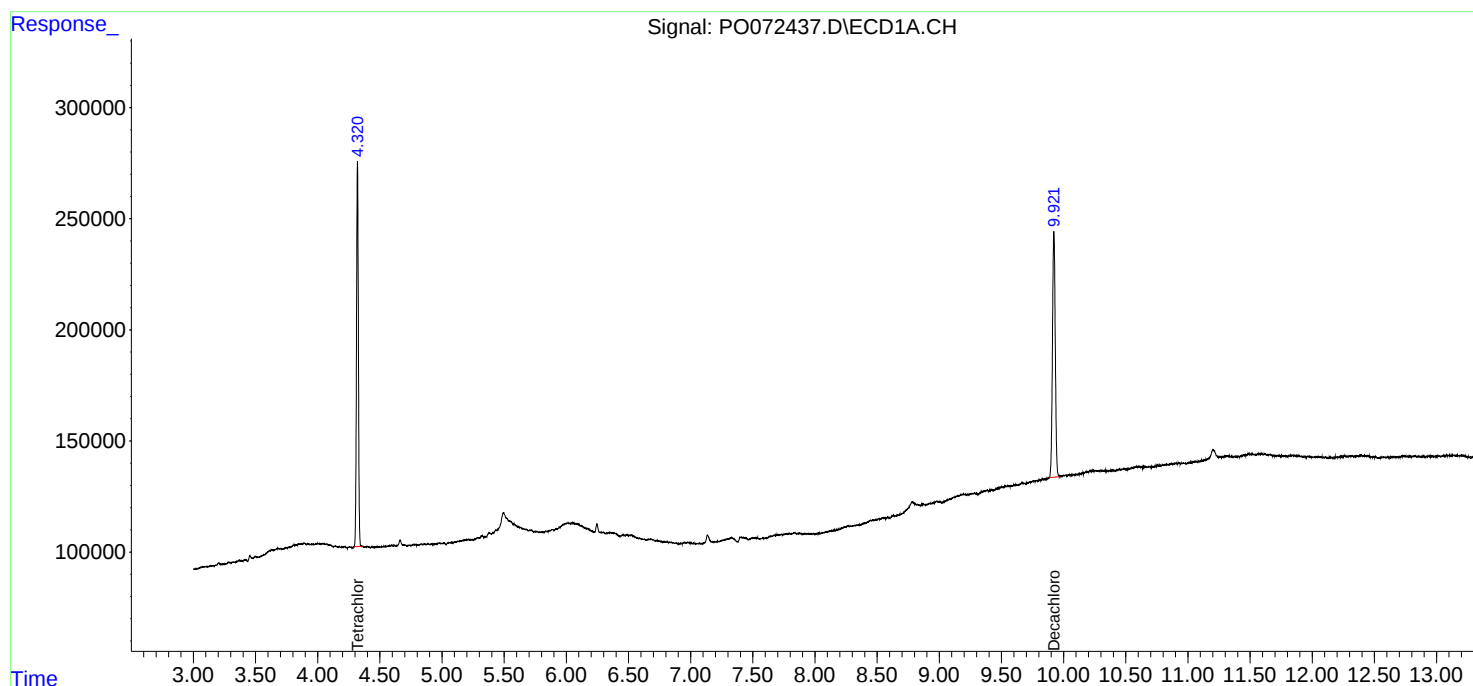


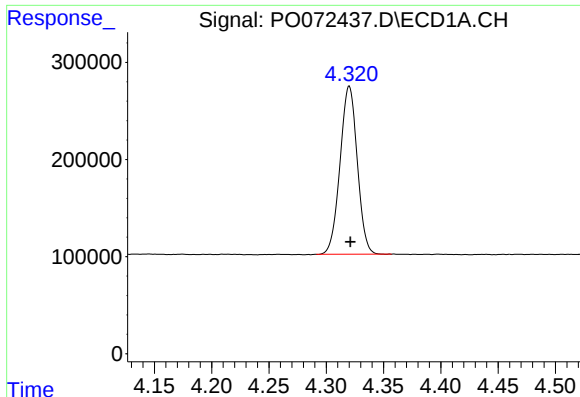

#1 Tetrachloro-m-xylene


R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 1811934
Conc: 21.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
CALTANK1-20201014

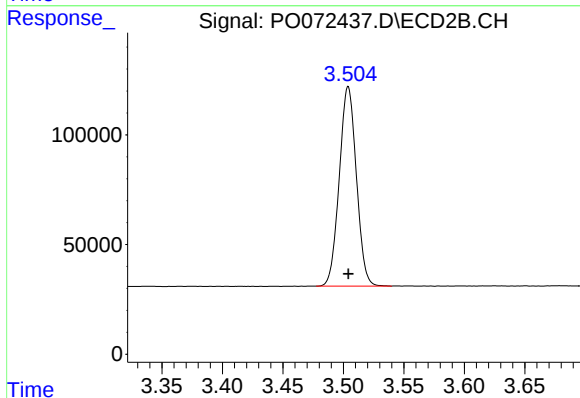


#1 Tetrachloro-m-xylene

R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 894540
Conc: 21.24 ng/ml

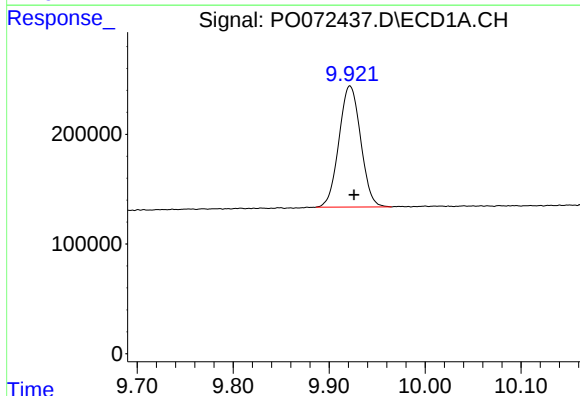

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.004 min
Response: 1735898
Conc: 15.74 ng/ml

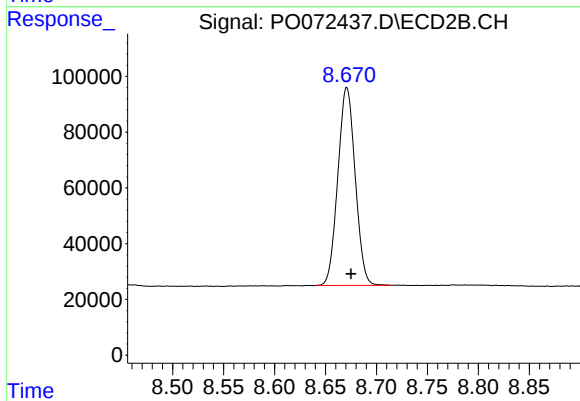

#2 Decachlorobiphenyl

R.T.: 8.671 min
Delta R.T.: -0.004 min
Response: 841562
Conc: 16.28 ng/ml