

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
 Data File : PO072444.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2020 19:10
 Operator : DD\AJ
 Sample : L4411-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 32696

Manual Integrations
 APPROVED

Ankita
 10/19/2020 3:07:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 05:59:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.507	2157531	758474	25.437m	18.007 #
2) SA Decachlor...	9.922	8.672	2291175	1066963	20.771	20.640

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
Data File : PO072444.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2020 19:10
Operator : DD\AJ
Sample : L4411-02
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
32696


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 05:59:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

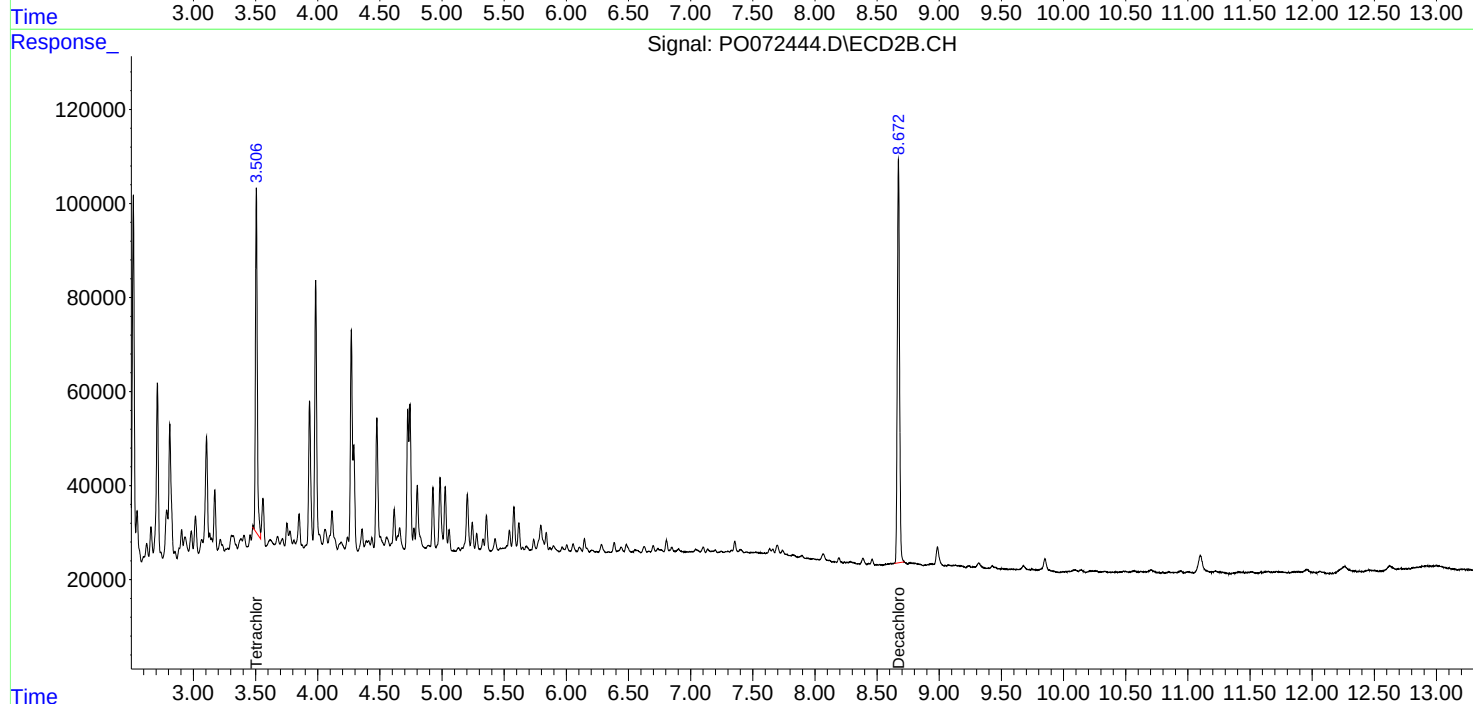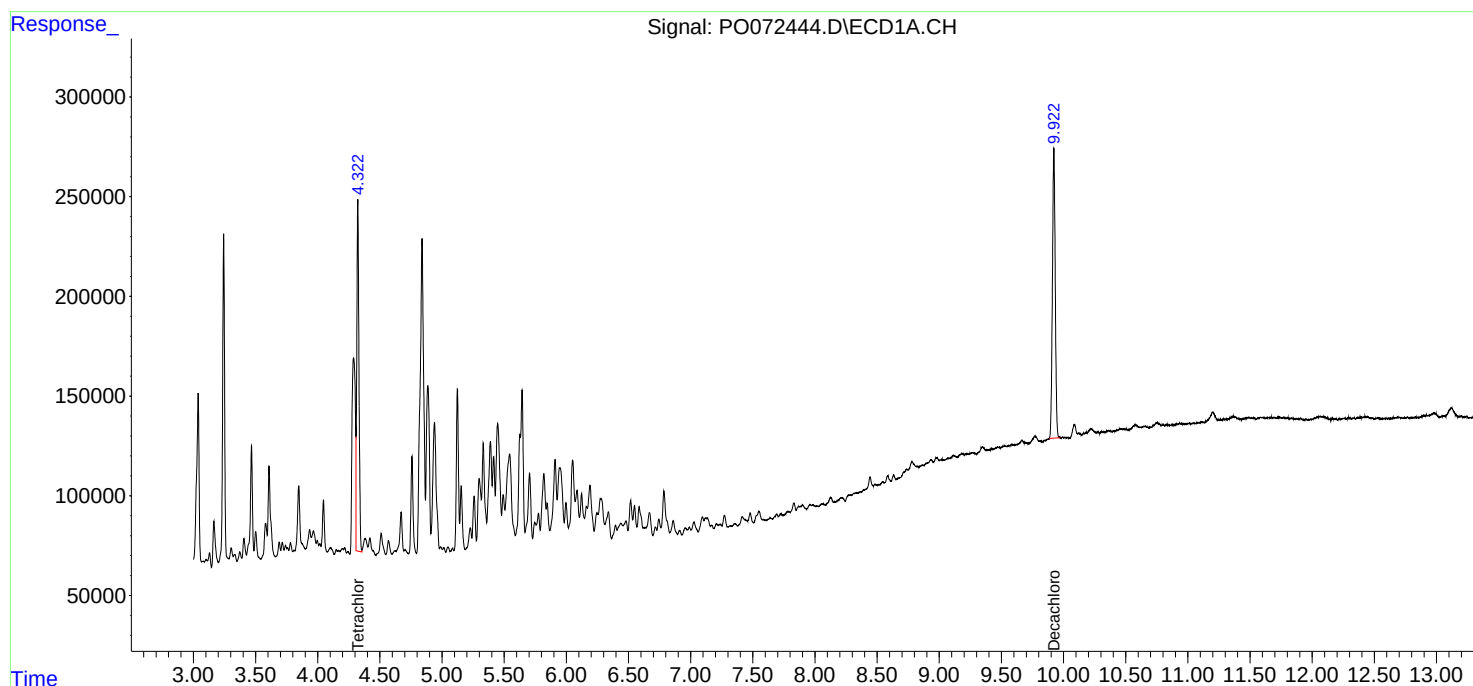

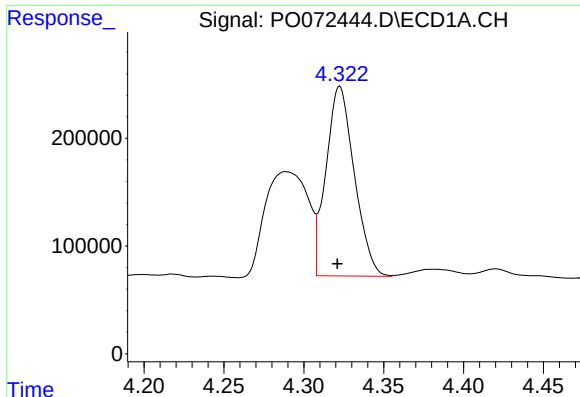


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: 0.001 min
Response: 2157531
Conc: 25.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
32696


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:38 PM

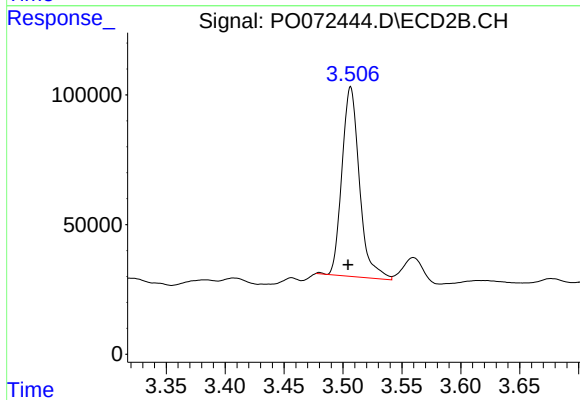


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: 0.002 min
Response: 758474
Conc: 18.01 ng/ml

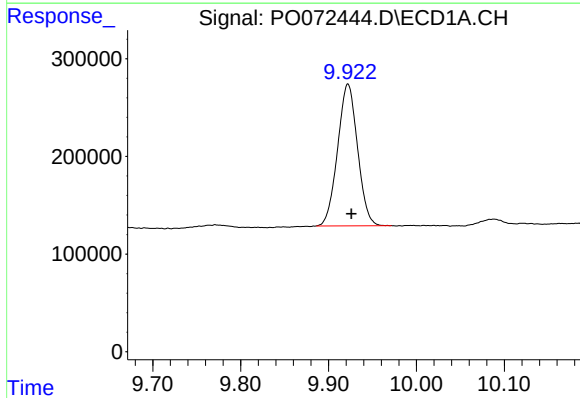

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.004 min
Response: 2291175
Conc: 20.77 ng/ml

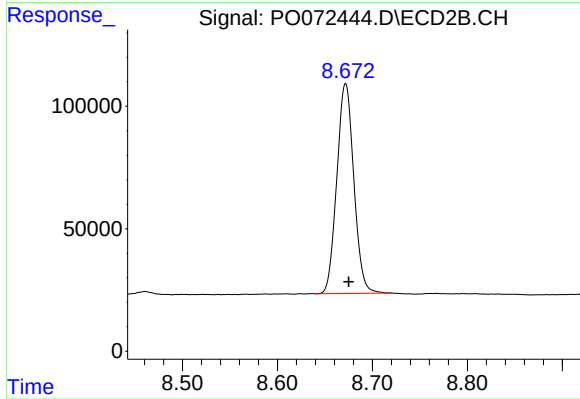

#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: -0.003 min
Response: 1066963
Conc: 20.64 ng/ml