

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0101620\
 Data File : P0072445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2020 19:27
 Operator : DD\AJ
 Sample : L4411-07 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 32697

Manual Integrations
 APPROVED

Ankita
 10/19/2020 3:07:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 06:23:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.503	733852	102913	8.652m	2.443m#
2) SA Decachlor...	9.922	8.670	239080	125721	2.167	2.432

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
Data File : PO072445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2020 19:27
Operator : DD\AJ
Sample : L4411-07 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
32697


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 06:23:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

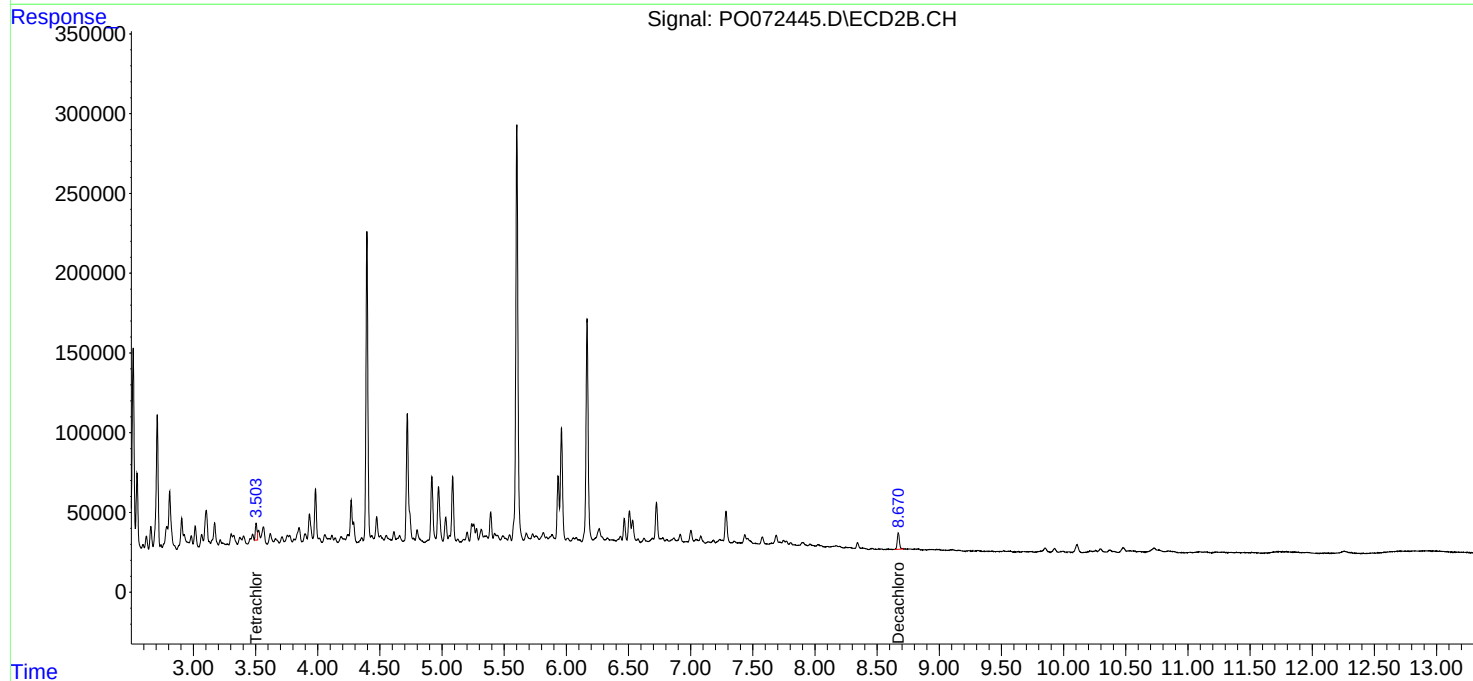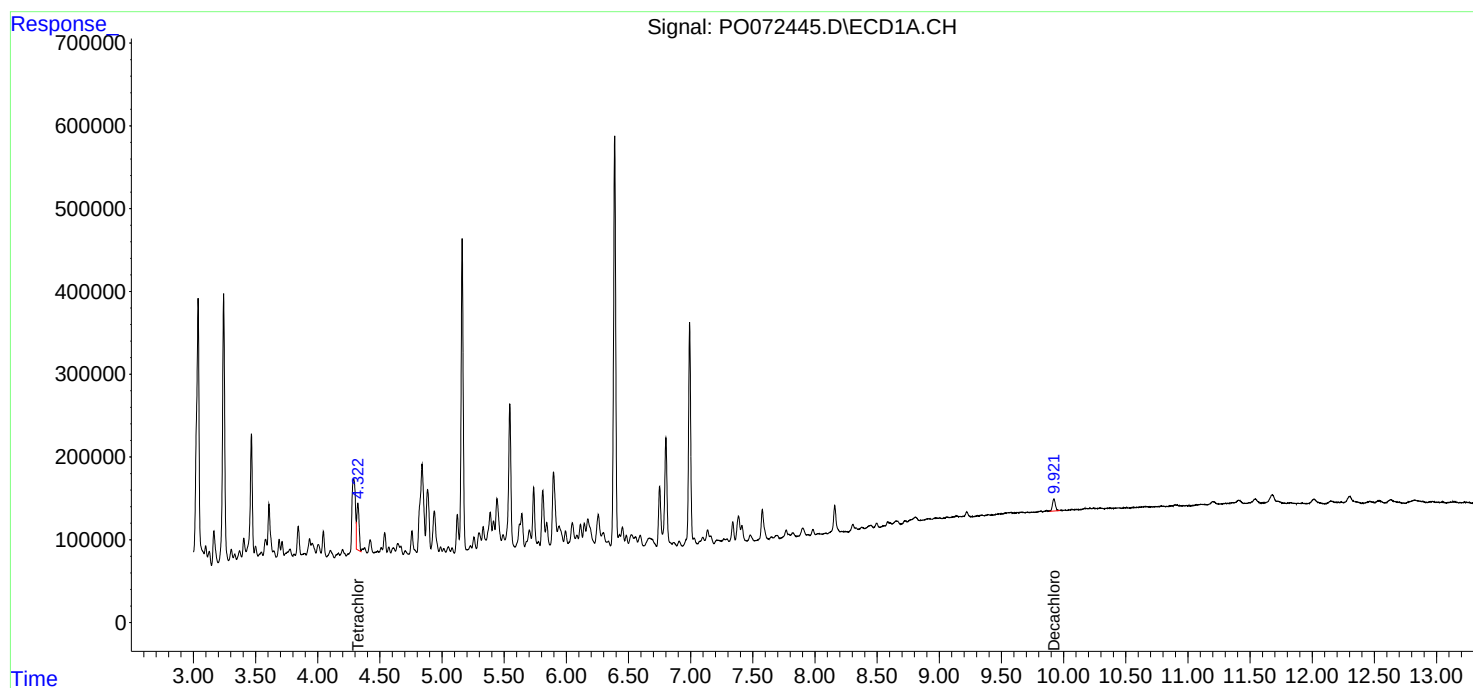

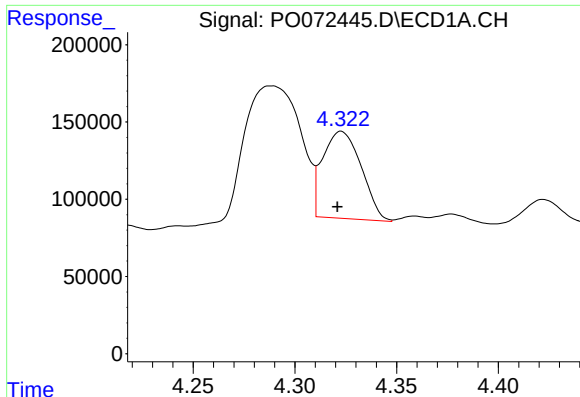


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: 0.001 min
Response: 733852
Conc: 8.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
32697


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:40 PM

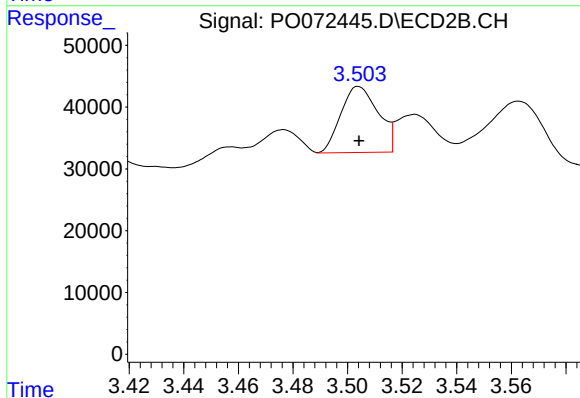


#1 Tetrachloro-m-xylene

R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 102913
Conc: 2.44 ng/ml m

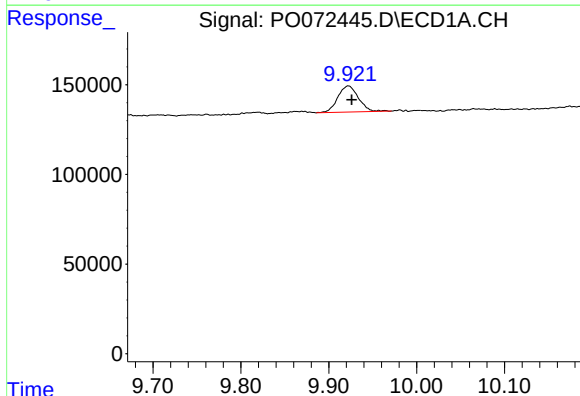

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.004 min
Response: 239080
Conc: 2.17 ng/ml

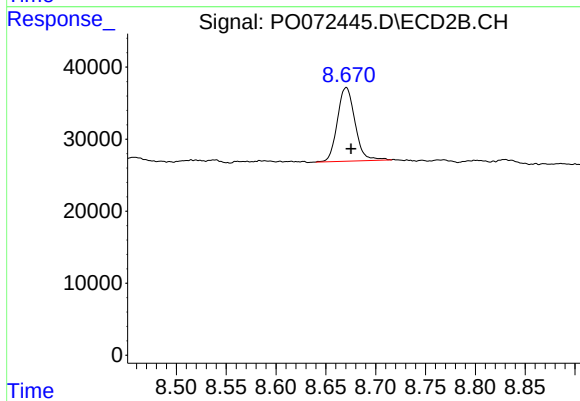

#2 Decachlorobiphenyl

R.T.: 8.670 min
Delta R.T.: -0.005 min
Response: 125721
Conc: 2.43 ng/ml