

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
 Data File : PO072446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Oct 2020 19:44
 Operator : DD\AJ
 Sample : L4413-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30688

Manual Integrations
 APPROVED

Ankita
 10/19/2020 3:07:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 06:24:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.507	1893946	1029052	22.329	24.430
2) SA Decachlor...	9.940	8.692f	1855826	861759	16.825m	16.670m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101620\
Data File : P0072446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Oct 2020 19:44
Operator : DD\AJ
Sample : L4413-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30688


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 06:24:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

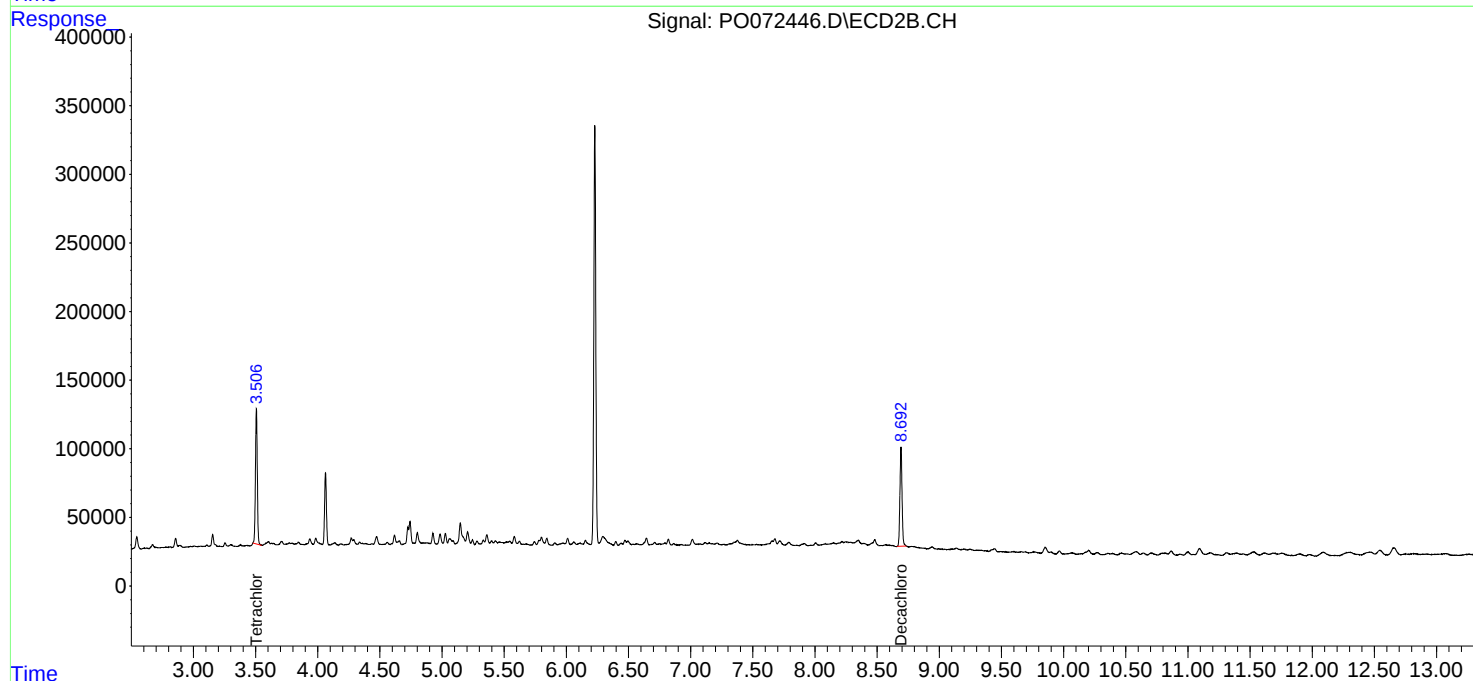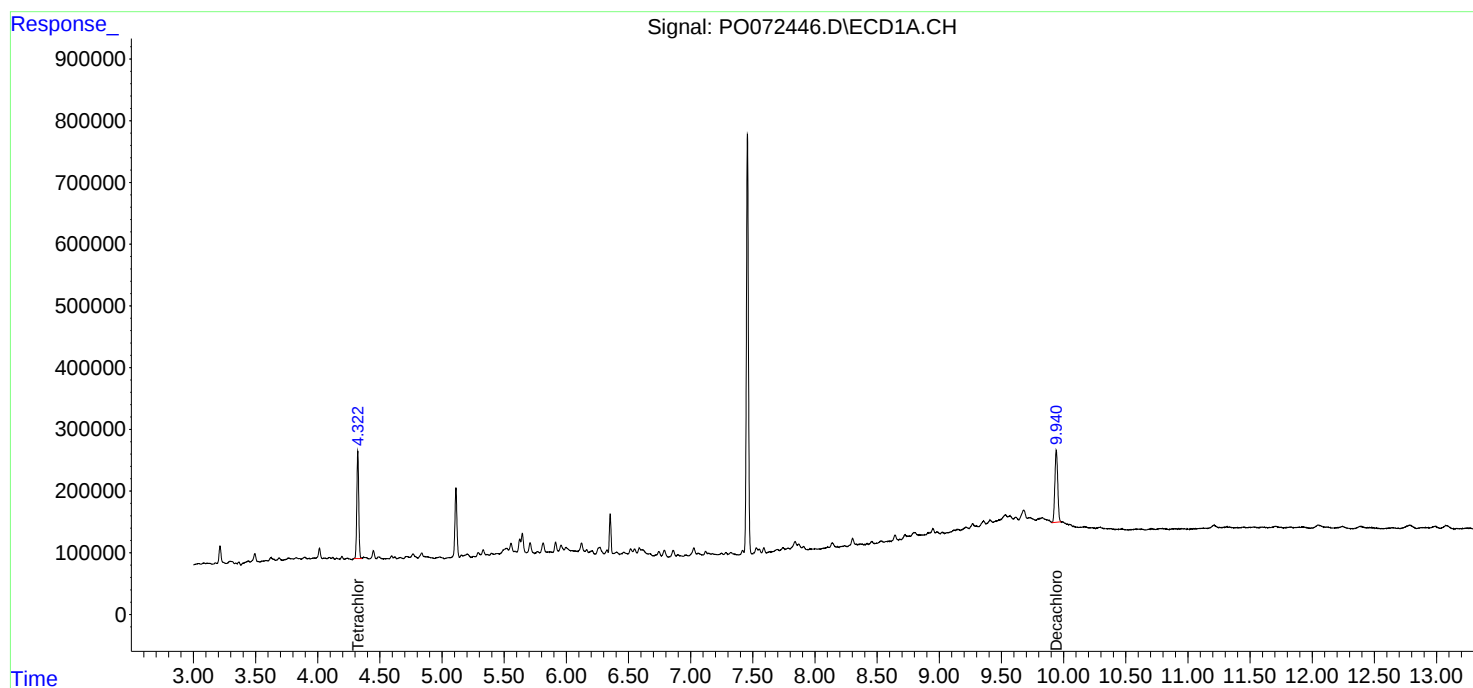

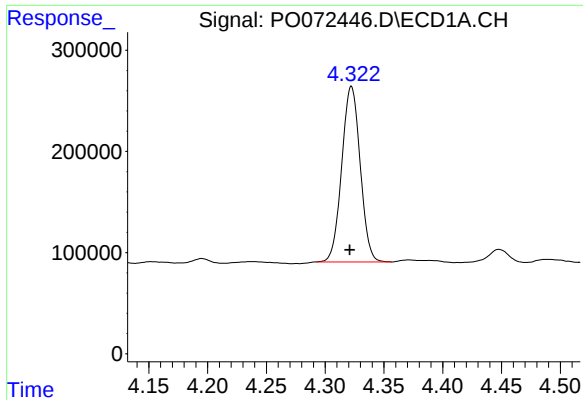


#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: 0.001 min
Response: 1893946
Conc: 22.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
30688


Manual Integrations
APPROVED

Ankita
10/19/2020 3:07:42 PM

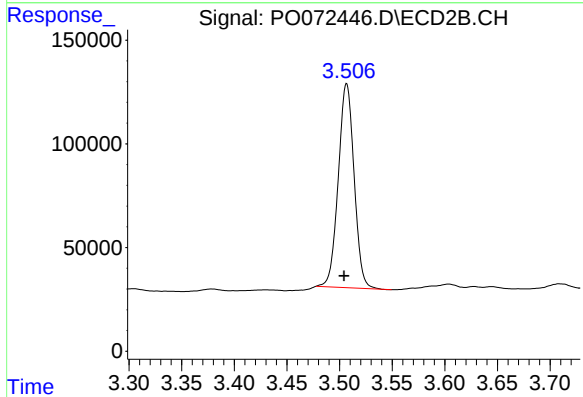


#1 Tetrachloro-m-xylene

R.T.: 3.507 min
Delta R.T.: 0.003 min
Response: 1029052
Conc: 24.43 ng/ml

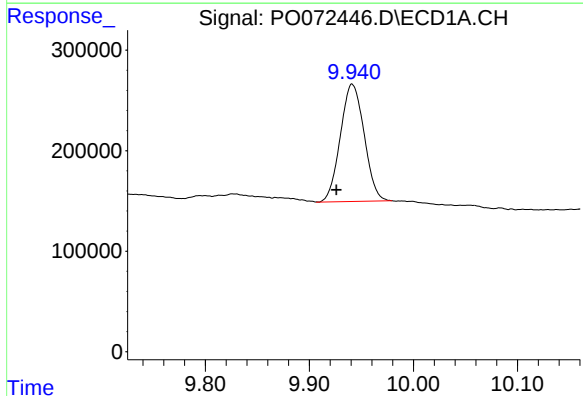

#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.014 min
Response: 1855826
Conc: 16.82 ng/ml m

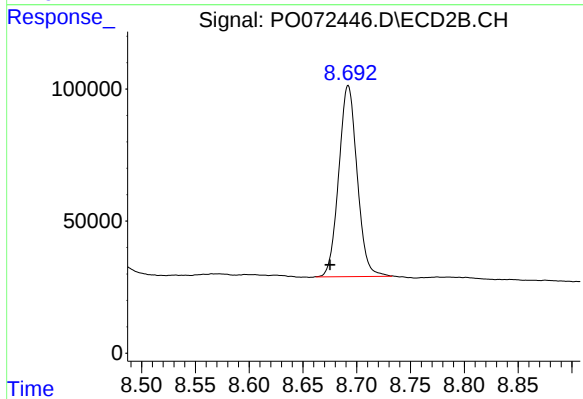

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: 0.016 min
Response: 861759
Conc: 16.67 ng/ml m