

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101623\
 Data File : P0098833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2023 15:03
 Operator : YP/AJ
 Sample : 04882-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-228

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/17/2023
 Supervised By :Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 15:47:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Sep 28 01:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.481	3.634	39677813	15282858	20.664	19.622
2) SA Decachlor...	10.294	8.639	22957624	9831796	18.913m	18.351m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101623\
Data File : P0098833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2023 15:03
Operator : YP/AJ
Sample : 04882-04
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 15:47:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0092723.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 28 01:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

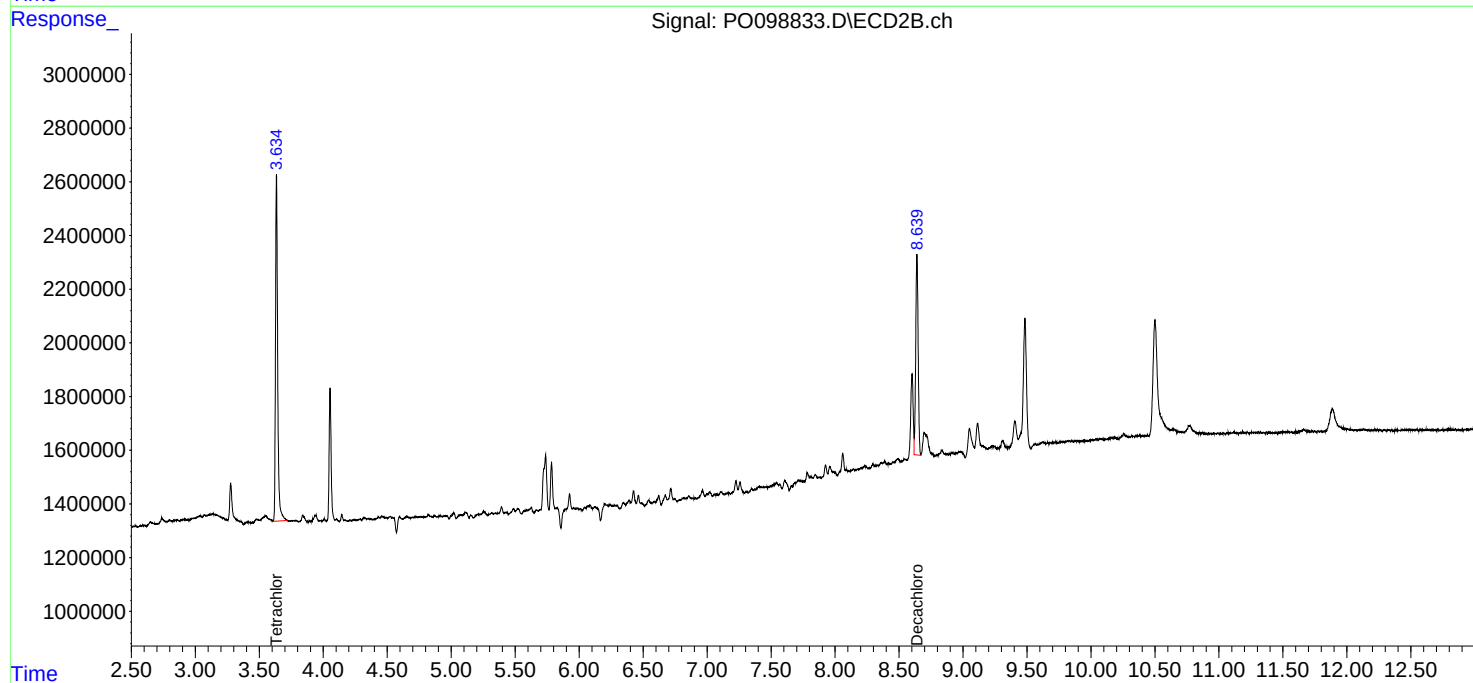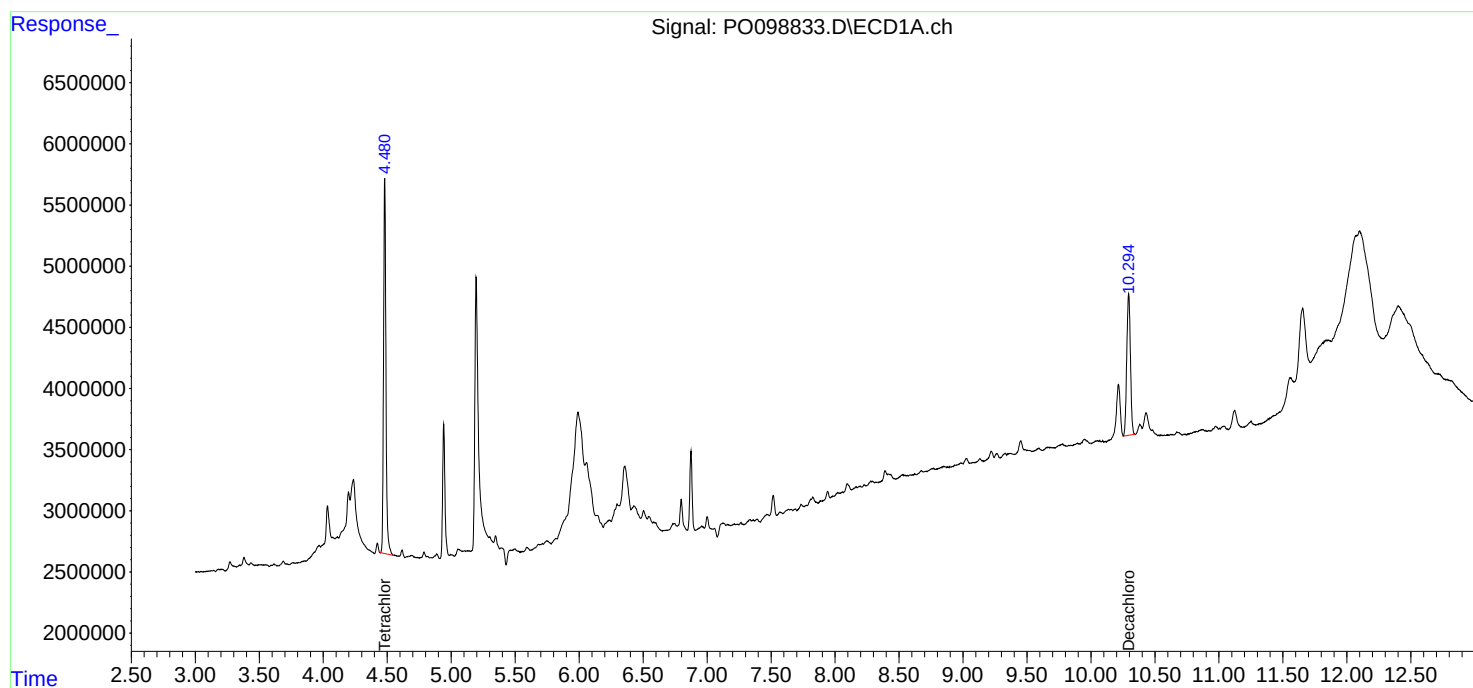

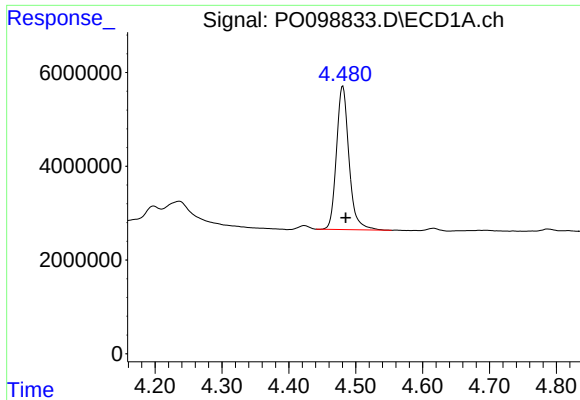


#1 Tetrachloro-m-xylene

R.T.: 4.481 min
Delta R.T.: -0.004 min
Response: 39677813
Conc: 20.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/17/2023
Supervised By :Ankita Jodhani 10/17/2023

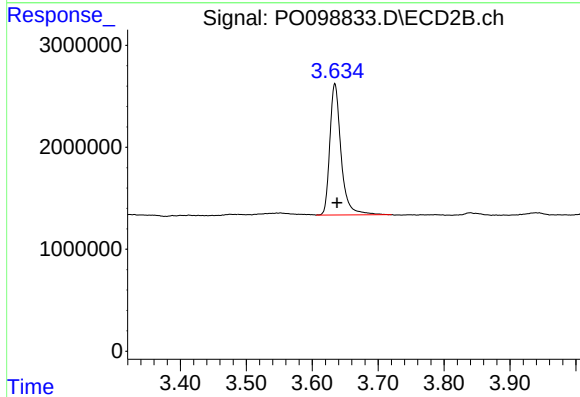


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.003 min
Response: 15282858
Conc: 19.62 ng/ml

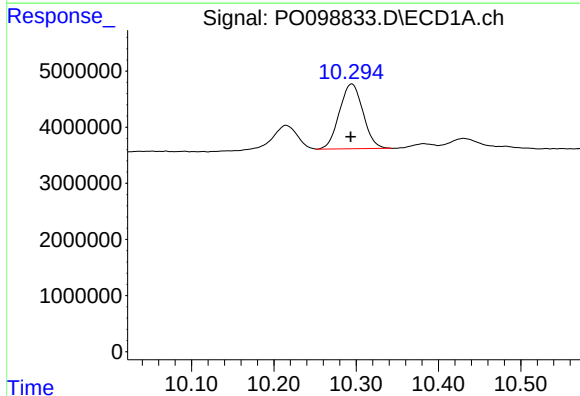

#2 Decachlorobiphenyl

R.T.: 10.294 min
Delta R.T.: 0.000 min
Response: 22957624
Conc: 18.91 ng/ml m

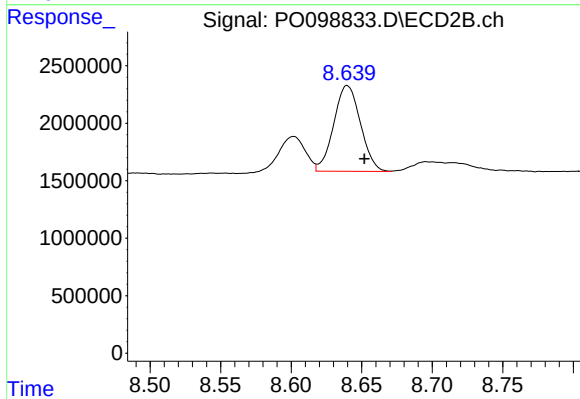

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.013 min
Response: 9831796
Conc: 18.35 ng/ml m