

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101624\
 Data File : PO107249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 01:28
 Operator : YP/AJ
 Sample : P4412-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KR-SS11

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/17/2024
 Supervised By :Ankita Jodhani 10/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 04:16:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:53:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.373	3.645	102.2E6	34677986	11.218	10.775
2) SA Decachlor...	10.062	8.640	151.6E6	64131076	61.810m	23.392 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101624\
Data File : PO107249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 01:28
Operator : YP/AJ
Sample : P4412-11
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KR-SS11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/17/2024
Supervised By :Ankita Jodhani 10/17/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 04:16:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:53:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

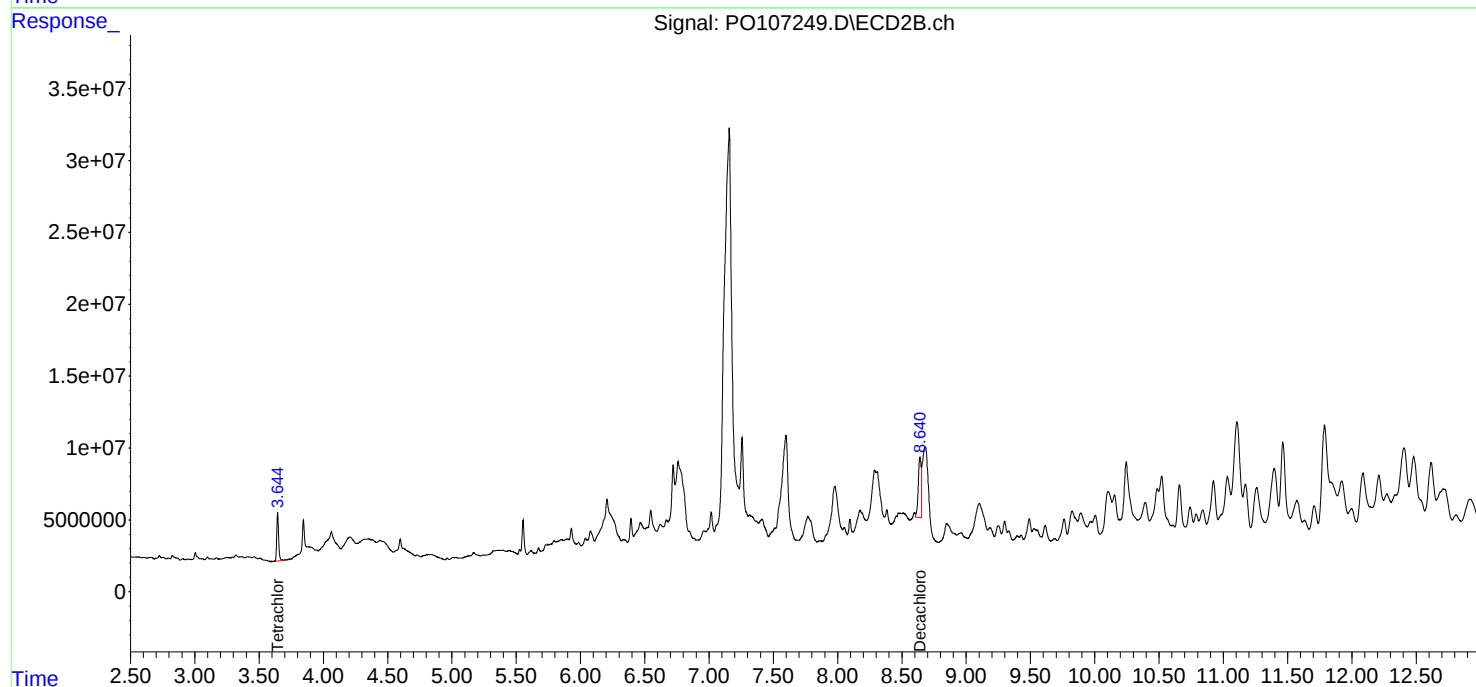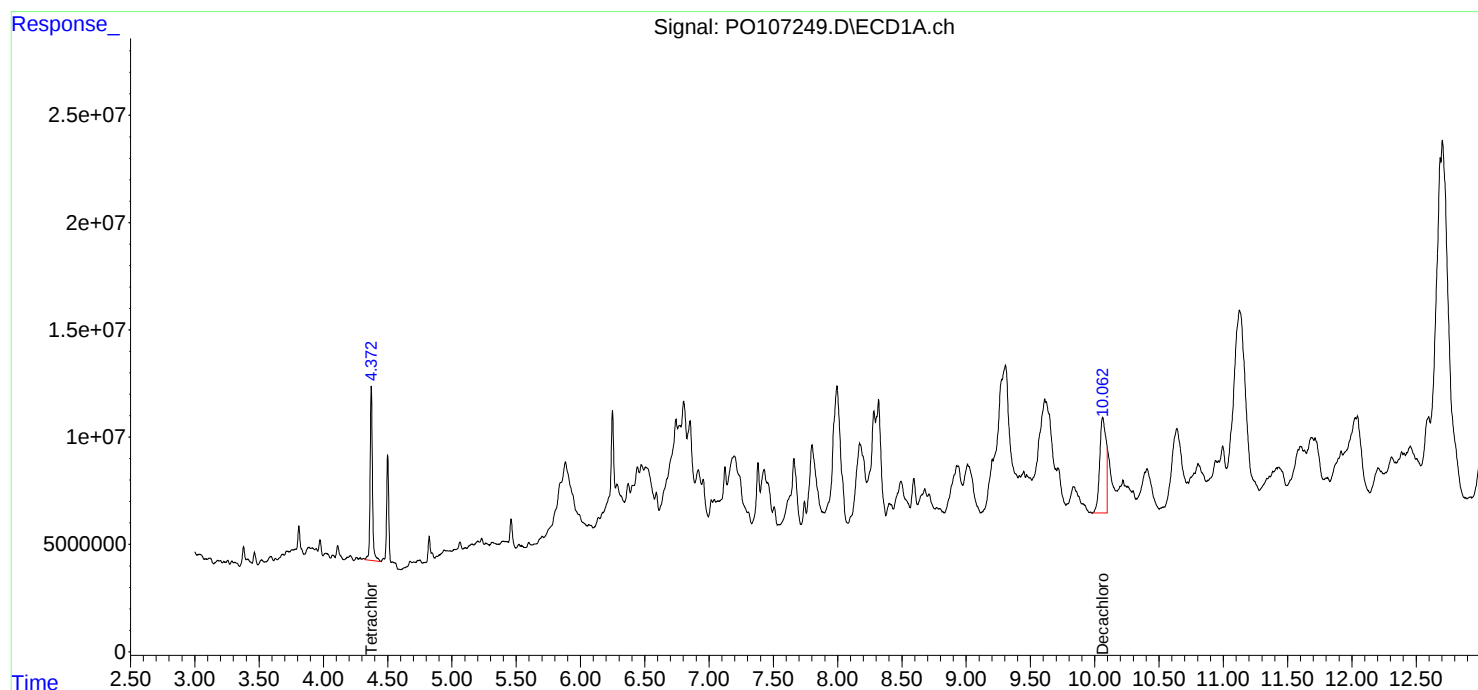

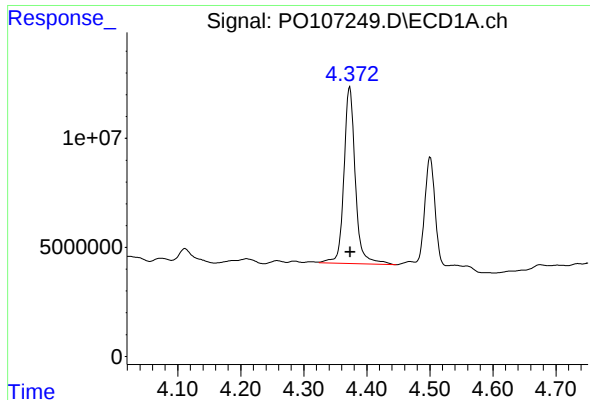


#1 Tetrachloro-m-xylene

R.T.: 4.373 min
Delta R.T.: -0.001 min
Response: 102243381
Conc: 11.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
KR-SS11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/17/2024
Supervised By :Ankita Jodhani 10/17/2024

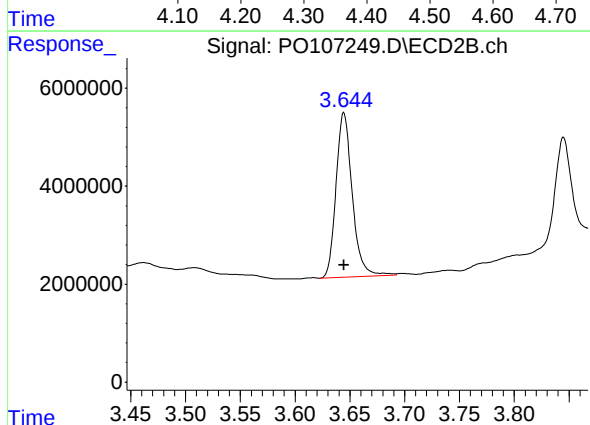


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 34677986
Conc: 10.77 ng/ml

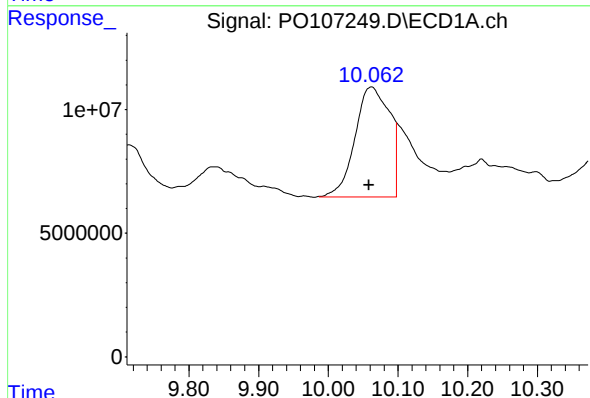

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: 0.003 min
Response: 151642073
Conc: 61.81 ng/ml m

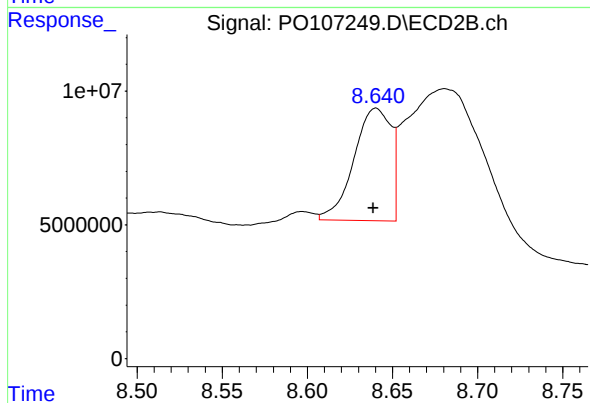

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.002 min
Response: 64131076
Conc: 23.39 ng/ml