

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101625\
Data File : PO114441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2025 17:27
Operator : YP/AJ
Sample : Q3356-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AUD-25-0169-AUD-25-0170

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:56:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 10 06:46:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.357	3.660	116.0E6	87026999	21.365	21.744
2) SA Decachlor...	9.942	8.667	26880435	24753523	7.382	7.426

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO101625\
Data File : PO114441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2025 17:27
Operator : YP/AJ
Sample : Q3356-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AUD-25-0169-AUD-25-0170

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:56:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 10 06:46:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

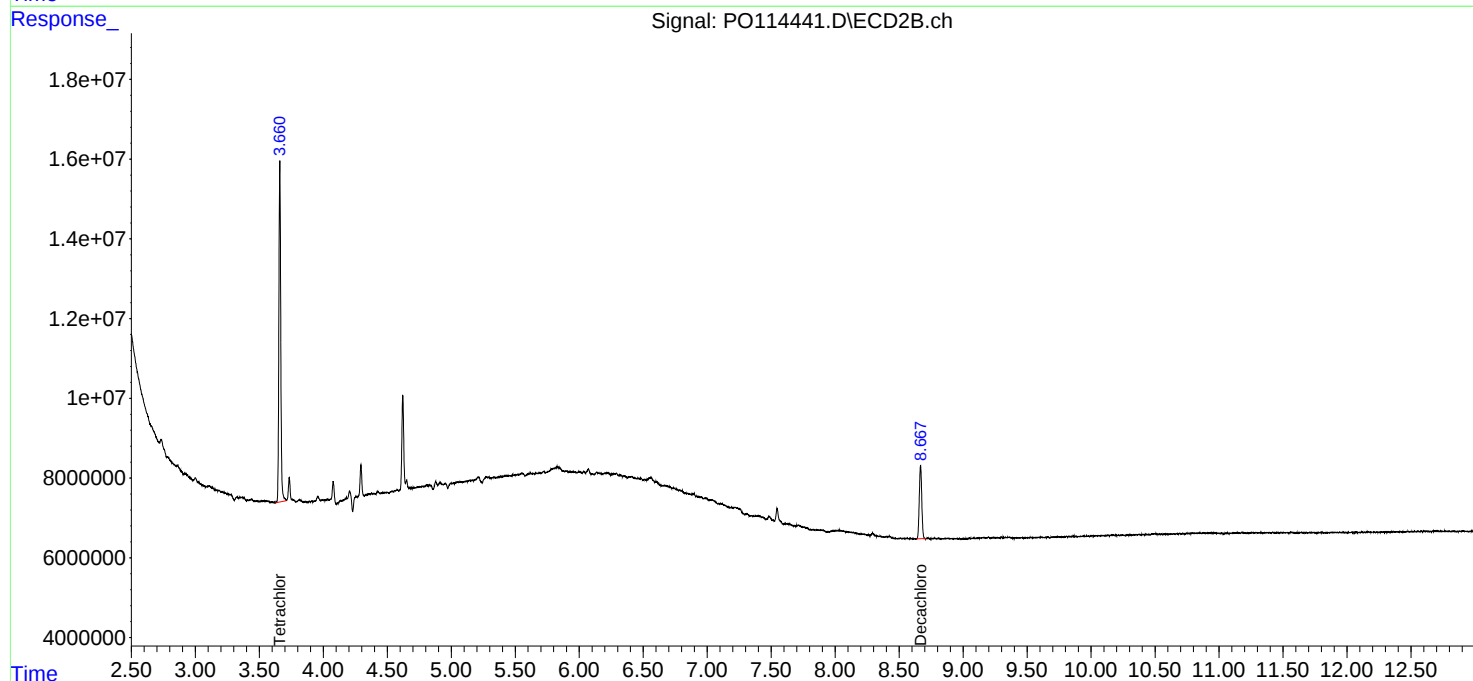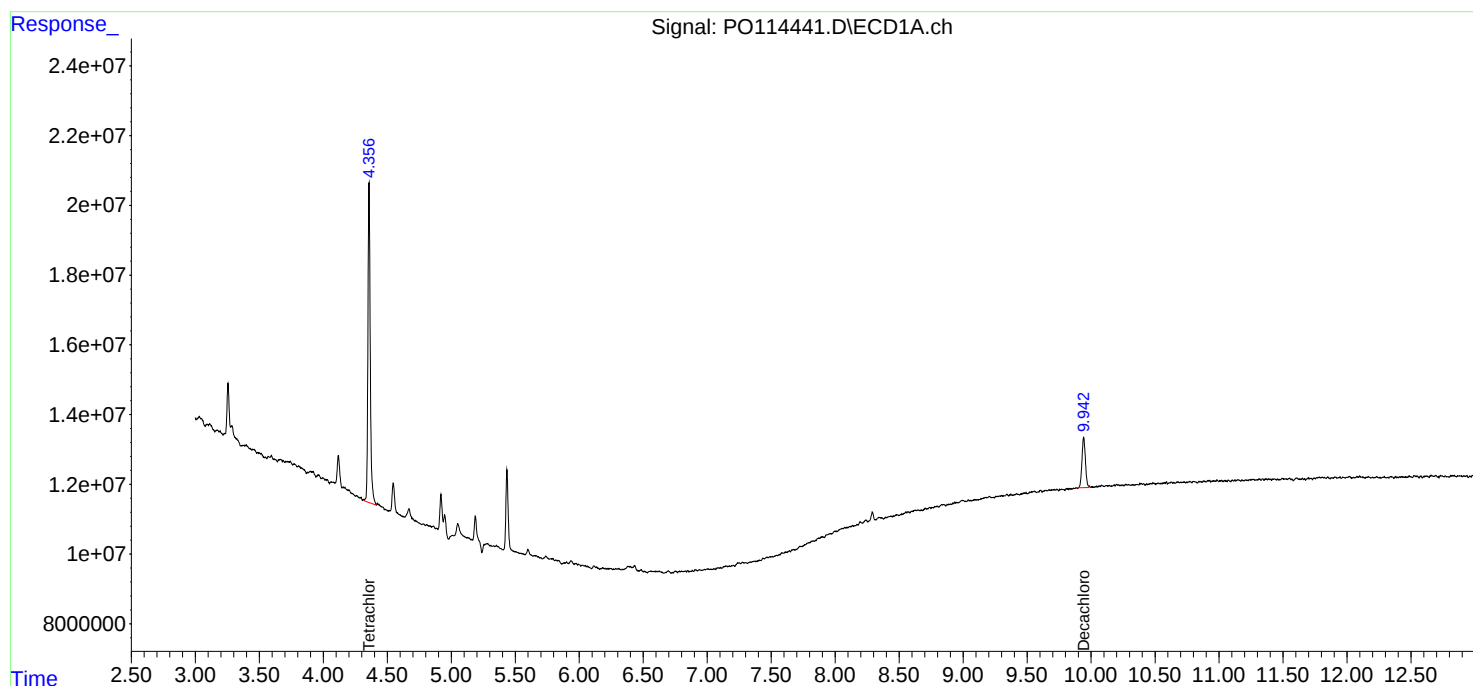


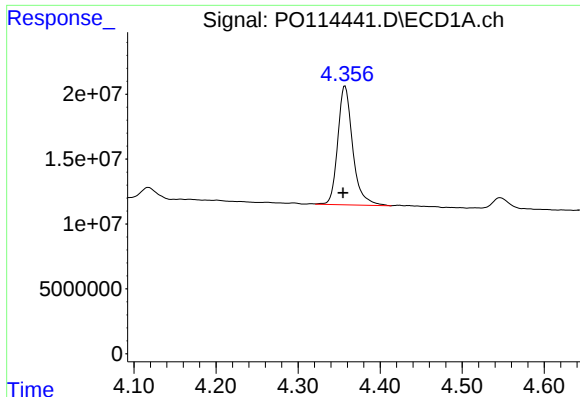

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: 0.002 min
Response: 115989680
Conc: 21.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-25-0169-AUD-25-0170

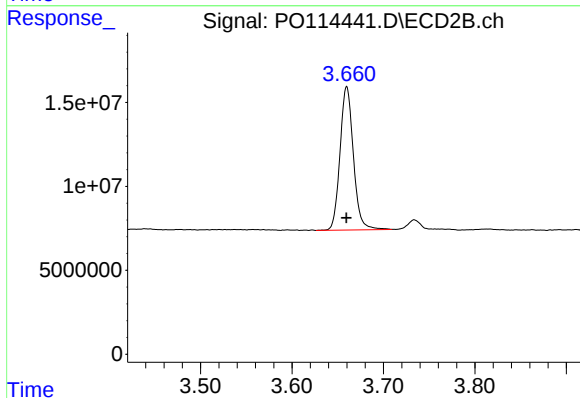


#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: 0.000 min
Response: 87026999
Conc: 21.74 ng/ml

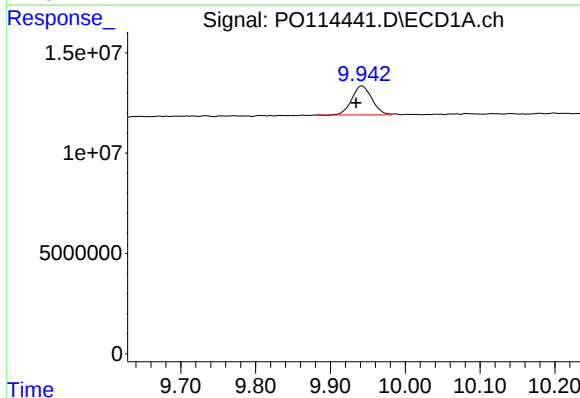

#2 Decachlorobiphenyl

R.T.: 9.942 min
Delta R.T.: 0.008 min
Response: 26880435
Conc: 7.38 ng/ml

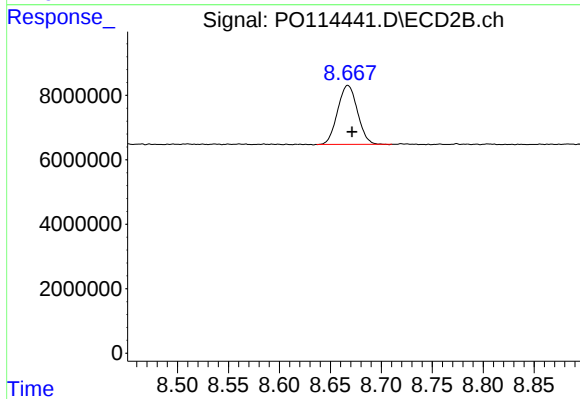

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.004 min
Response: 24753523
Conc: 7.43 ng/ml