

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101718\
 Data File : PO050148.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Oct 2018 20:09
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 07:47:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 18 07:47:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.361	4942645	4205080	24.350	21.050
2) SA Decachlor...	10.075	8.121	5208501	4489180	21.628	23.076

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO101718\
Data File : P0050148.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Oct 2018 20:09
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 07:47:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101718.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 18 07:47:12 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

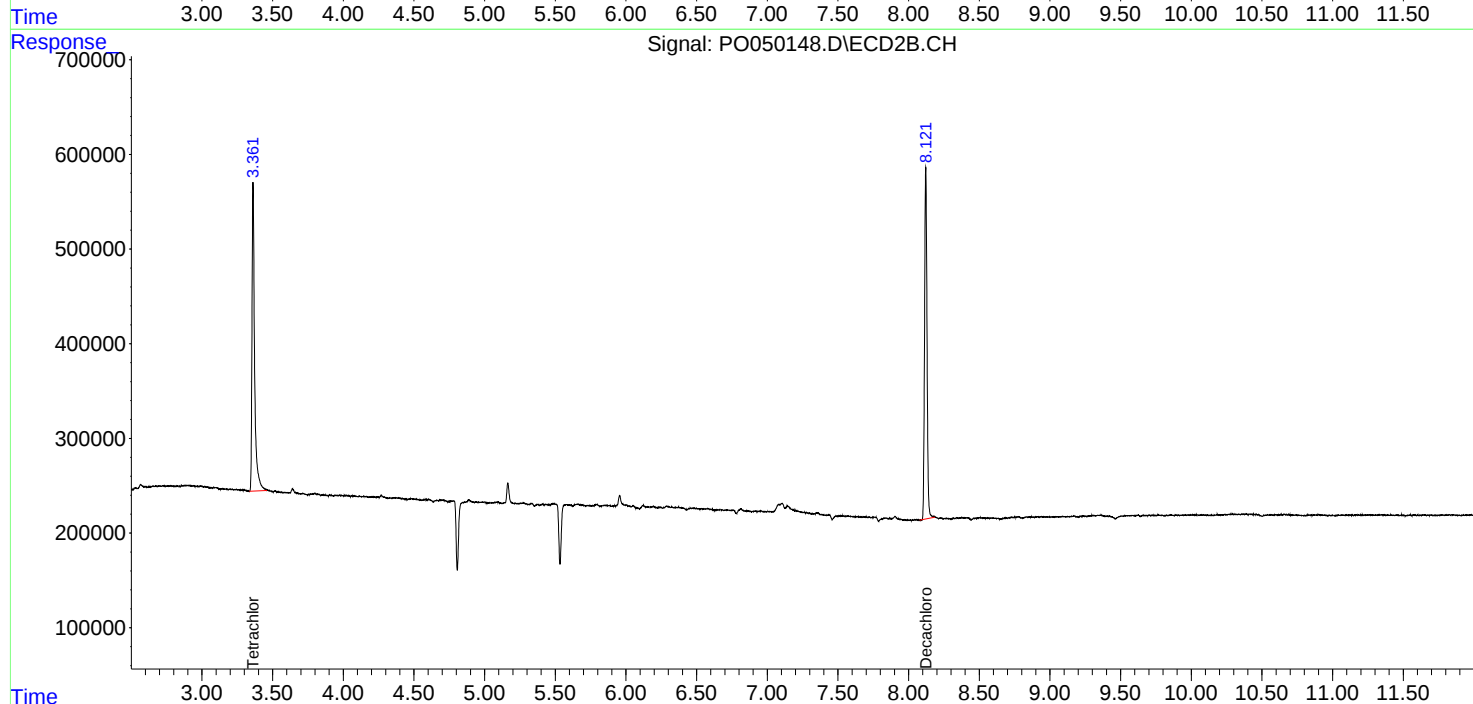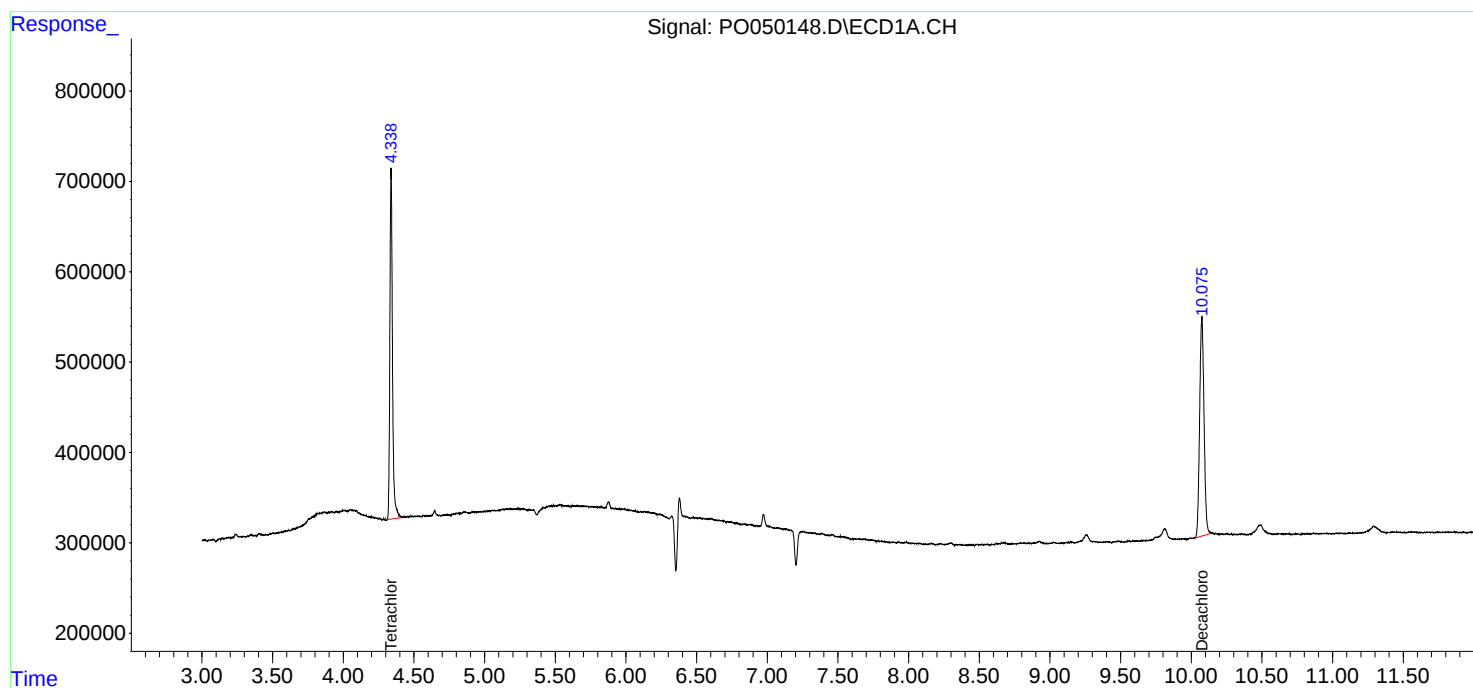


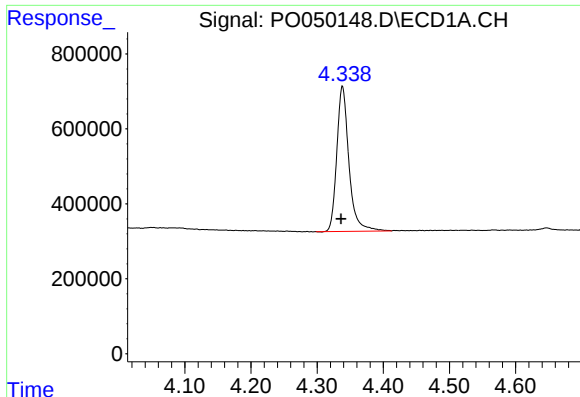

#1 Tetrachloro-m-xylene


R.T.: 4.338 min
Delta R.T.: 0.002 min
Response: 4942645
Conc: 24.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

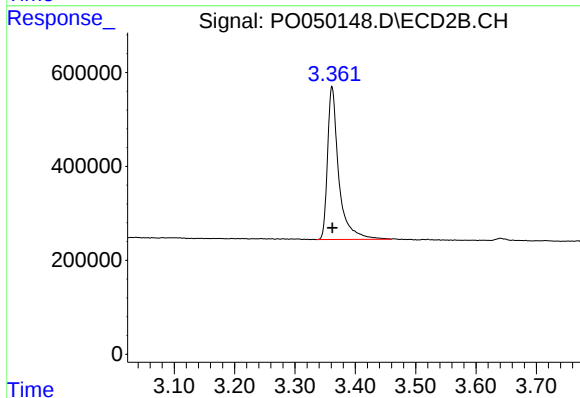


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 4205080
Conc: 21.05 ng/ml

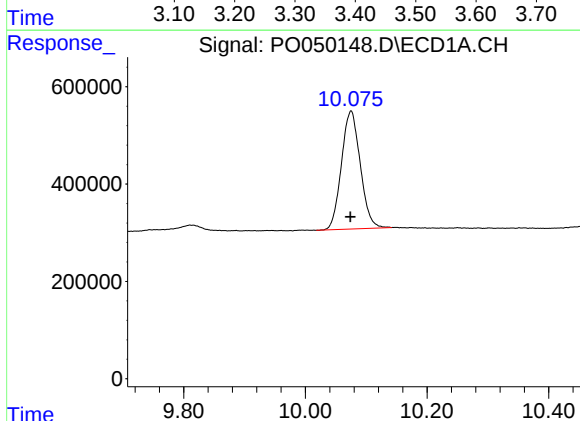

#2 Decachlorobiphenyl

R.T.: 10.075 min
Delta R.T.: 0.001 min
Response: 5208501
Conc: 21.63 ng/ml

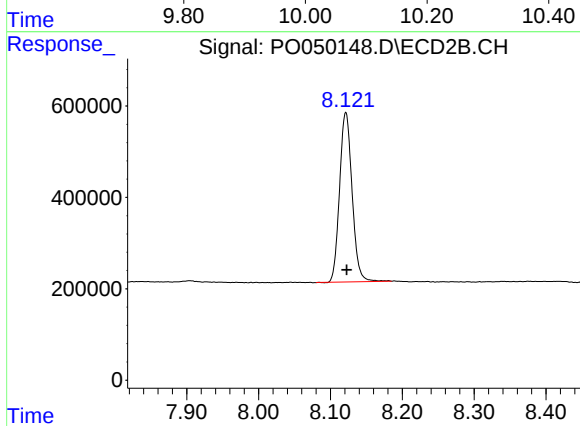

#2 Decachlorobiphenyl

R.T.: 8.121 min
Delta R.T.: -0.001 min
Response: 4489180
Conc: 23.08 ng/ml